


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112125\
Data File : BG064837.D
Acq On : 21 Nov 2025 9:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

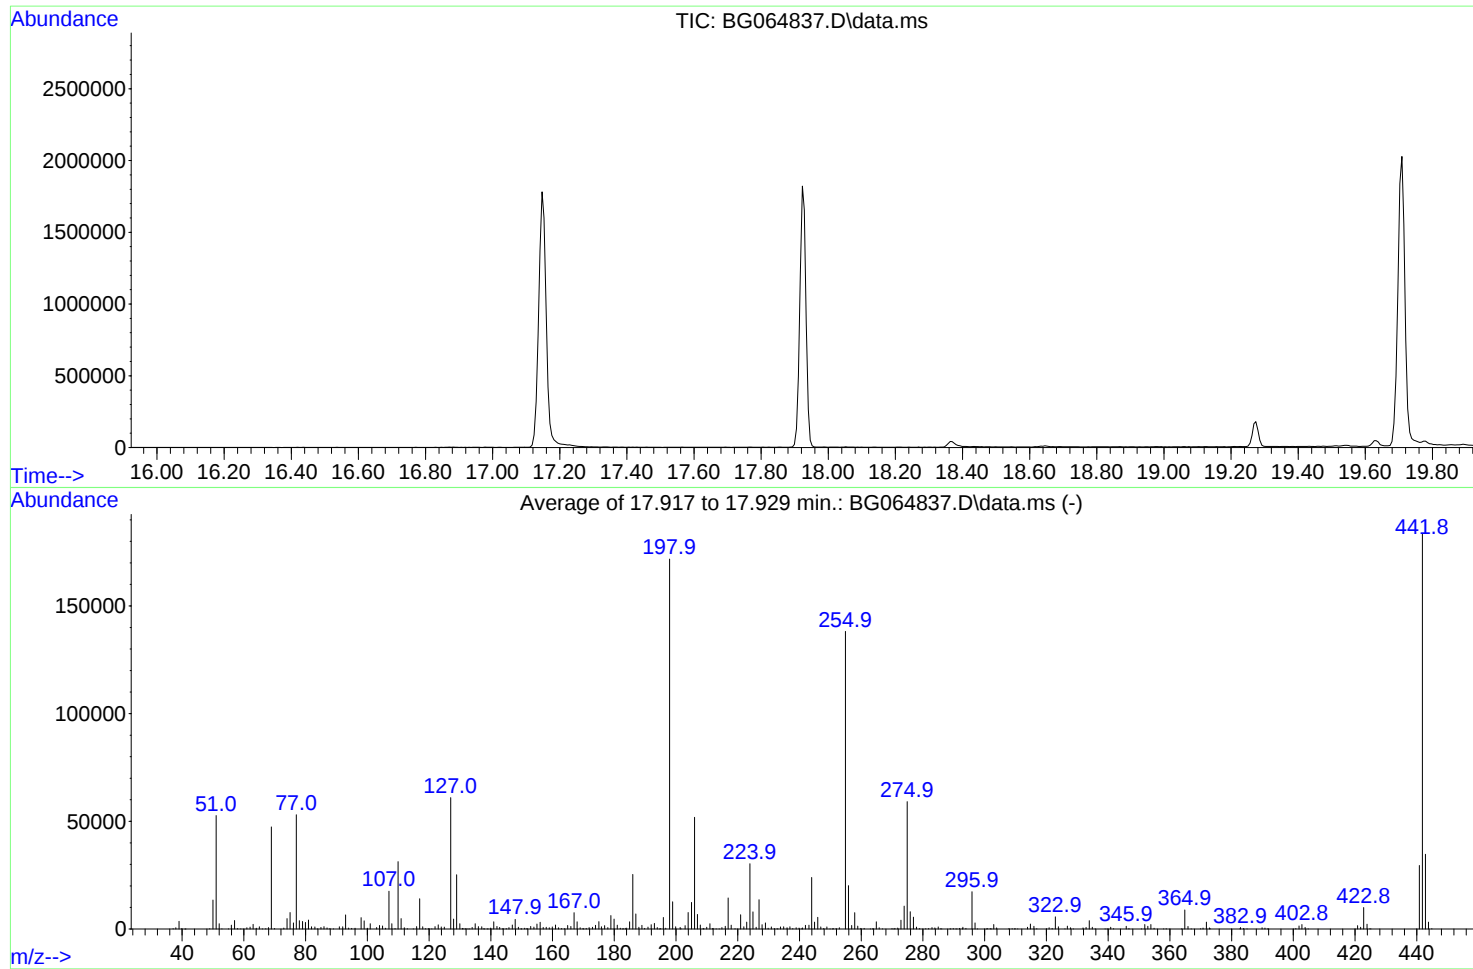

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.4	670	PASS
69	69	100	100	100.0	47407	PASS
70	69	0.00	2	0.5	257	PASS
197	198	0.00	2	0.2	403	PASS
198	198	100	100	100.0	171797	PASS
199	198	5	9	7.3	12618	PASS
365	198	1	100	5.2	8871	PASS
441	443	0.01	150	85.0	29480	PASS
442	442	100	100	100.0	183325	PASS
443	442	15	24	18.9	34693	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/21/2025	BNA_G	<u>BG064837.D</u>
Compound Name	Response	Retention Time
DDT	839562	20.937
DDD	16378	20.496
DDE	57	19.621
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16435	855997	1.92

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112125\
Data File : BG064837.D
Acq On : 21 Nov 2025 9:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 21 10:03:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

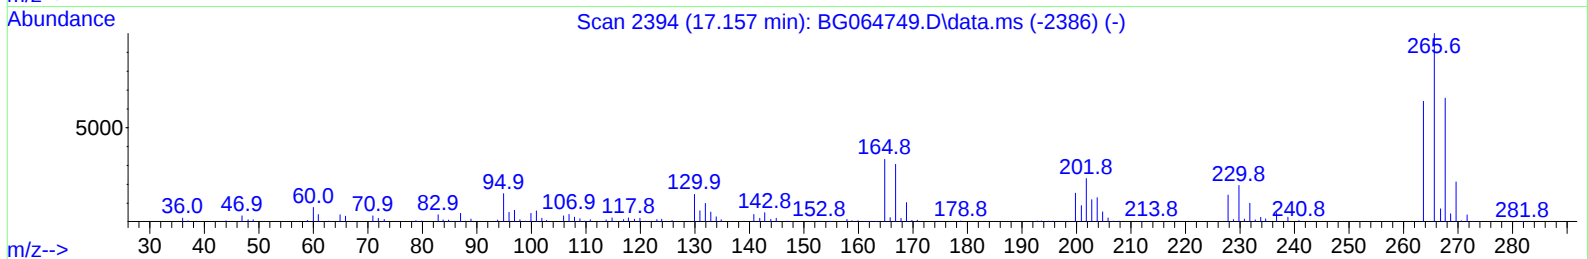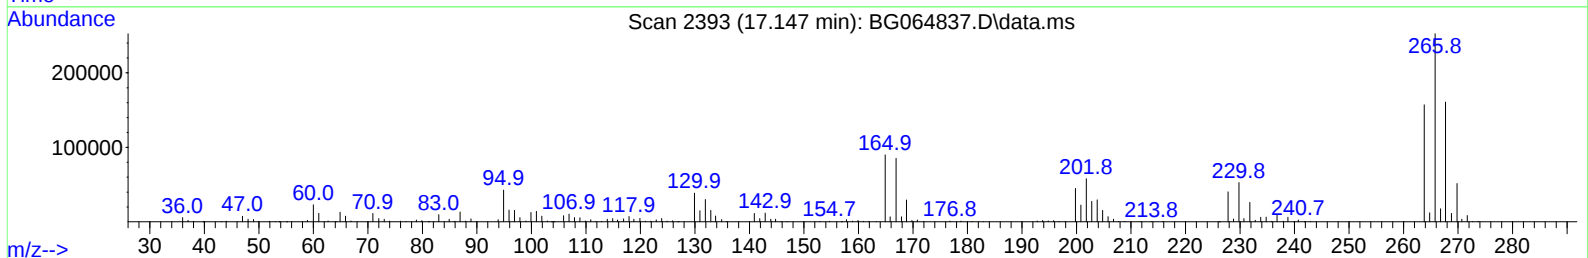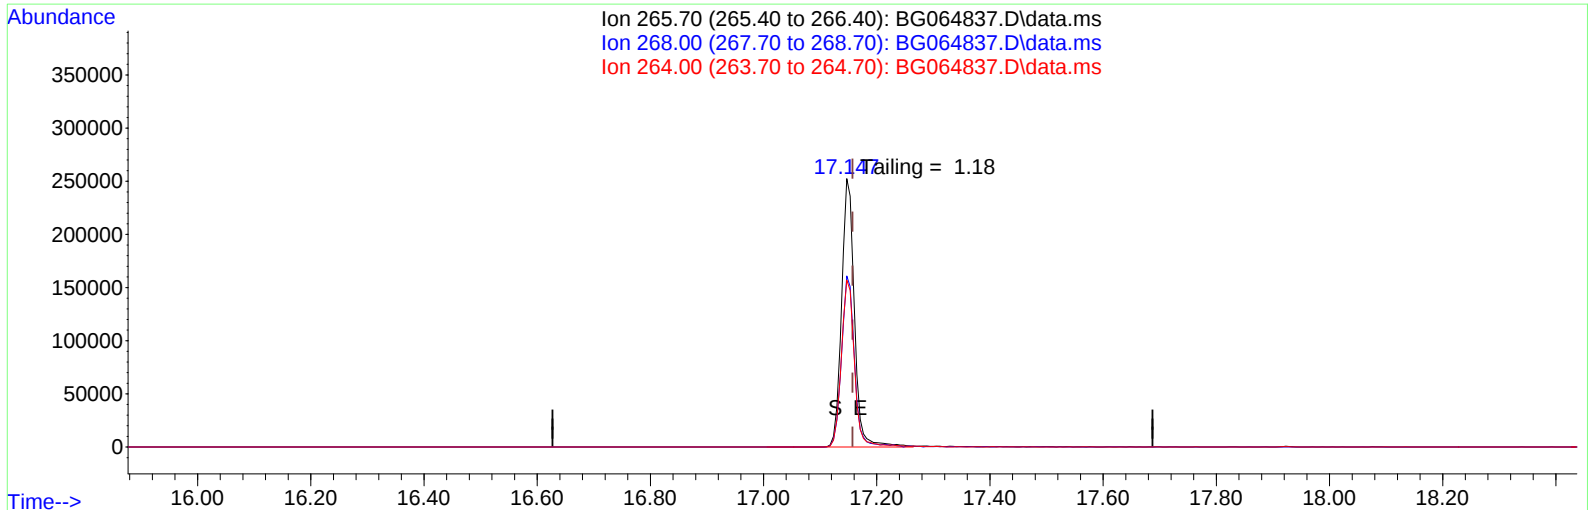

TIC: BG064837.D\data.ms

(70) Pentachlorophenol (C)

17.147min (-0.010) 696296.48 ng




response 397657

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	63.73
264.00	64.00	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112125\
Data File : BG064837.D
Acq On : 21 Nov 2025 9:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 21 10:03:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

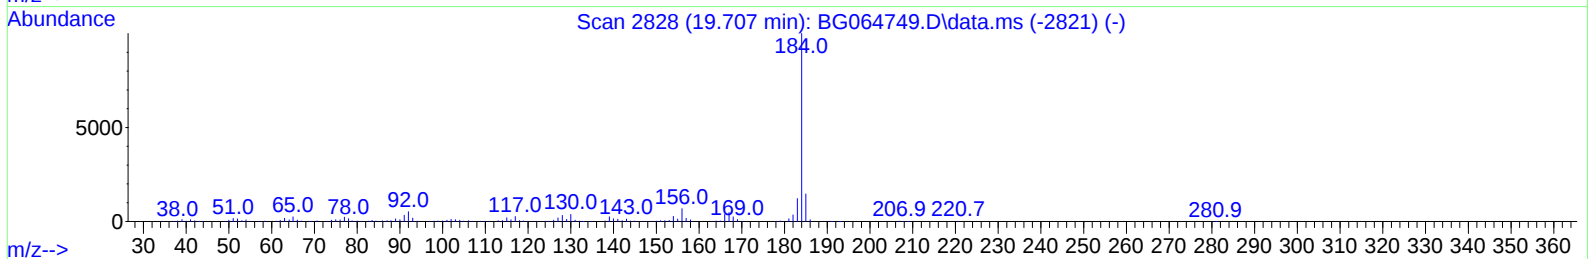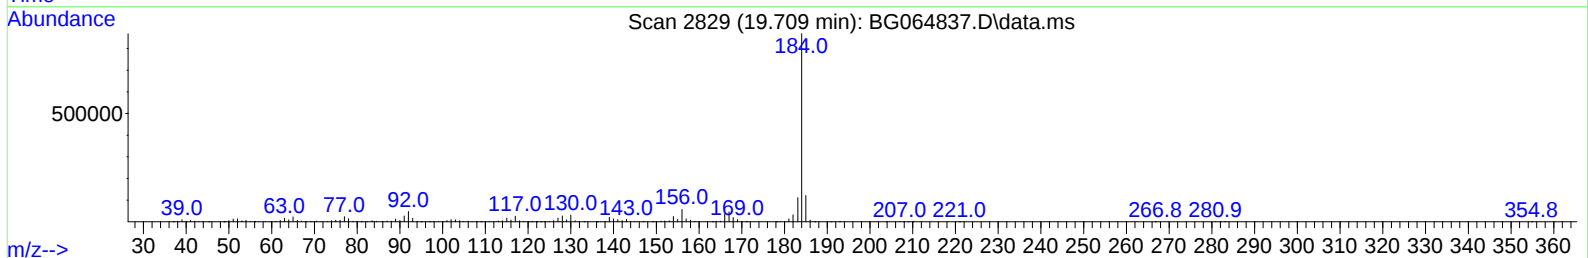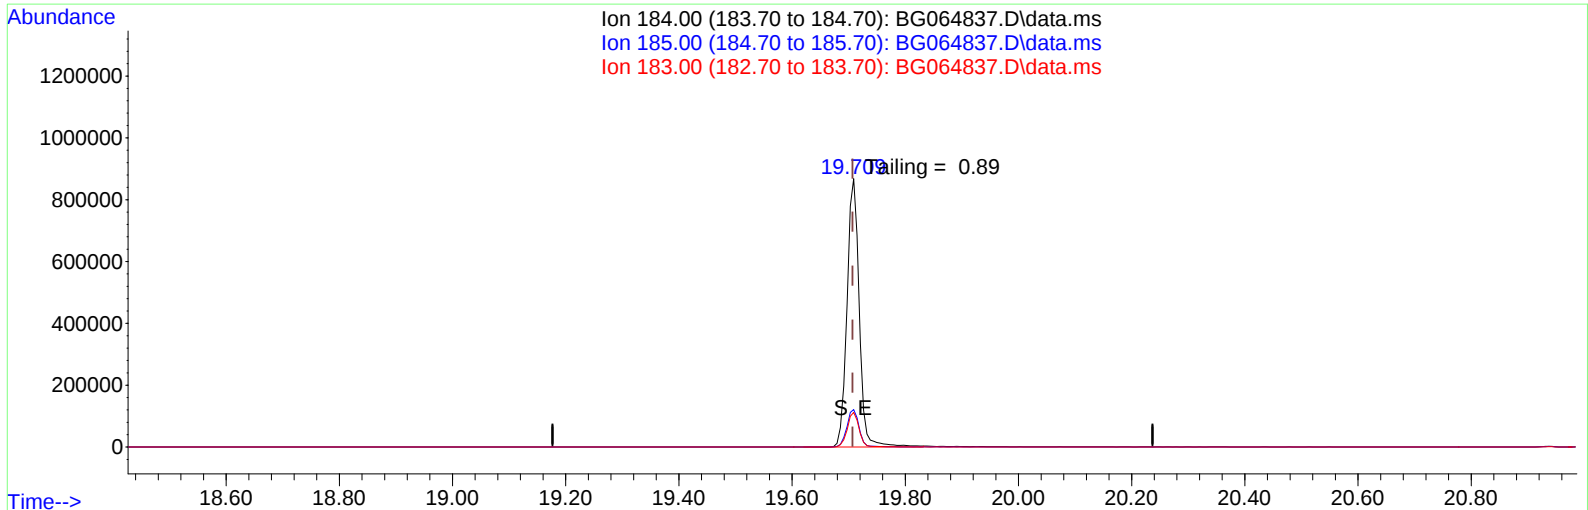

TIC: BG064837.D\data.ms

(77) Benzidine

19.709min (+ 0.002) 27434.59 ng

response 1309666

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.97
183.00	12.20	12.90
0.00	0.00	0.00