


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112219\
 Data File : BG043742.D
 Acq On : 22 Nov 2019 14:59
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG112219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 23 00:54:00 2019

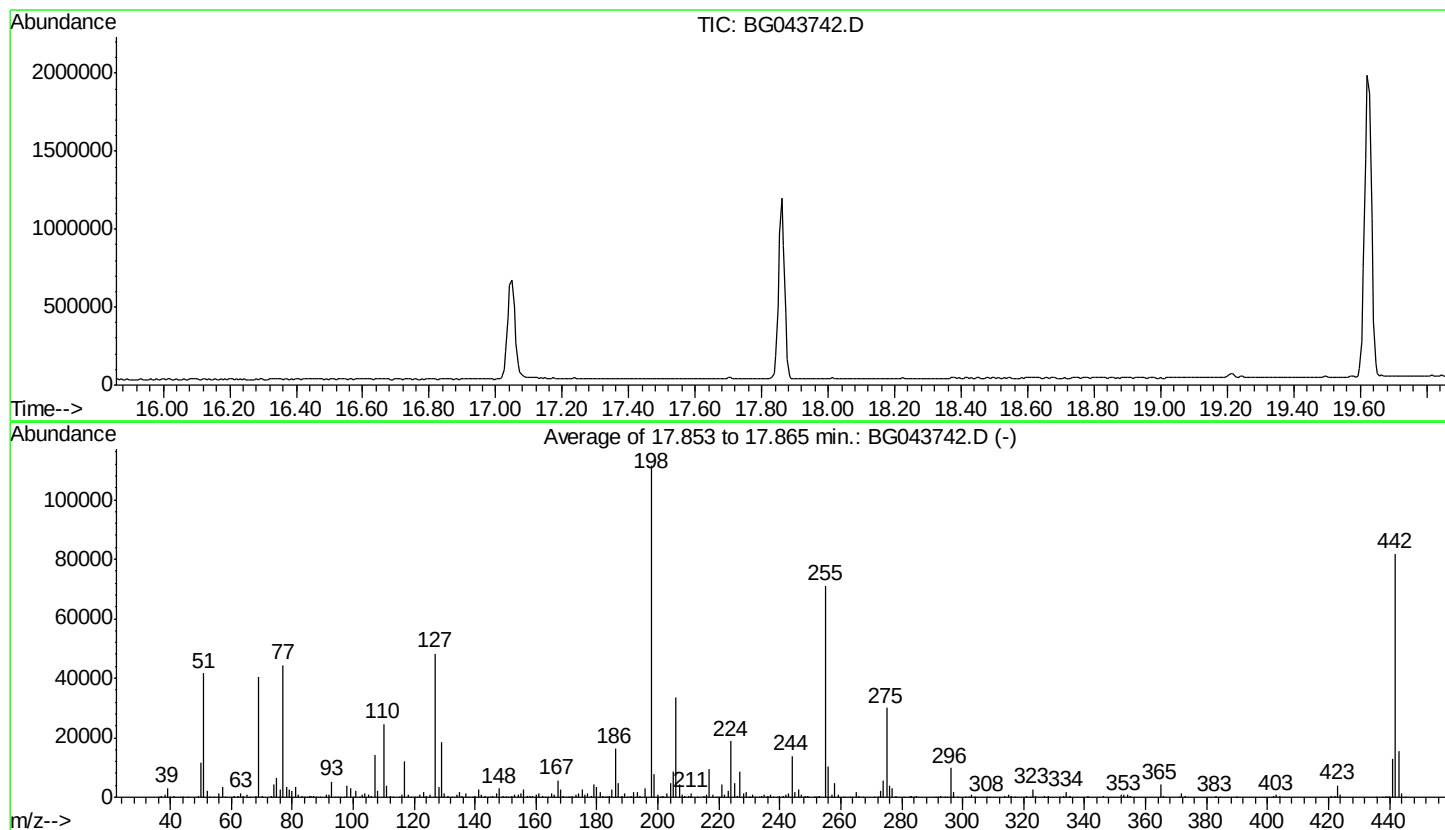

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	41533	PASS
68	69	0.00	2	1.0	389	PASS
69	198	0.00	100	36.1	40271	PASS
70	69	0.00	2	0.9	350	PASS
127	198	10	80	43.3	48209	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111421	PASS
199	198	5	9	7.1	7857	PASS
275	198	10	60	26.9	30021	PASS
365	198	1	100	3.8	4232	PASS
441	198	0.01	100	11.4	12728	PASS
442	198	50	100	73.5	81925	PASS
443	442	15	24	19.1	15611	PASS