
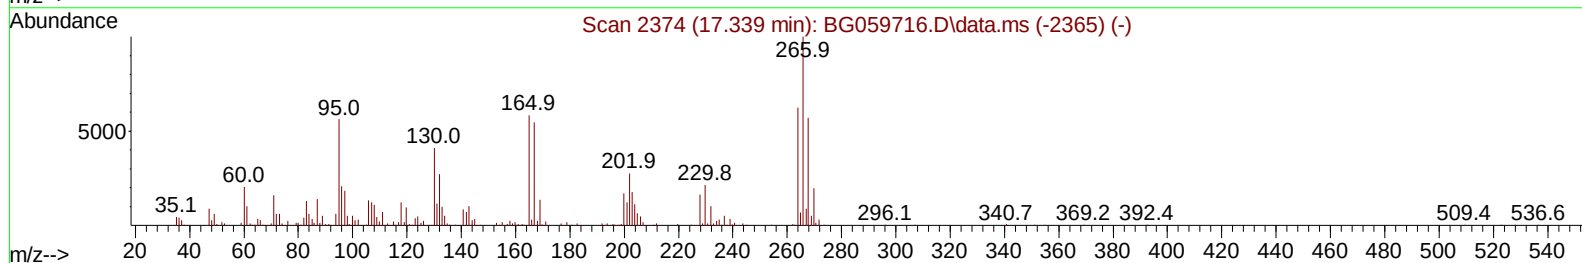
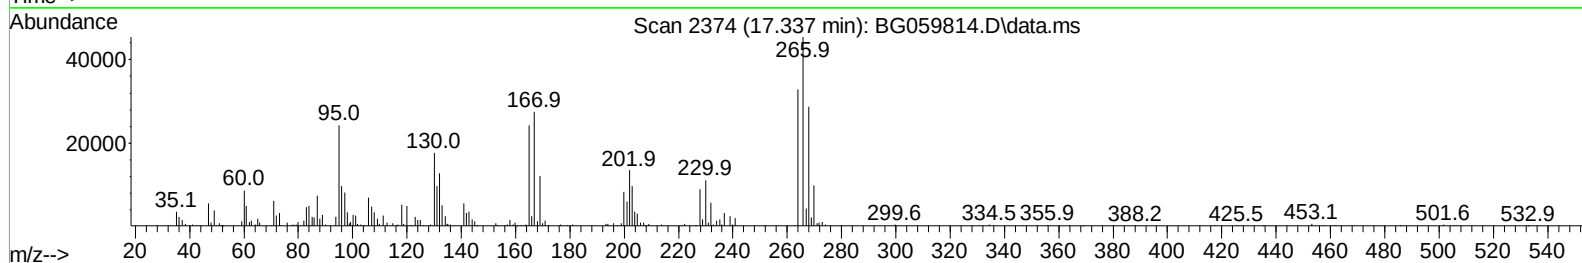


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059814.D
Acq On : 22 Nov 2023 11:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 13:32:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

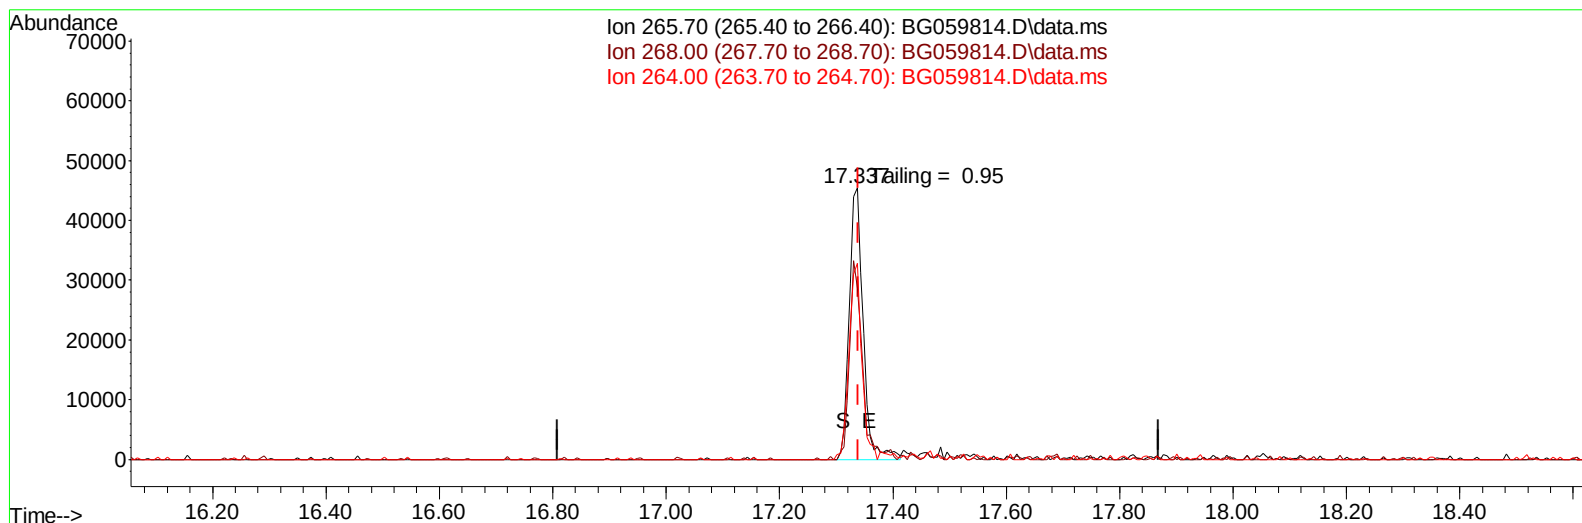

TIC: BG059814.D\data.ms

(70) Pentachlorophenol (C)




17.337min (-0.002) 175563.72 ng

response 75208

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	63.09
264.00	62.30	72.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059814.D
Acq On : 22 Nov 2023 11:11
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 13:32:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

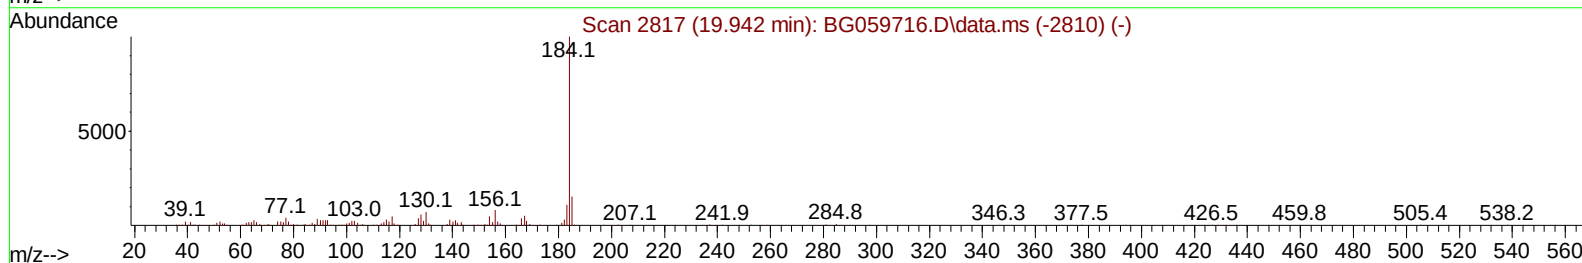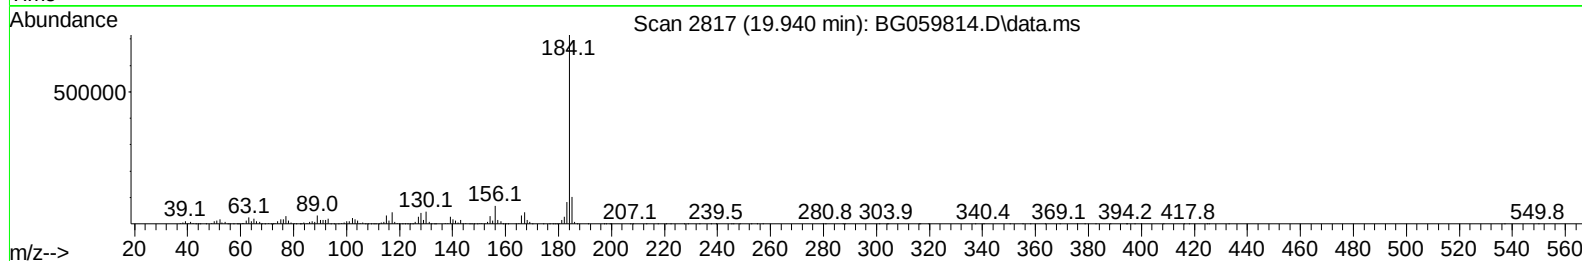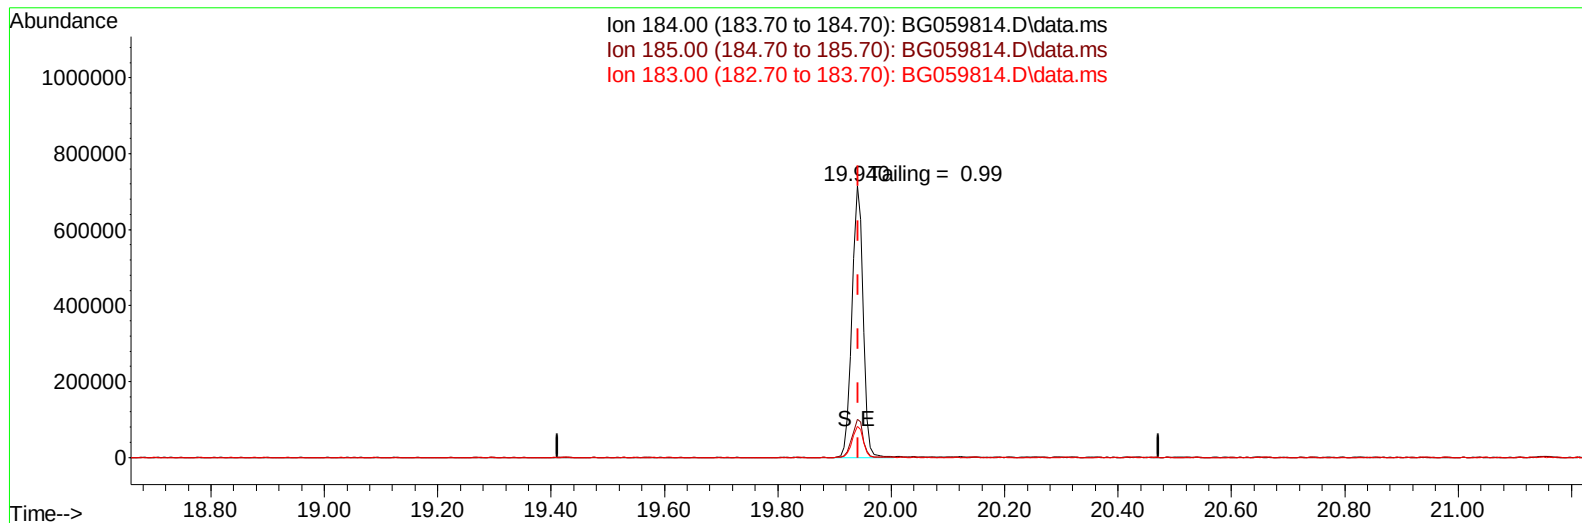

TIC: BG059814.D\data.ms

(77) Benzidine**19.940min (-0.002) 141867.82 ng****response 968305**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.11
183.00	11.00	11.42
0.00	0.00	0.00