
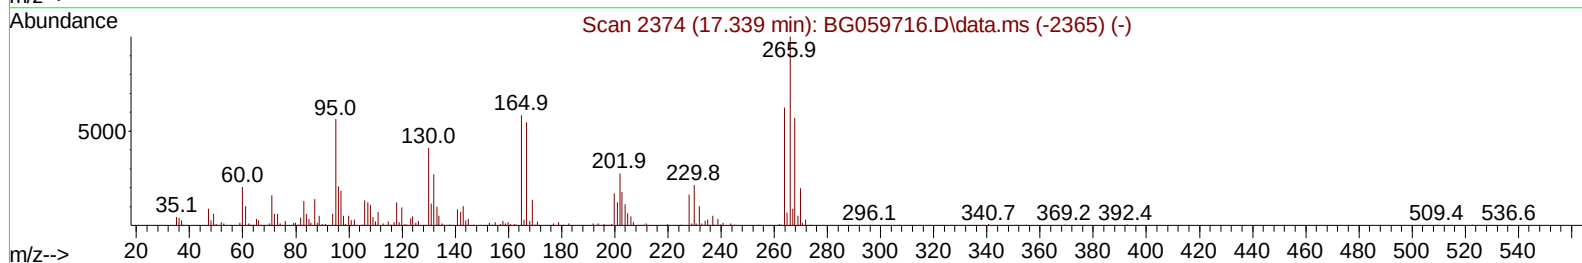
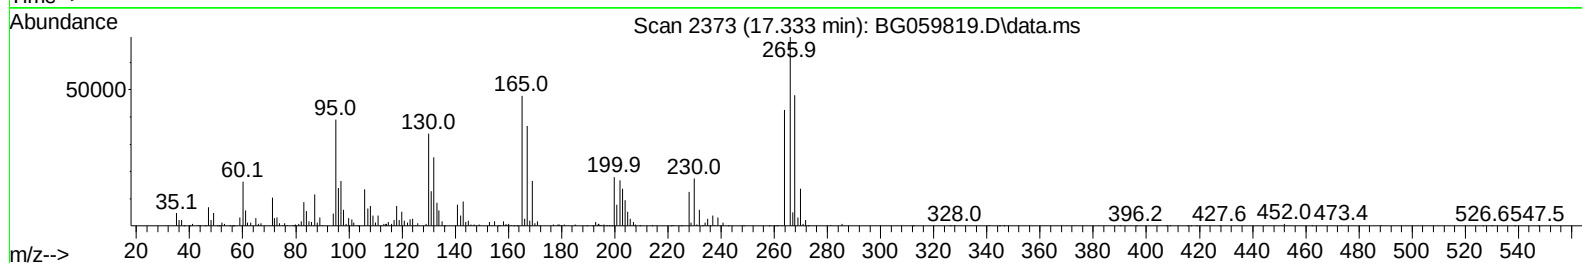


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059819.D
Acq On : 22 Nov 2023 15:38
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 16:37:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

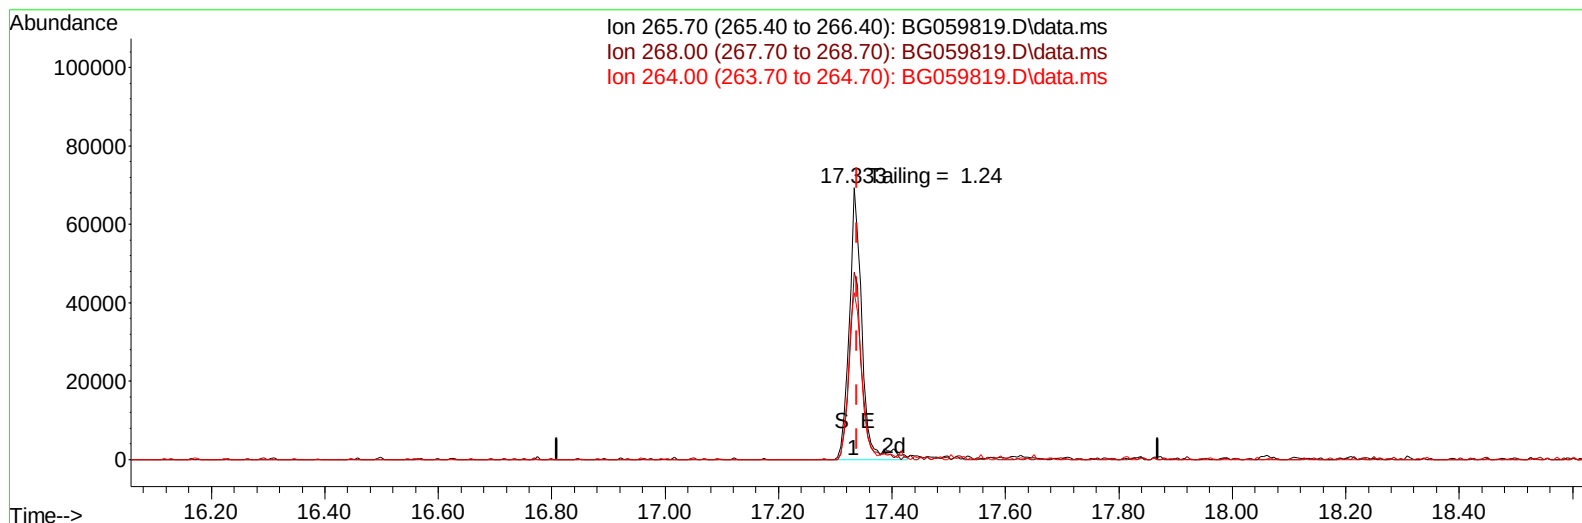

TIC: BG059819.D\data.ms

(70) Pentachlorophenol (C)




17.333min (-0.006) 60741.80 ng

response 103153

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	69.08#
264.00	62.30	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059819.D
Acq On : 22 Nov 2023 15:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 16:37:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

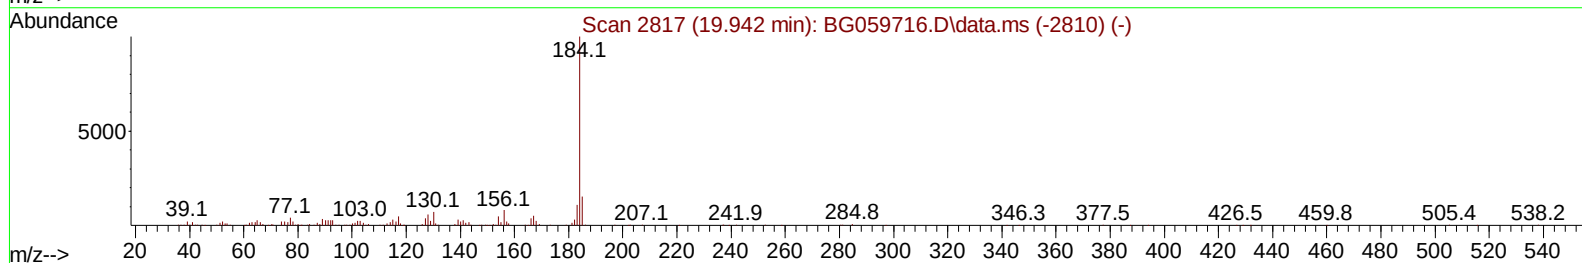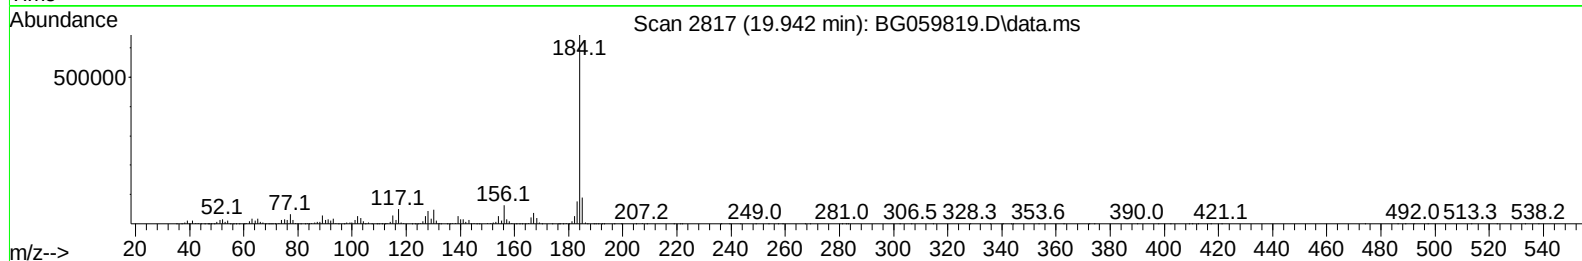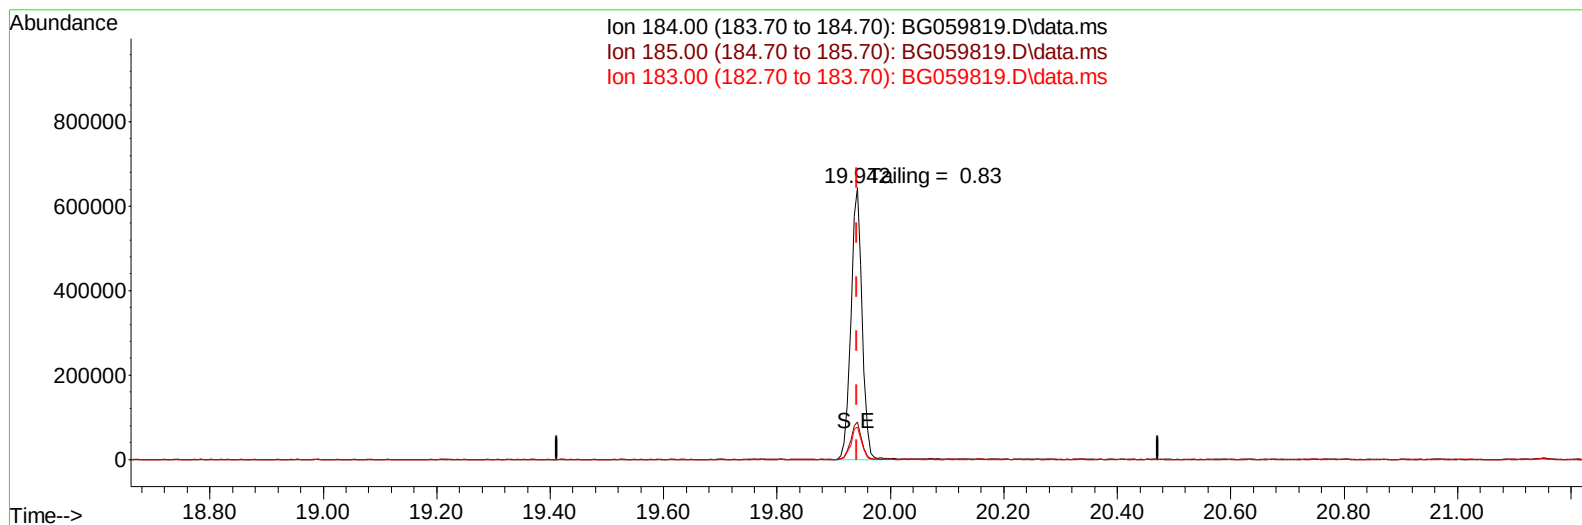

TIC: BG059819.D\data.ms

(77) Benzidine**19.942min (+ 0.000) 61148.45 ng****response 880483**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.82
183.00	11.00	11.92
0.00	0.00	0.00