

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
 Data File : BG059842.D
 Acq On : 23 Nov 2023 7:54
 Operator : MA/JU
 Sample : 05447-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP1

Quant Time: Nov 24 00:18:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 01:51:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.329	152	25003	20.000	ng	-0.01
21) Naphthalene-d8	11.179	136	114659	20.000	ng	#-0.01
39) Acenaphthene-d10	14.963	164	96067	20.000	ng	0.00
64) Phenanthrene-d10	17.707	188	235100	20.000	ng	#-0.01
76) Chrysene-d12	22.037	240	201443	20.000	ng	#-0.01
86) Perylene-d12	25.621	264	238580	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.826	112	111799	75.260	ng	0.00
7) Phenol-d6	7.454	99	164062	74.527	ng	0.00
23) Nitrobenzene-d5	9.528	82	159558	53.147	ng	-0.01
42) 2,4,6-Tribromophenol	16.449	330	113606	104.226	ng	0.00
45) 2-Fluorobiphenyl	13.582	172	386108	54.100	ng	-0.01
79) Terphenyl-d14	20.286	244	722814	52.970	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059842.D
Acq On : 23 Nov 2023 7:54
Operator : MA/JU
Sample : 05447-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP1

Quant Time: Nov 24 00:18:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration




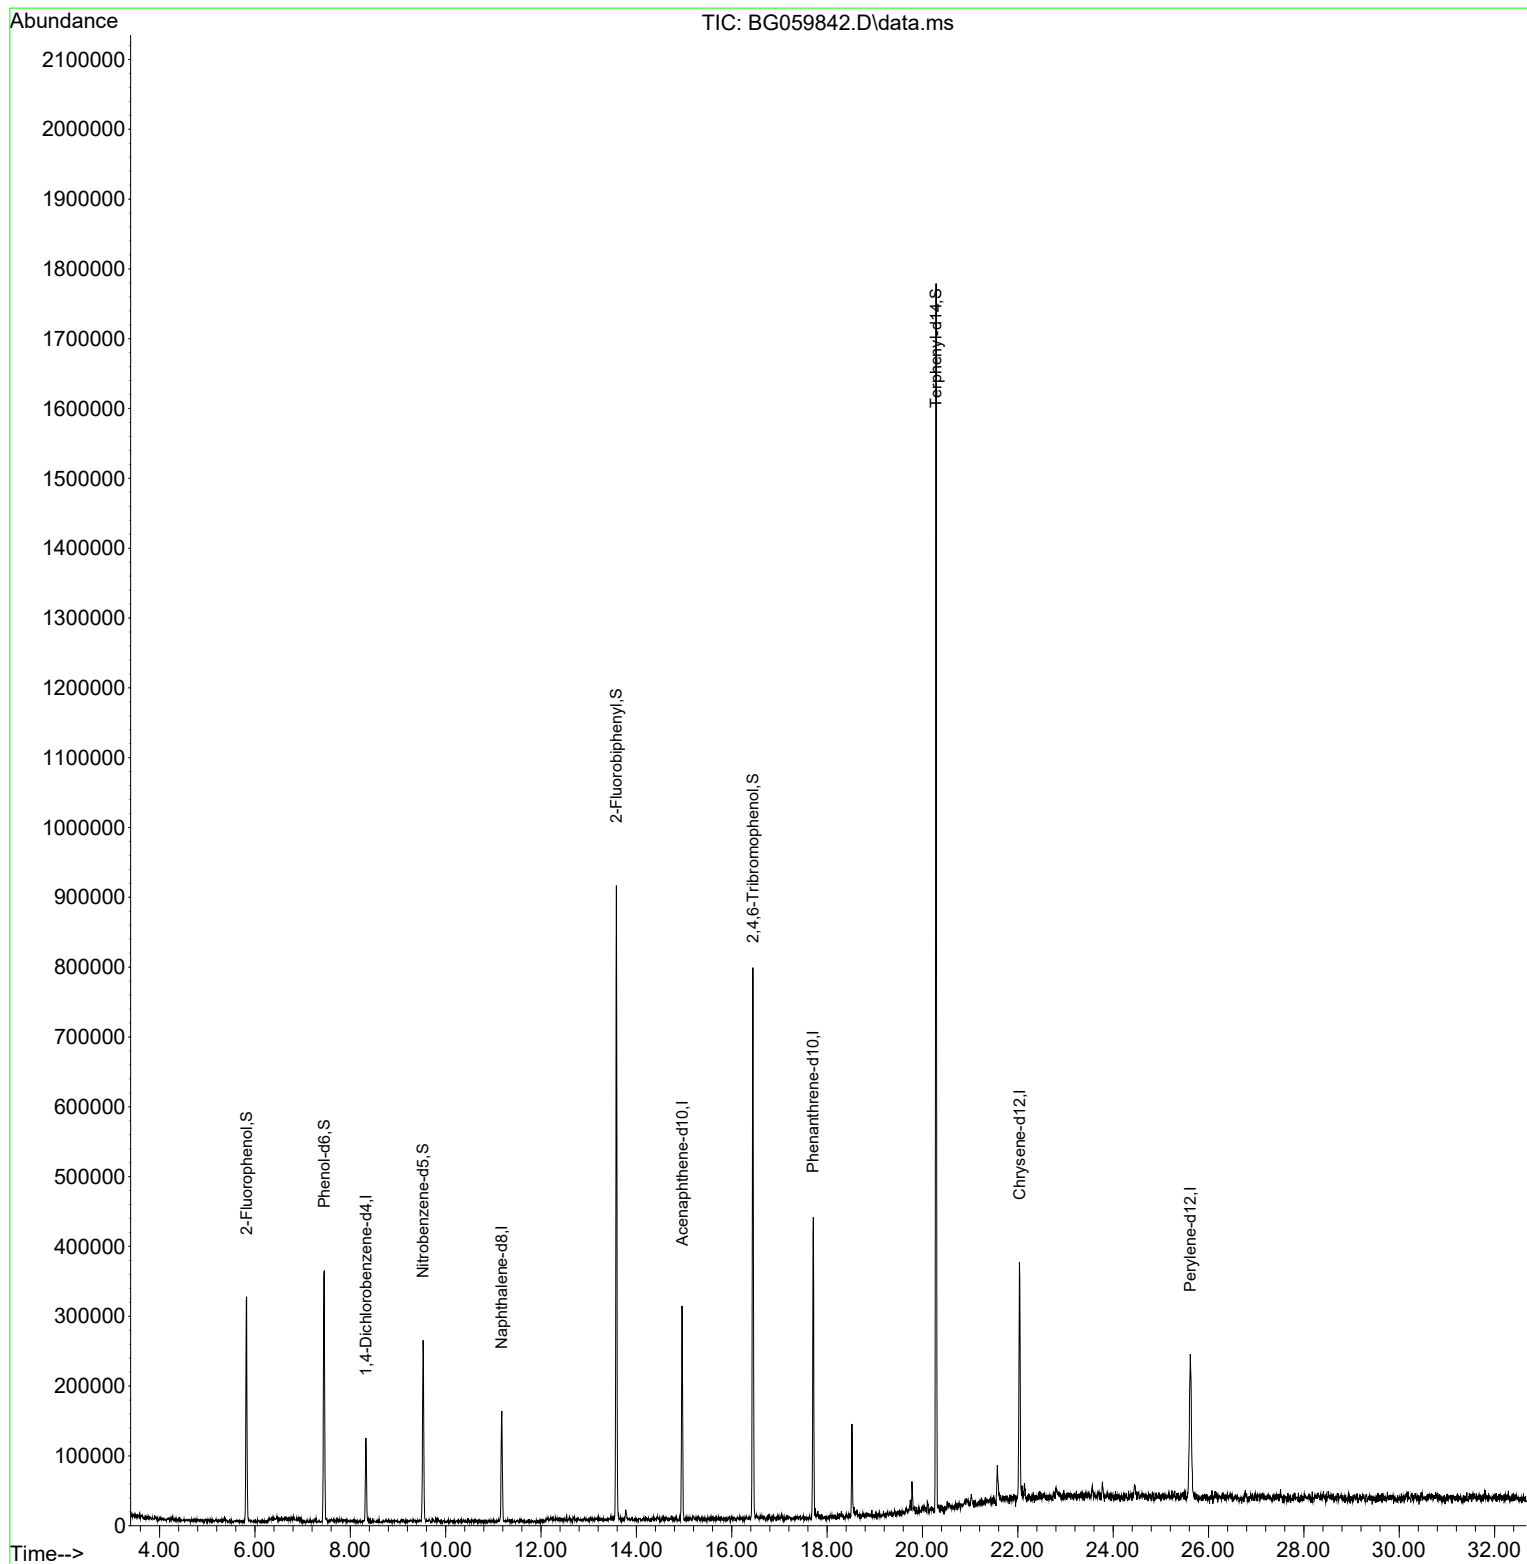




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.329 min Scan# 843
Delta R.T. -0.014 min
Lab File: BG059842.D
Acq: 23 Nov 2023 7:54




Instrument :
BNA_G
ClientSampleId :
SP1


Tgt Ion:152 Resp: 25003
Ion Ratio Lower Upper
152 100
150 129.3 122.2 183.4
115 72.6 54.2 81.4

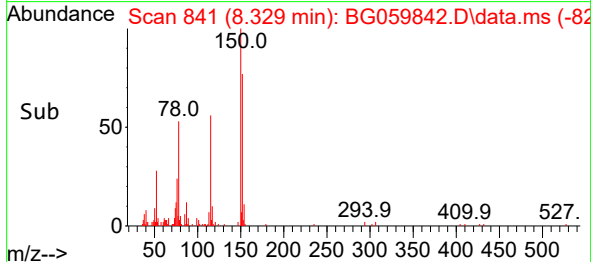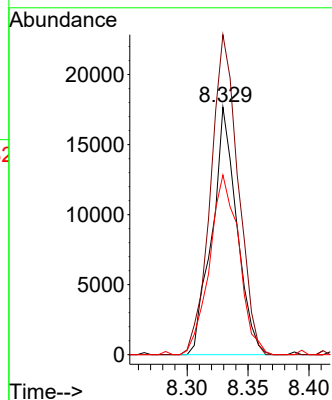

#5
2-Fluorophenol
Concen: 75.260 ng
RT: 5.826 min Scan# 415
Delta R.T. -0.002 min
Lab File: BG059842.D
Acq: 23 Nov 2023 7:54

Tgt Ion:112 Resp: 111799
Ion Ratio Lower Upper
112 100
64 50.0 49.5 74.3
63 45.9 37.4 56.2



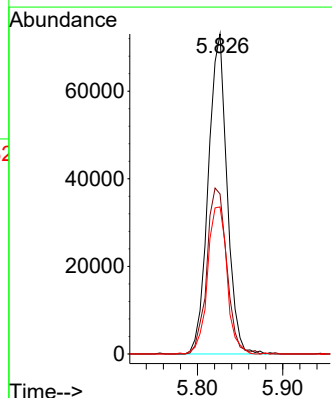
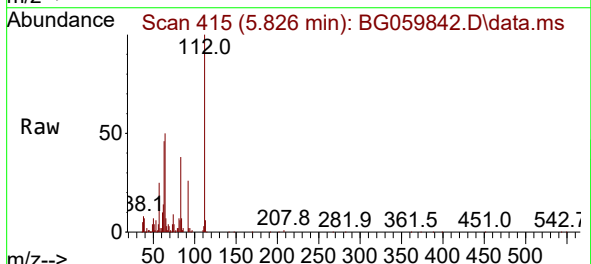




#7
Phenol-d6
Concen: 74.527 ng
RT: 7.454 min Scan# 692
Delta R.T. -0.002 min
Lab File: BG059842.D
Acq: 23 Nov 2023 7:54




Instrument :
BNA_G
ClientSampleId :
SP1


Tgt Ion: 99 Resp: 164062
Ion Ratio Lower Upper
99 100
42 19.9 14.3 21.5
71 82.4 59.3 88.9

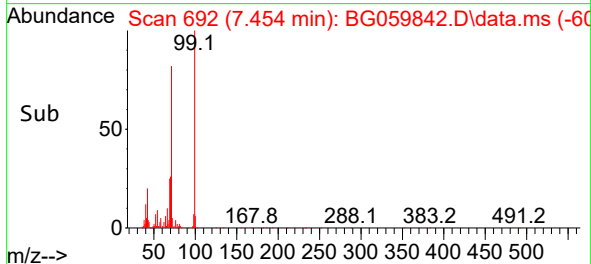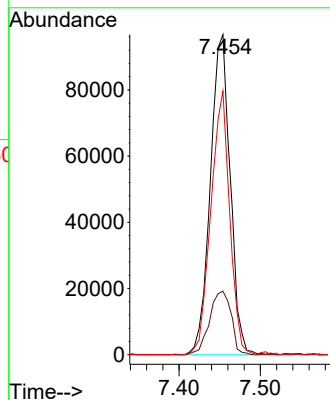

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.179 min Scan# 1326
Delta R.T. -0.014 min
Lab File: BG059842.D
Acq: 23 Nov 2023 7:54

Tgt Ion: 136 Resp: 114659
Ion Ratio Lower Upper
136 100
137 9.7 7.4 11.0
54 6.5 3.1 4.7#
68 1.6 1.8 2.8#



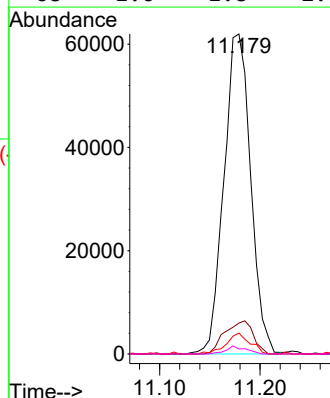
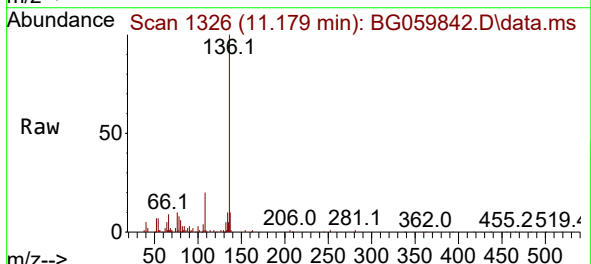




#23
Nitrobenzene-d5
Concen: 53.147 ng
RT: 9.528 min Scan# 1045
Delta R.T. -0.014 min
Lab File: BG059842.D
Acq: 23 Nov 2023 7:54




Instrument :
BNA_G
ClientSampleId :
SP1


Tgt Ion: 82 Resp: 159558
Ion Ratio Lower Upper
82 100
128 27.2 23.0 34.6
54 37.7 28.7 43.1

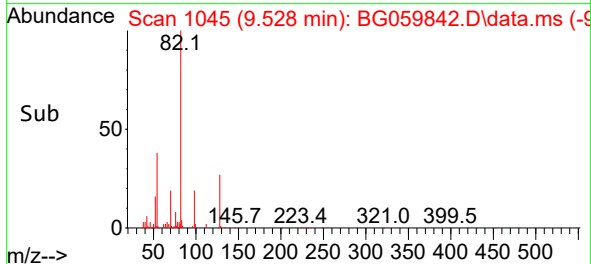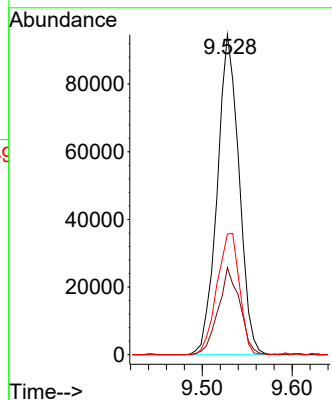

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.963 min Scan# 1970
Delta R.T. -0.008 min
Lab File: BG059842.D
Acq: 23 Nov 2023 7:54

Tgt Ion:164 Resp: 96067
Ion Ratio Lower Upper
164 100
162 101.8 73.3 109.9
160 45.4 34.1 51.1


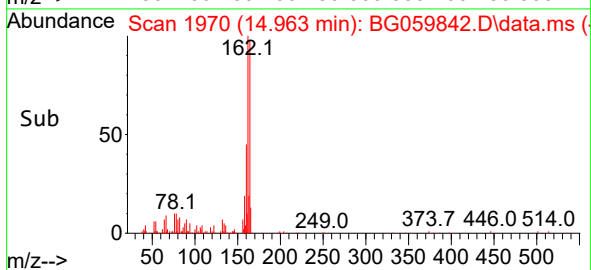
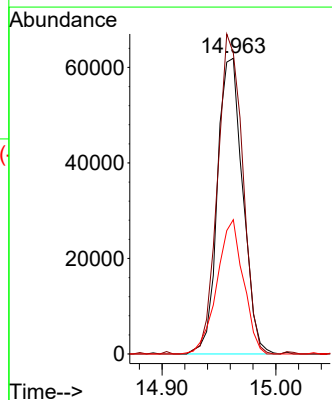
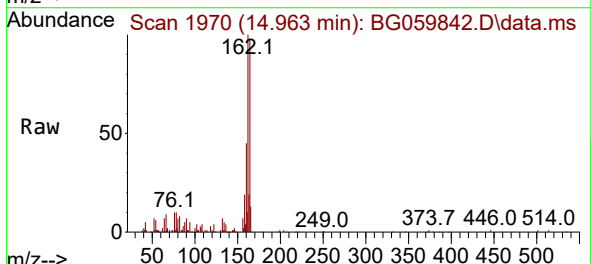




#42
2,4,6-Tribromophenol
Concen: 104.226 ng
RT: 16.449 min Scan# 21
Delta R.T. -0.008 min
Lab File: BG059842.D
Acq: 23 Nov 2023 7:54




Instrument :
BNA_G
ClientSampleId :
SP1


Tgt Ion: 330 Resp: 113606
Ion Ratio Lower Upper
330 100
332 95.7 73.3 109.9
141 61.8 52.1 78.1

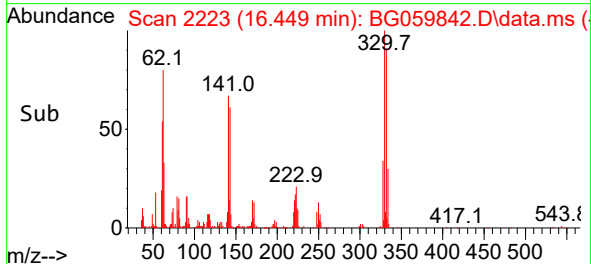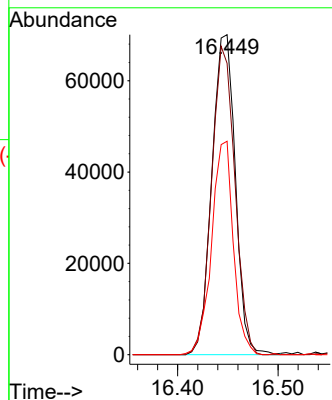

#45
2-Fluorobiphenyl
Concen: 54.100 ng
RT: 13.582 min Scan# 1735
Delta R.T. -0.014 min
Lab File: BG059842.D
Acq: 23 Nov 2023 7:54

Tgt Ion: 172 Resp: 386108
Ion Ratio Lower Upper
172 100
171 36.6 27.7 41.5
170 25.9 18.4 27.6

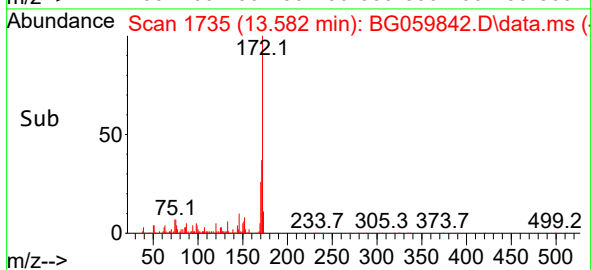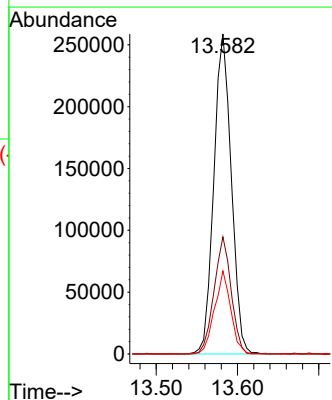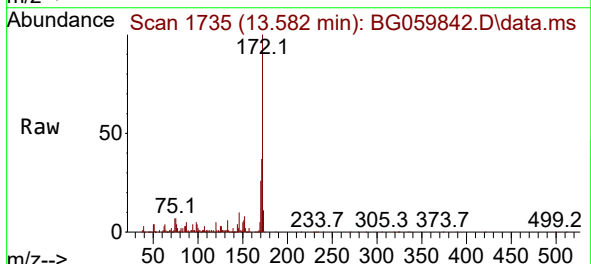



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.707 min Scan# 2439

Delta R.T. -0.014 min

Lab File: BG059842.D

Acq: 23 Nov 2023 7:54

Instrument :

BNA_G

ClientSampleId :

SP1





Tgt Ion:188 Resp: 235100

Ion Ratio Lower Upper

188 100

94 3.2 3.0 4.4

80 4.1 4.2 6.4#

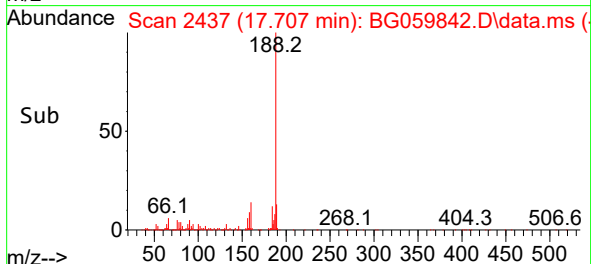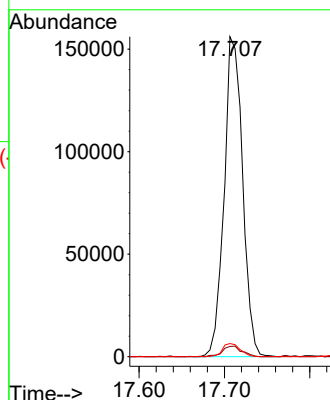

#76

Chrysene-d12

Concen: 20.000 ng

RT: 22.037 min Scan# 3174

Delta R.T. -0.014 min

Lab File: BG059842.D

Acq: 23 Nov 2023 7:54




Tgt Ion:240 Resp: 201443


Ion Ratio Lower Upper

240 100

120 2.1 2.2 3.2#

236 26.4 19.4 29.2

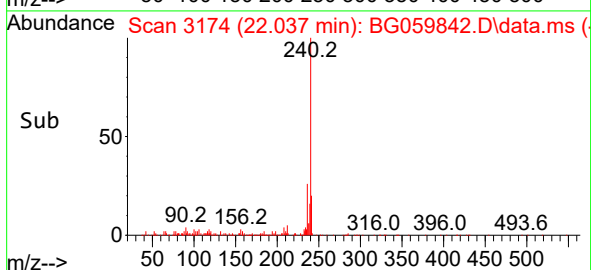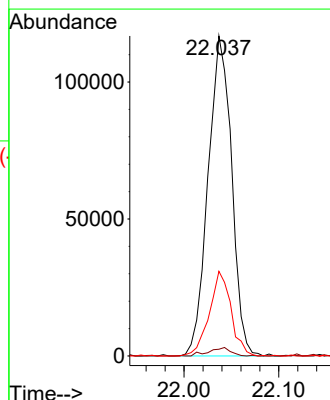



#79

Terphenyl-d14

Concen: 52.970 ng

RT: 20.286 min Scan# 21

Delta R.T. -0.008 min

Lab File: BG059842.D

Acq: 23 Nov 2023 7:54

Instrument :

BNA_G

ClientSampleId :

SP1





Tgt Ion:244 Resp: 722814

Ion Ratio Lower Upper

244 100

212 7.7 6.6 10.0

122 5.4 4.4 6.6

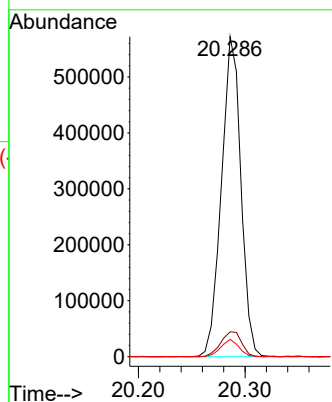

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.621 min Scan# 3784

Delta R.T. -0.014 min

Lab File: BG059842.D

Acq: 23 Nov 2023 7:54

Tgt Ion:264 Resp: 238580

Ion Ratio Lower Upper

264 100

260 21.2 18.5 27.7

265 20.4 17.0 25.6

