

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
 Data File : BG059827.D
 Acq On : 22 Nov 2023 21:04
 Operator : MA/JU
 Sample : 05449-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-SED-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG059827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.366	332	336	340	rBV	18255	26305	1.34%	0.296%
2	5.824	407	414	421	rBV	290007	465755	23.78%	5.233%
3	7.451	683	691	698	rBV	305567	537429	27.44%	6.038%
4	8.333	834	841	847	rBV4	95227	169251	8.64%	1.901%
5	9.531	1036	1045	1051	rBV	199997	371148	18.95%	4.170%
6	11.176	1319	1325	1337	rVB2	130918	235796	12.04%	2.649%
7	13.580	1728	1734	1743	rVB	765992	1178776	60.19%	13.243%
8	13.779	1763	1768	1777	rVB2	12103	32894	1.68%	0.370%
9	14.960	1961	1969	1976	rVB2	295708	486614	24.85%	5.467%
10	16.447	2214	2222	2229	rBV2	796885	1215810	62.08%	13.659%
11	17.710	2431	2437	2444	rBV	399325	634600	32.40%	7.130%
12	18.527	2572	2576	2581	rBV6	40974	57354	2.93%	0.644%
13	19.790	2787	2791	2794	rBV6	26781	31277	1.60%	0.351%
14	20.289	2869	2876	2881	rVV	1505222	1958519	100.00%	22.003%
15	21.570	3092	3094	3099	rBV6	23066	43300	2.21%	0.486%
16	22.040	3168	3174	3180	rVB3	355367	608100	31.05%	6.832%
17	22.252	3208	3210	3213	rVB3	23851	24458	1.25%	0.275%
18	22.346	3219	3226	3227	rBV7	22628	38383	1.96%	0.431%
19	23.591	3437	3438	3444	rVB6	33299	37994	1.94%	0.427%
20	24.461	3585	3586	3592	rBV5	16485	25282	1.29%	0.284%
21	24.972	3672	3673	3678	rBV5	15907	19856	1.01%	0.223%
22	25.624	3772	3784	3794	rBV	215449	655545	33.47%	7.365%
23	26.400	3911	3916	3917	rBV5	14244	24003	1.23%	0.270%
24	29.784	4489	4492	4495	rBV4	14118	22509	1.15%	0.253%




Sum of corrected areas: 8900958

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059827.D
Acq On : 22 Nov 2023 21:04
Operator : MA/JU
Sample : 05449-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-SED-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

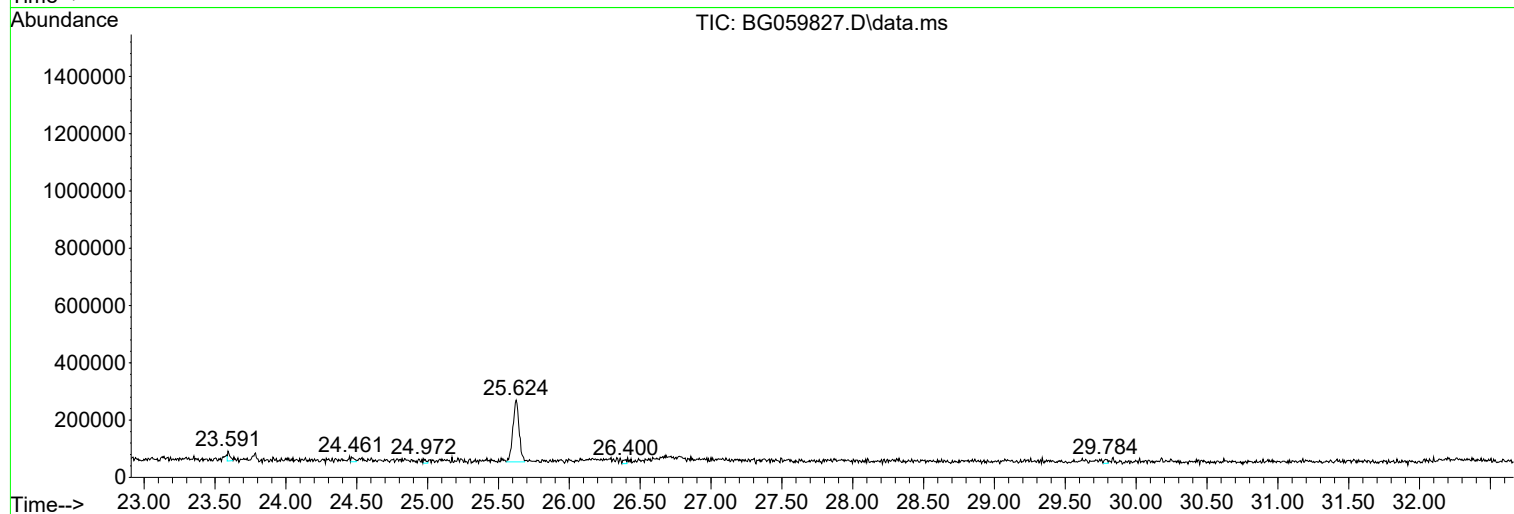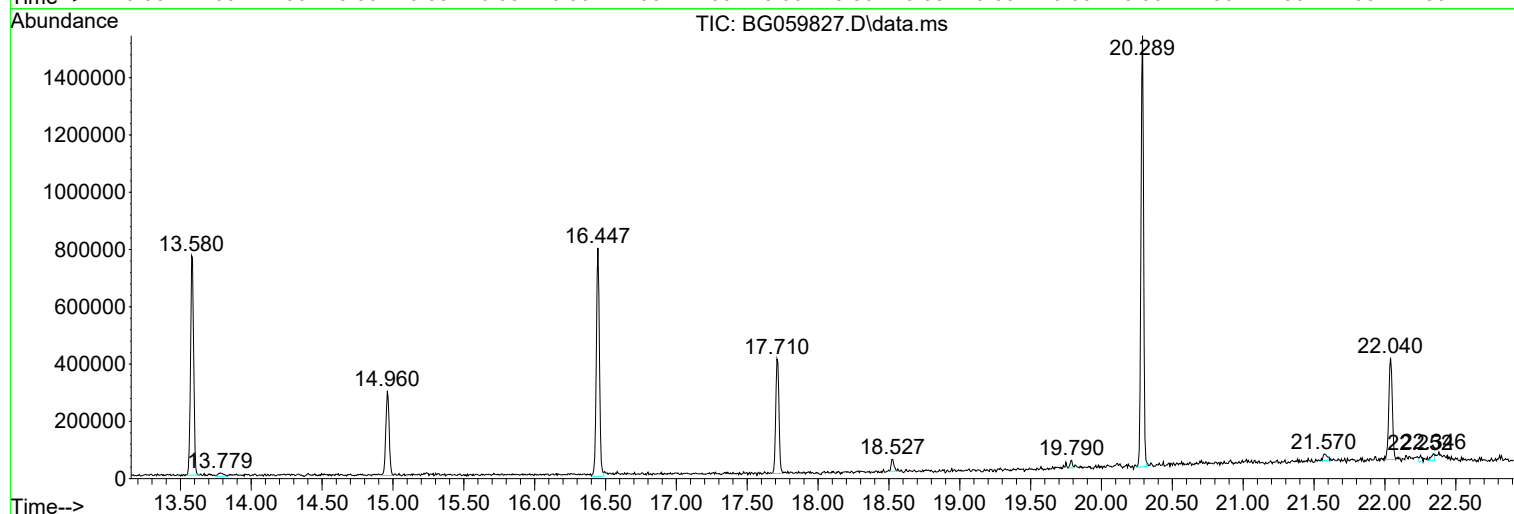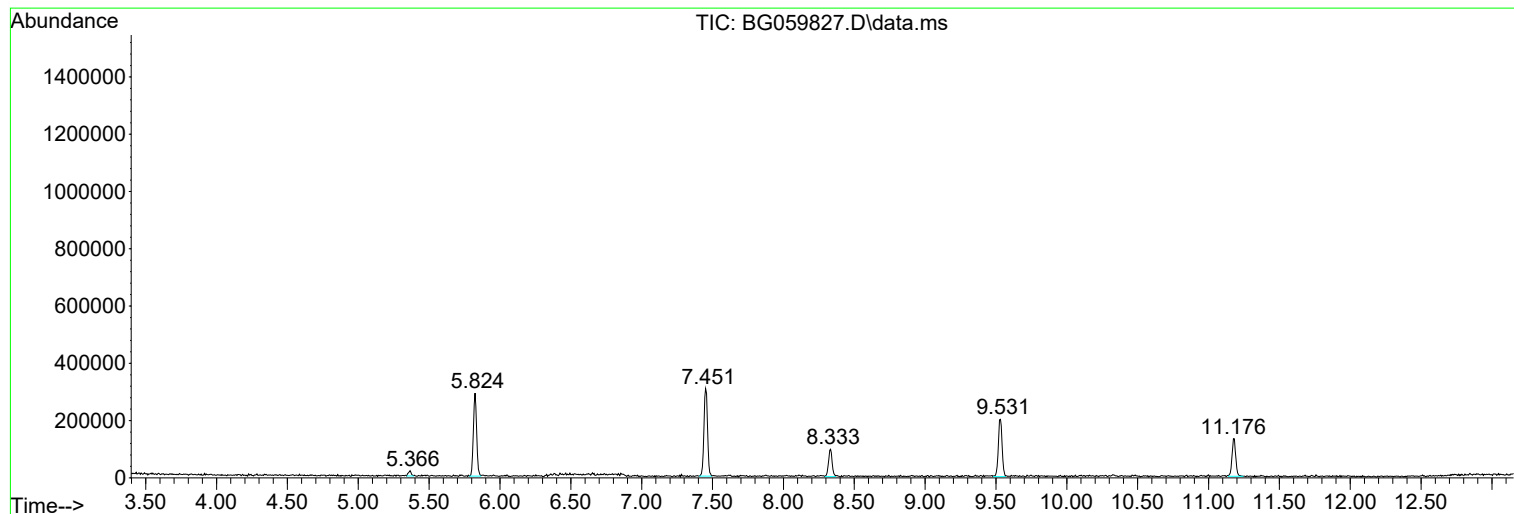

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059827.D
Acq On : 22 Nov 2023 21:04
Operator : MA/JU
Sample : 05449-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-SED-02










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.366 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.366	3.11 ng	26305	1,4-Dichlorobenzene-d4	8.327

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanol, 2,4-dimethyl-	116	C7H16O	000625-06-9	47
2		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	28
3		3-Octanol	130	C8H18O	000589-98-0	23
4		1-Propanol, 3,3'-oxybis-	134	C6H14O3	002396-61-4	12
5		Pentan-2-ol, 4-allyloxy-2-methyl-	158	C9H18O2	102840-52-8	12

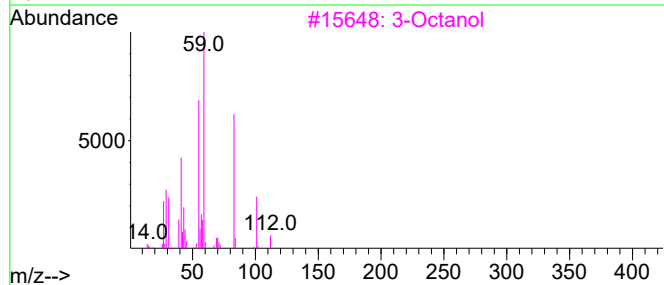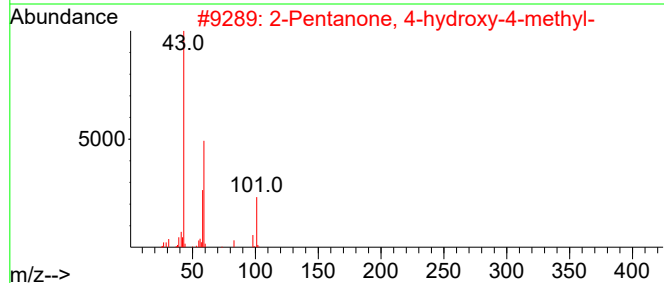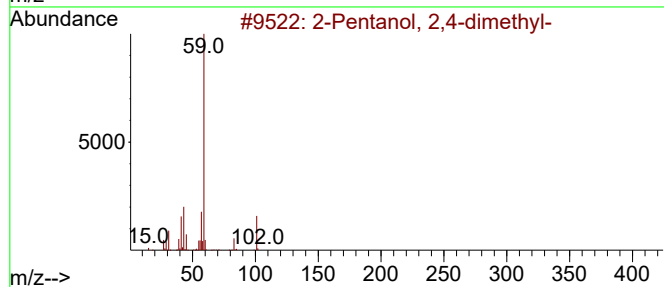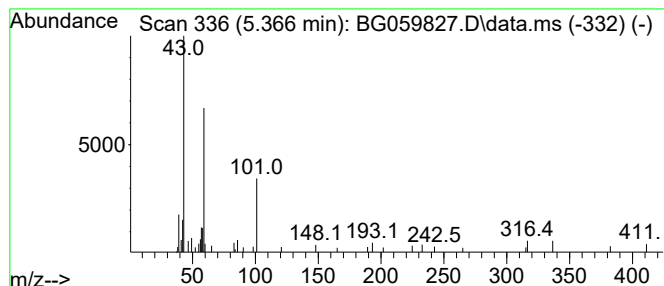

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059827.D
Acq On : 22 Nov 2023 21:04
Operator : MA/JU
Sample : 05449-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-SED-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.366	5.366	3.1	ng	26305	1	8.327	169251	20.0