
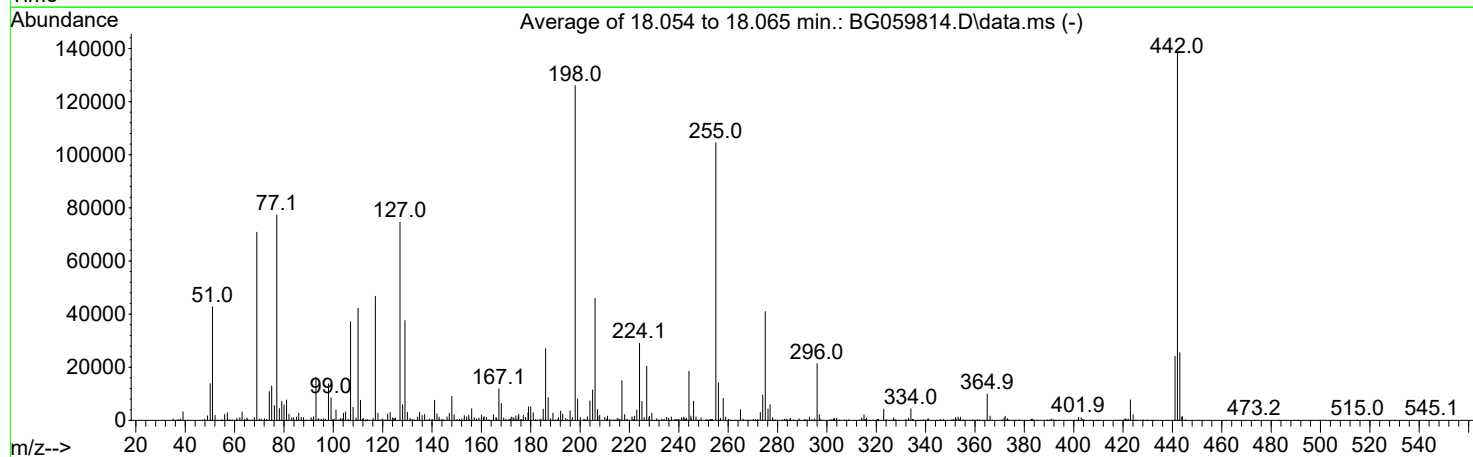


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059814.D
Acq On : 22 Nov 2023 11:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 17 01:51:38 2023

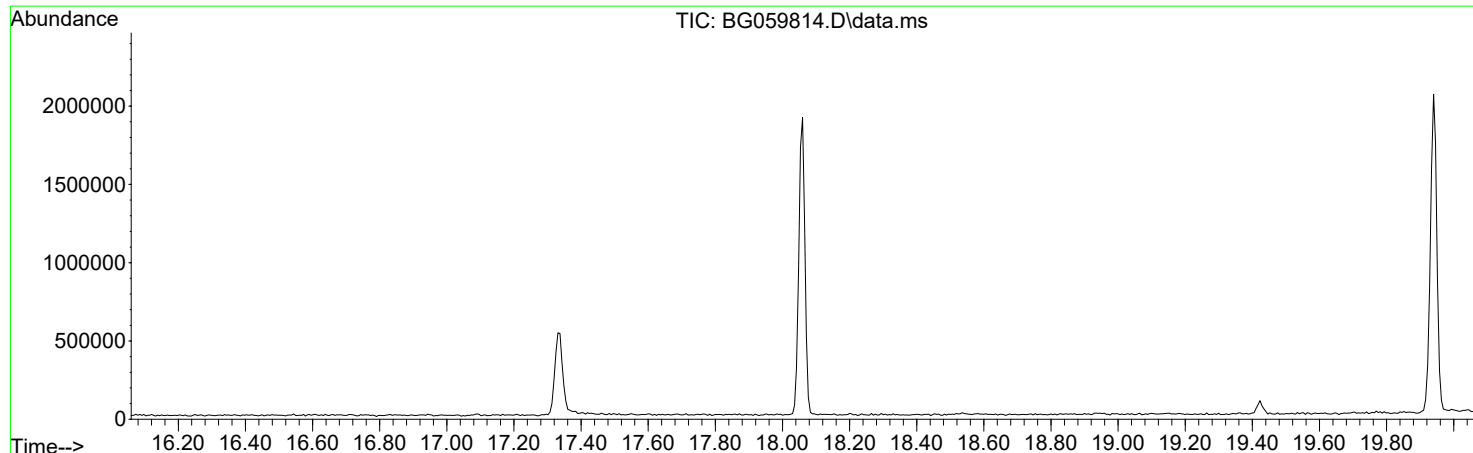

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	42773	PASS
68	69	0.00	2	1.5	1046	PASS
69	198	0.00	100	56.2	70815	PASS
70	69	0.00	2	0.8	532	PASS
127	198	10	80	59.2	74603	PASS
197	198	0.00	2	0.9	1187	PASS
198	198	100	100	100.0	126045	PASS
199	198	5	9	6.3	7996	PASS
275	198	10	60	32.5	40963	PASS
365	198	1	100	7.9	9964	PASS
441	198	0.01	100	19.2	24152	PASS
442	442	50	100	100.0	138469	PASS
443	442	15	24	18.4	25507	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/22/2023	BNA_G	BG059814.D
Compound Name	Response	Retention Time
DDT	420161	21.15
DDD	8776	20.739
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8776	428937	2.05

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059814.D
Acq On : 22 Nov 2023 11:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 13:32:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

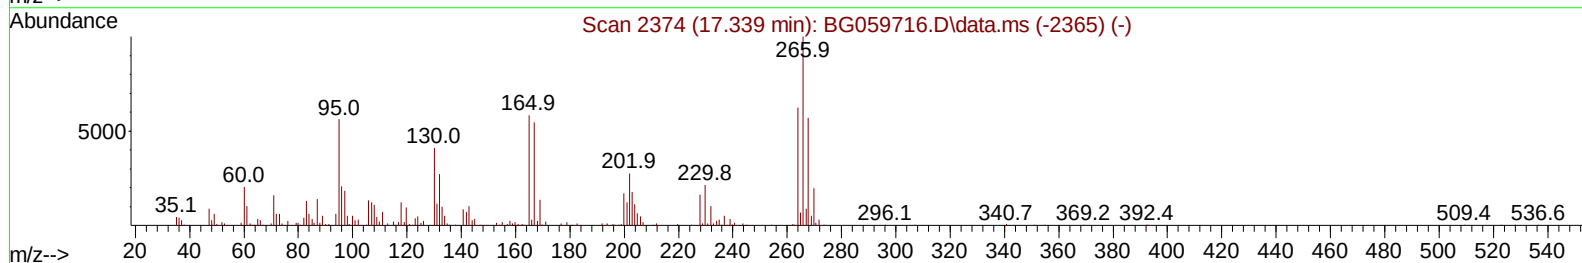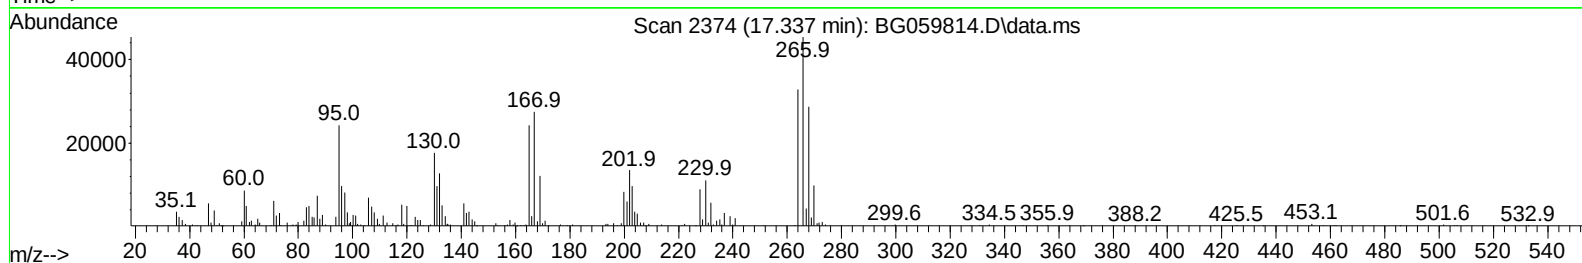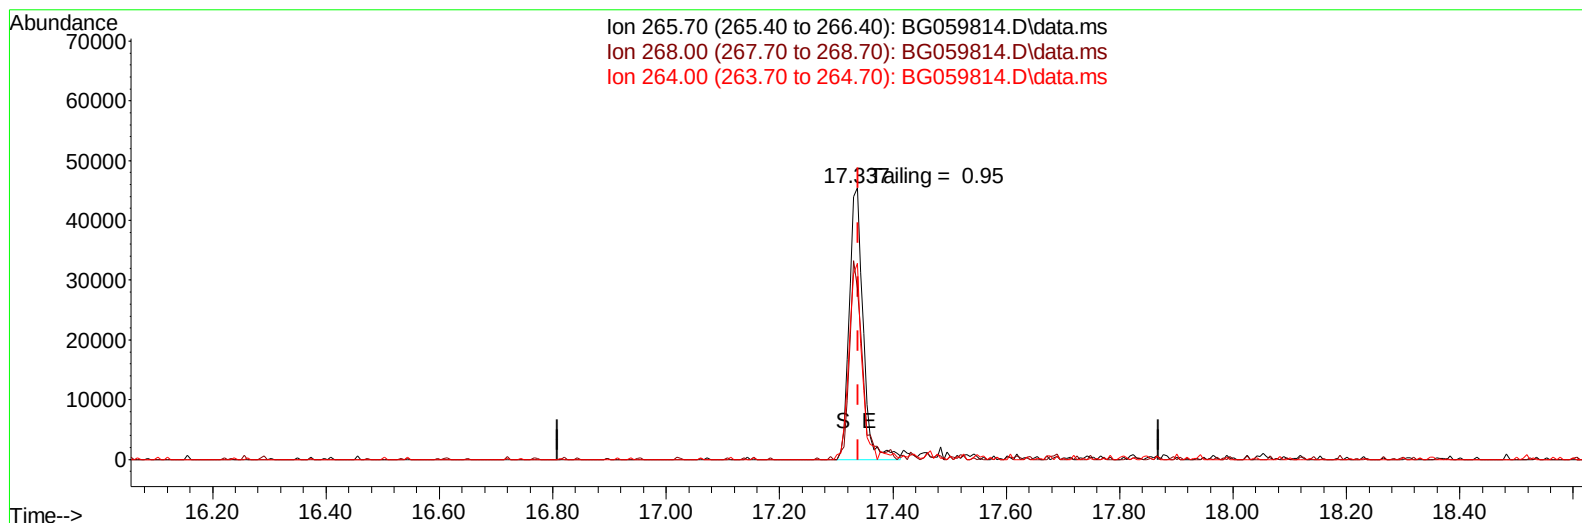

TIC: BG059814.D\data.ms

(70) Pentachlorophenol (C)

17.337min (-0.002) 175563.72 ng




response 75208

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	63.09
264.00	62.30	72.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059814.D
Acq On : 22 Nov 2023 11:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 13:32:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

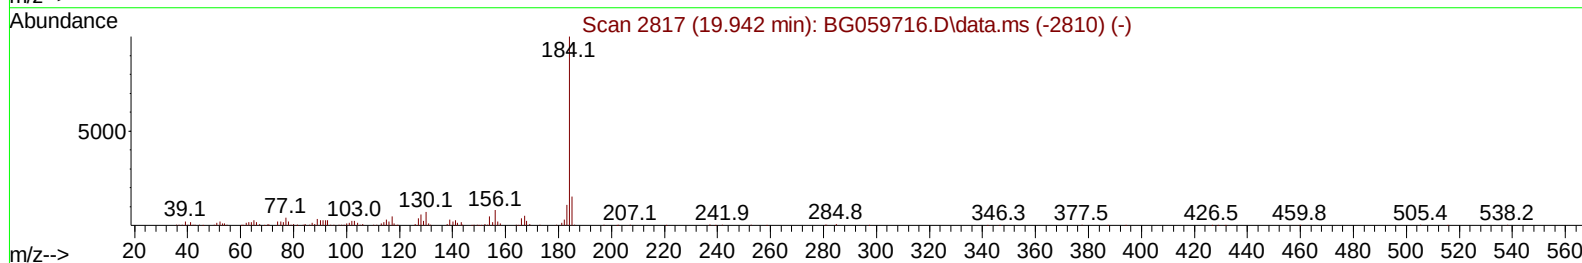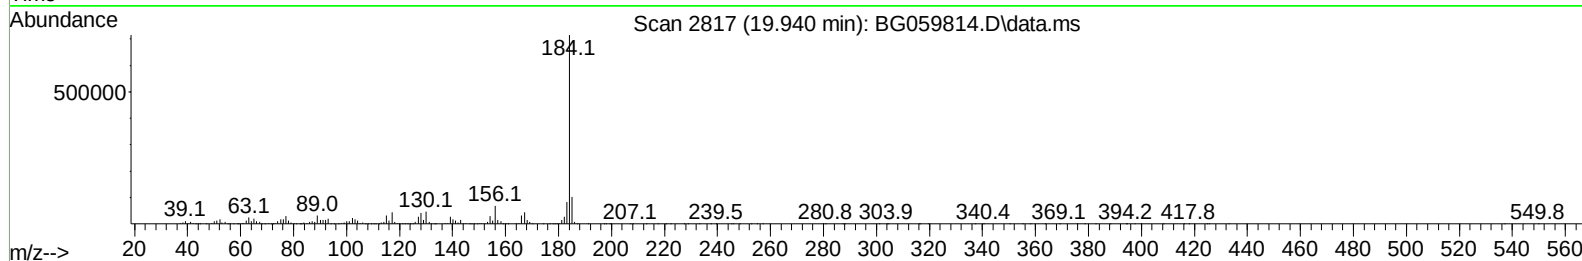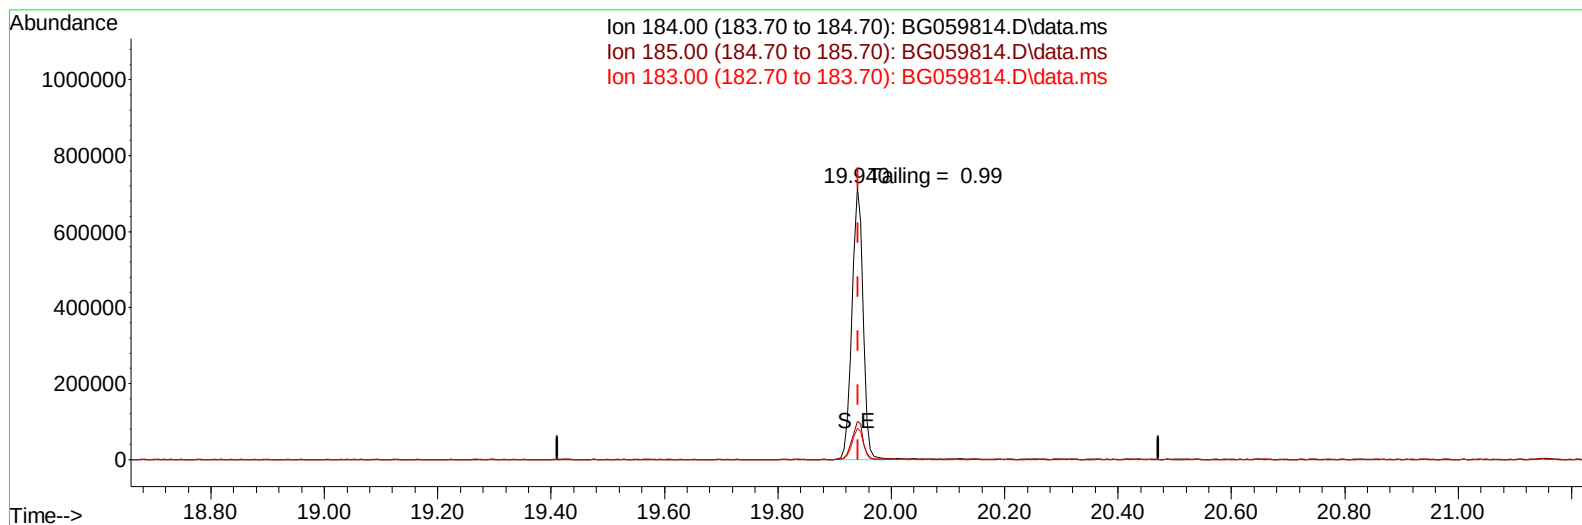

TIC: BG059814.D\data.ms

(77) Benzidine

19.940min (-0.002) 141867.82 ng

response 968305

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.11
183.00	11.00	11.42
0.00	0.00	0.00