
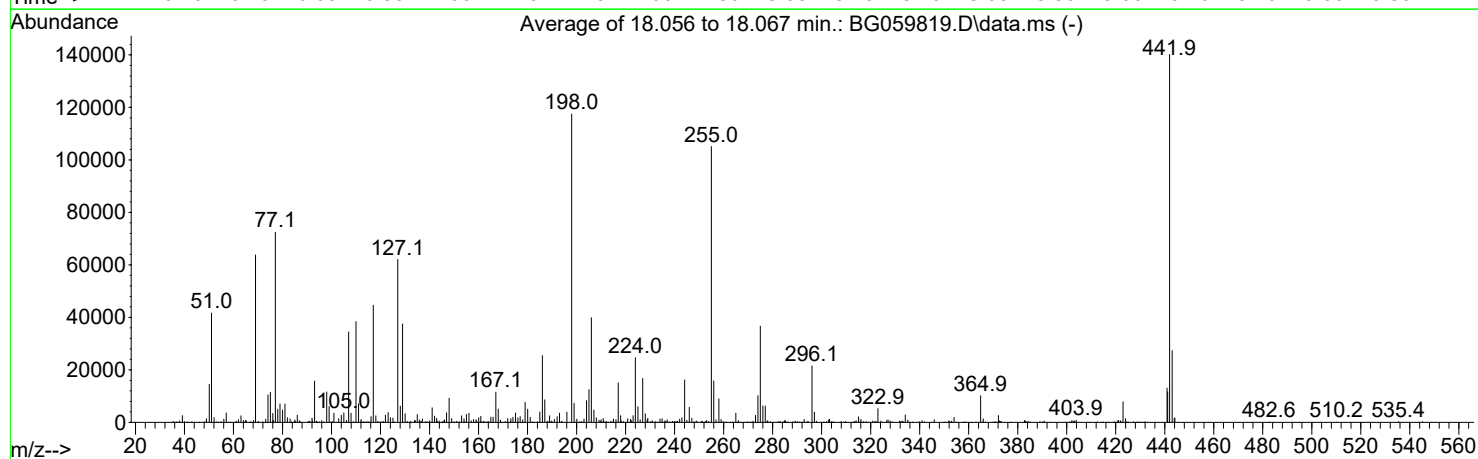


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059819.D
Acq On : 22 Nov 2023 15:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 17 01:51:38 2023

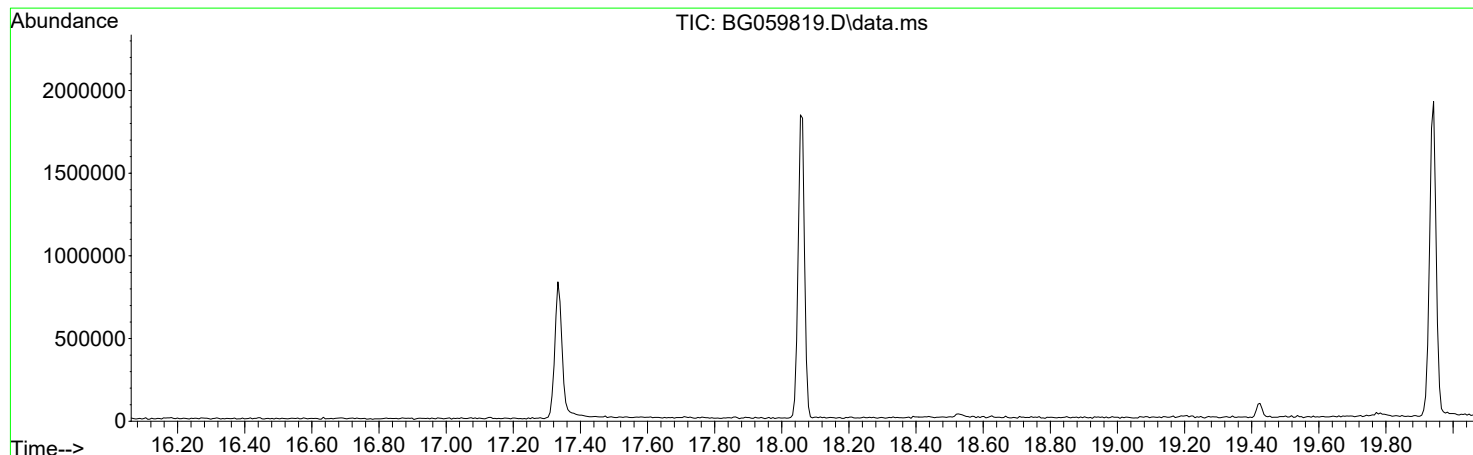

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	41608	PASS
68	69	0.00	2	1.2	736	PASS
69	198	0.00	100	54.3	63767	PASS
70	69	0.00	2	0.5	330	PASS
127	198	10	80	52.8	62077	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	117461	PASS
199	198	5	9	6.2	7266	PASS
275	198	10	60	31.2	36637	PASS
365	198	1	100	8.6	10145	PASS
441	198	0.01	100	11.1	13069	PASS
442	442	50	100	100.0	140149	PASS
443	442	15	24	19.6	27400	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/22/2023	BNA_G	BG059819.D
Compound Name	Response	Retention Time
DDT	396057	21.152
DDD	10446	20.688
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10446	406503	2.57

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
 Data File : BG059819.D
 Acq On : 22 Nov 2023 15:38
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 22 16:37:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 01:51:38 2023
 Response via : Initial Calibration

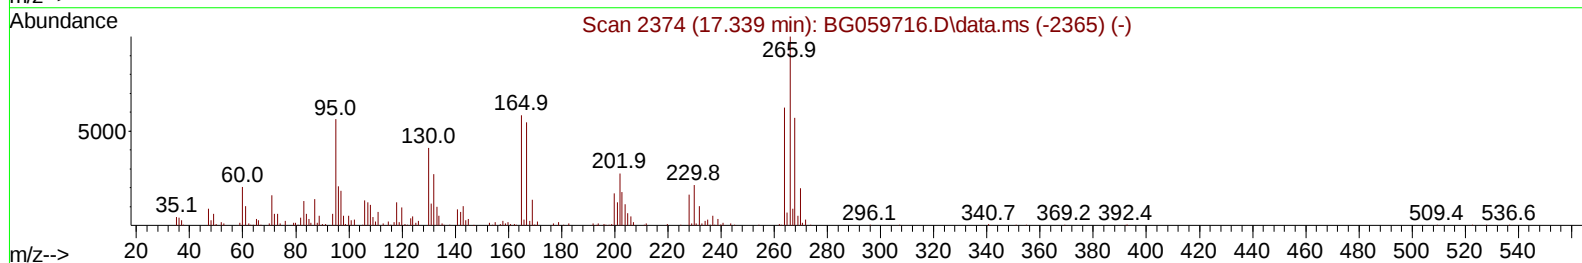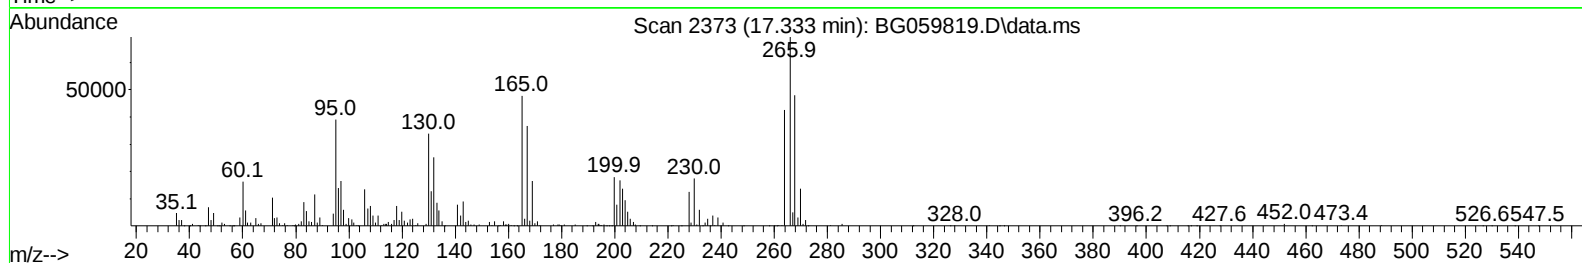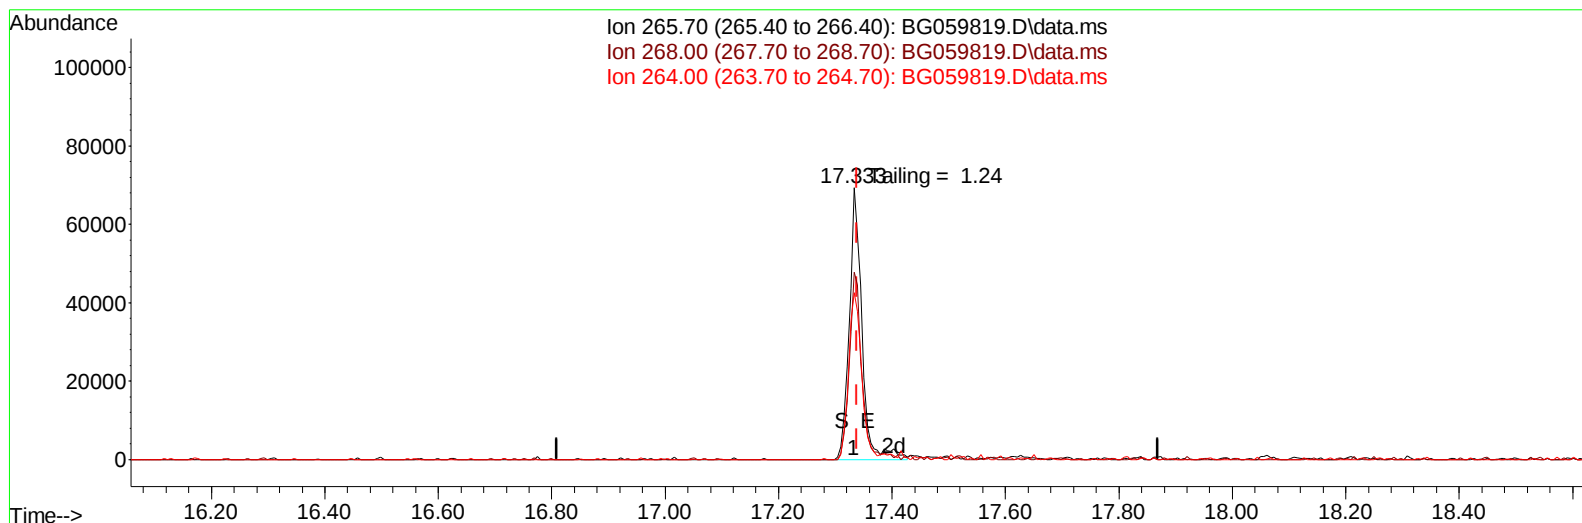

TIC: BG059819.D\data.ms

(70) Pentachlorophenol (C)

17.333min (-0.006) 60741.80 ng




response 103153

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	69.08#
264.00	62.30	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059819.D
Acq On : 22 Nov 2023 15:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 16:37:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

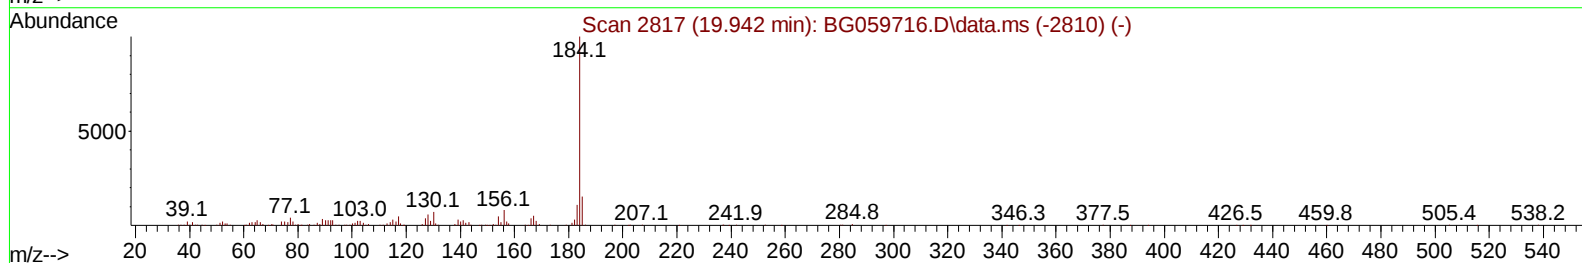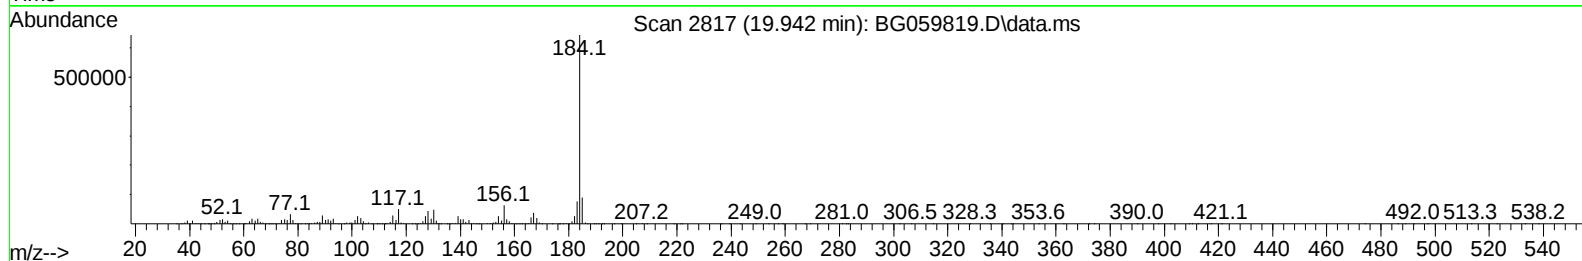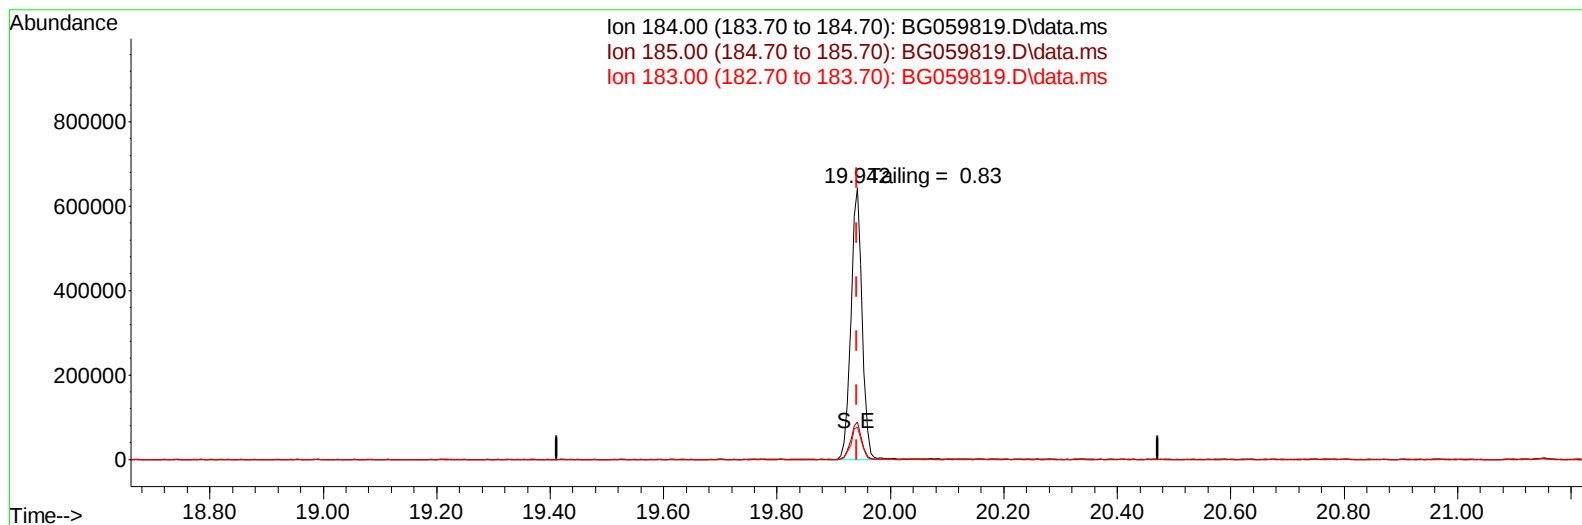

TIC: BG059819.D\data.ms

(77) Benzidine

19.942min (+ 0.000) 61148.45 ng

response 880483

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.82
183.00	11.00	11.92
0.00	0.00	0.00