
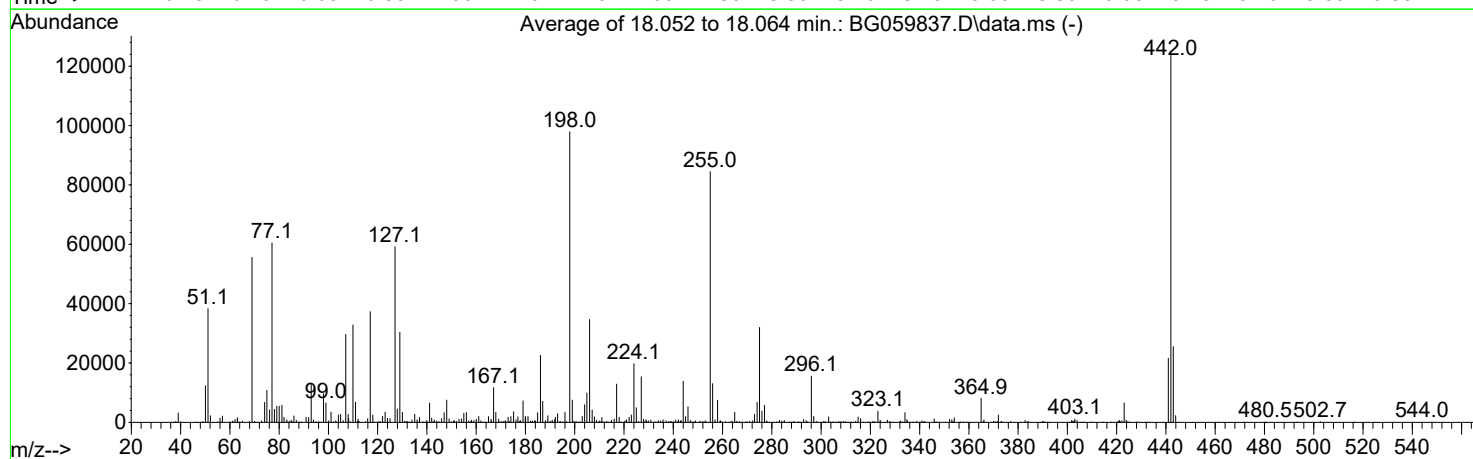


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
 Data File : BG059837.D
 Acq On : 23 Nov 2023 4:31
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 01:51:38 2023

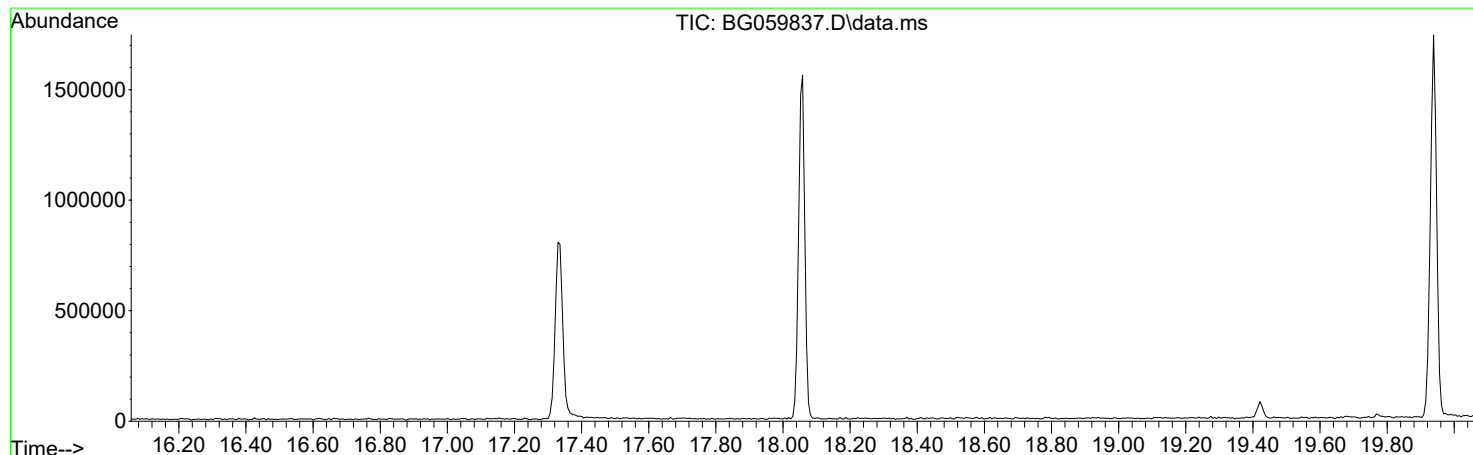

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	38328	PASS
68	69	0.00	2	0.5	286	PASS
69	198	0.00	100	56.8	55587	PASS
70	69	0.00	2	0.7	364	PASS
127	198	10	80	60.5	59189	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97893	PASS
199	198	5	9	7.7	7508	PASS
275	198	10	60	32.6	31949	PASS
365	198	1	100	8.2	8072	PASS
441	198	0.01	100	22.0	21571	PASS
442	442	50	100	100.0	123925	PASS
443	442	15	24	20.6	25477	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/22/2023	BNA_G	<u>BG059837.D</u>
Compound Name	Response	Retention Time
DDT	289529	21.149
DDD	27410	20.685
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27410	316939	8.65

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112223\
Data File : BG059837.D
Acq On : 23 Nov 2023 4:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 23 05:59:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

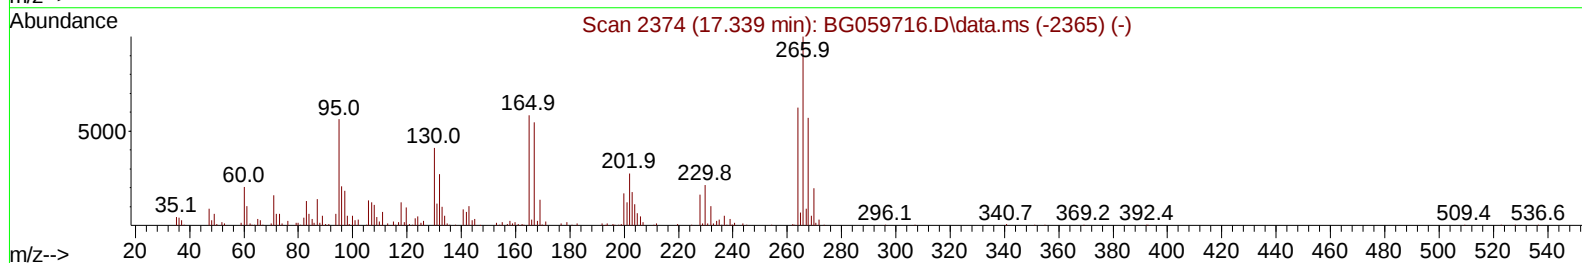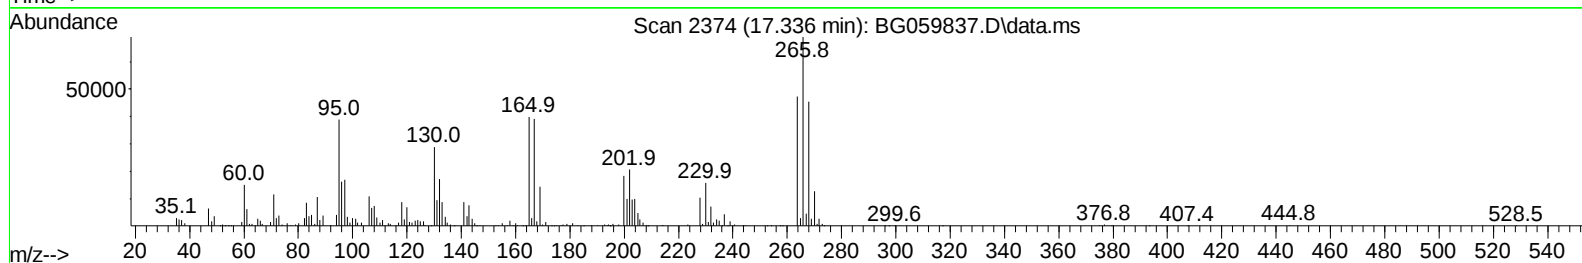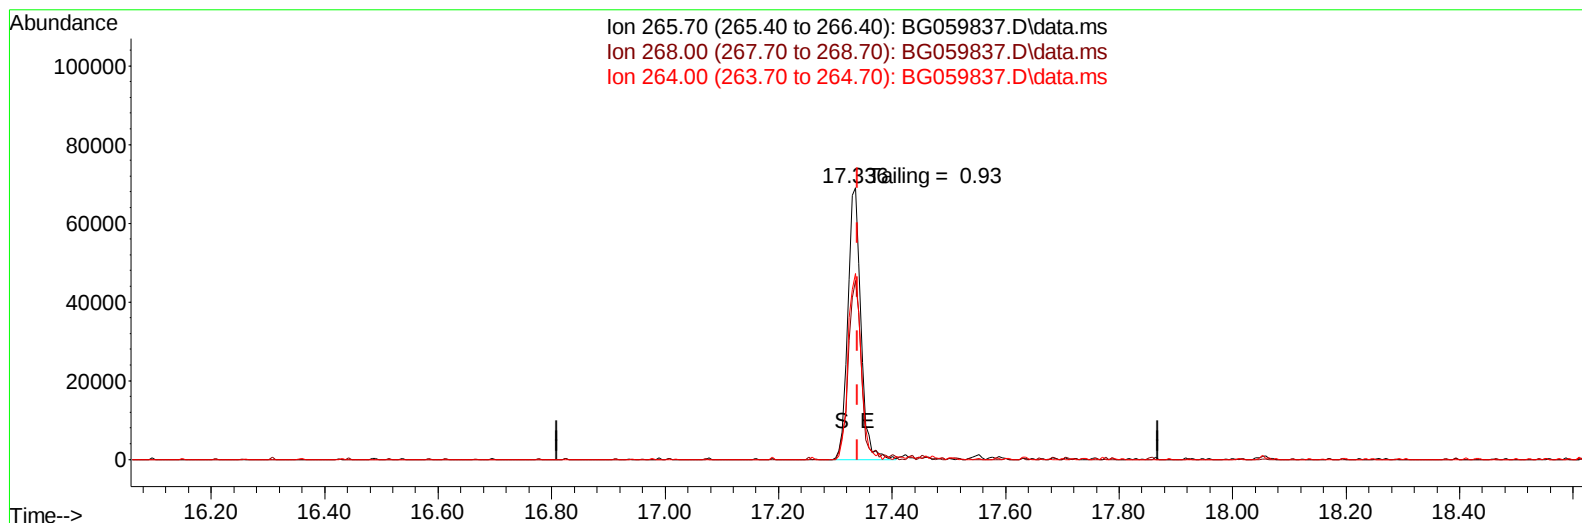

TIC: BG059837.D\data.ms

(70) Pentachlorophenol (C)

17.336min (-0.003) 83730.90 ng

response 110168

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	65.82
264.00	62.30	68.39
0.00	0.00	0.00

