


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112319\
 Data File : BG043751.D
 Acq On : 23 Nov 2019 10:36
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG112219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 23 00:54:00 2019

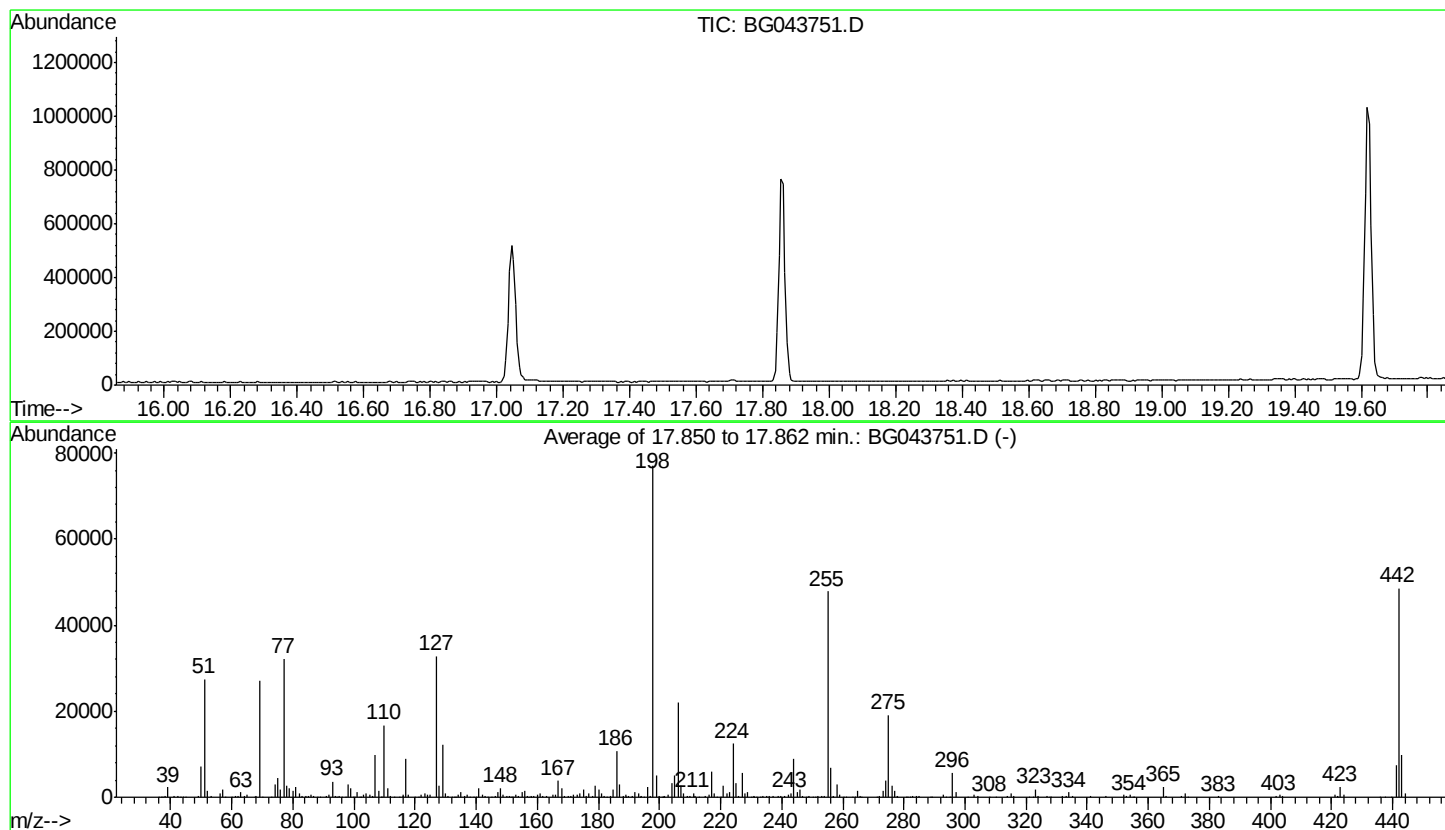

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	27498	PASS
68	69	0.00	2	0.8	229	PASS
69	198	0.00	100	35.3	27190	PASS
70	69	0.00	2	0.1	20	PASS
127	198	10	80	42.5	32730	PASS
197	198	0.00	2	0.4	344	PASS
198	198	100	100	100.0	77056	PASS
199	198	5	9	6.7	5167	PASS
275	198	10	60	24.9	19190	PASS
365	198	1	100	3.3	2524	PASS
441	198	0.01	100	9.8	7535	PASS
442	198	50	100	63.1	48597	PASS
443	442	15	24	20.1	9781	PASS