

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051208.D
 Acq On : 24 Nov 2021 12:05
 Operator : CG/JU
 Sample : M4752-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG1X2

Quant Time: Nov 24 14:29:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.197	152	30464	20.000	ng/ul	0.00
20) Naphthalene-d8	11.023	136	142930	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.830	164	101901	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.580	188	223719	20.000	ng/ul	0.00
79) Chrysene-d12	21.875	240	199601	20.000	ng/ul	0.00
88) Perylene-d12	25.271	264	194795	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.544	96	3549	4.048	ng/uL	0.00
4) Pyridine-d5	3.972	84	17568	6.829	ng/ul	0.00
7) Phenol-d5	7.357	99	21095	7.006	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.515	67	59143	31.277	ng/ul	0.00
11) 2-Chlorophenol-d4	7.727	132	53040	24.464	ng/ul	0.00
15) 4-Methylphenol-d8	8.908	113	39566	16.284	ng/ul	0.00
21) Nitrobenzene-d5	9.378	128	35926	29.776	ng/ul	0.00
24) 2-Nitrophenol-d4	10.101	143	41344	30.377	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.647	165	65296	28.276	ng/ul	0.00
31) 4-Chloroaniline-d4	11.164	131	82633	24.456	ng/ul	0.00
46) Dimethylphthalate-d6	14.225	166	269282	34.344	ng/ul	0.00
49) Acenaphthylene-d8	14.525	160	323535	32.723	ng/ul	0.00
54) 4-Nitrophenol-d4	15.054	143	7876	6.206	ng/ul	0.00
60) Fluorene-d10	15.817	176	238082	33.720	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.947	200	42358	30.683	ng/ul	0.00
73) Anthracene-d10	17.680	188	384889	35.972	ng/ul	0.00
81) Pyrene-d10	19.954	212	433376	35.883	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.042	264	389653	37.454	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.386	94	3261	1.045	ng/ul#	89
78) Di-n-butylphthalate	18.508	149	15062	1.085	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051208.D
Acq On : 24 Nov 2021 12:05
Operator : CG/JU
Sample : M4752-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG1X2

Quant Time: Nov 24 14:29:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration




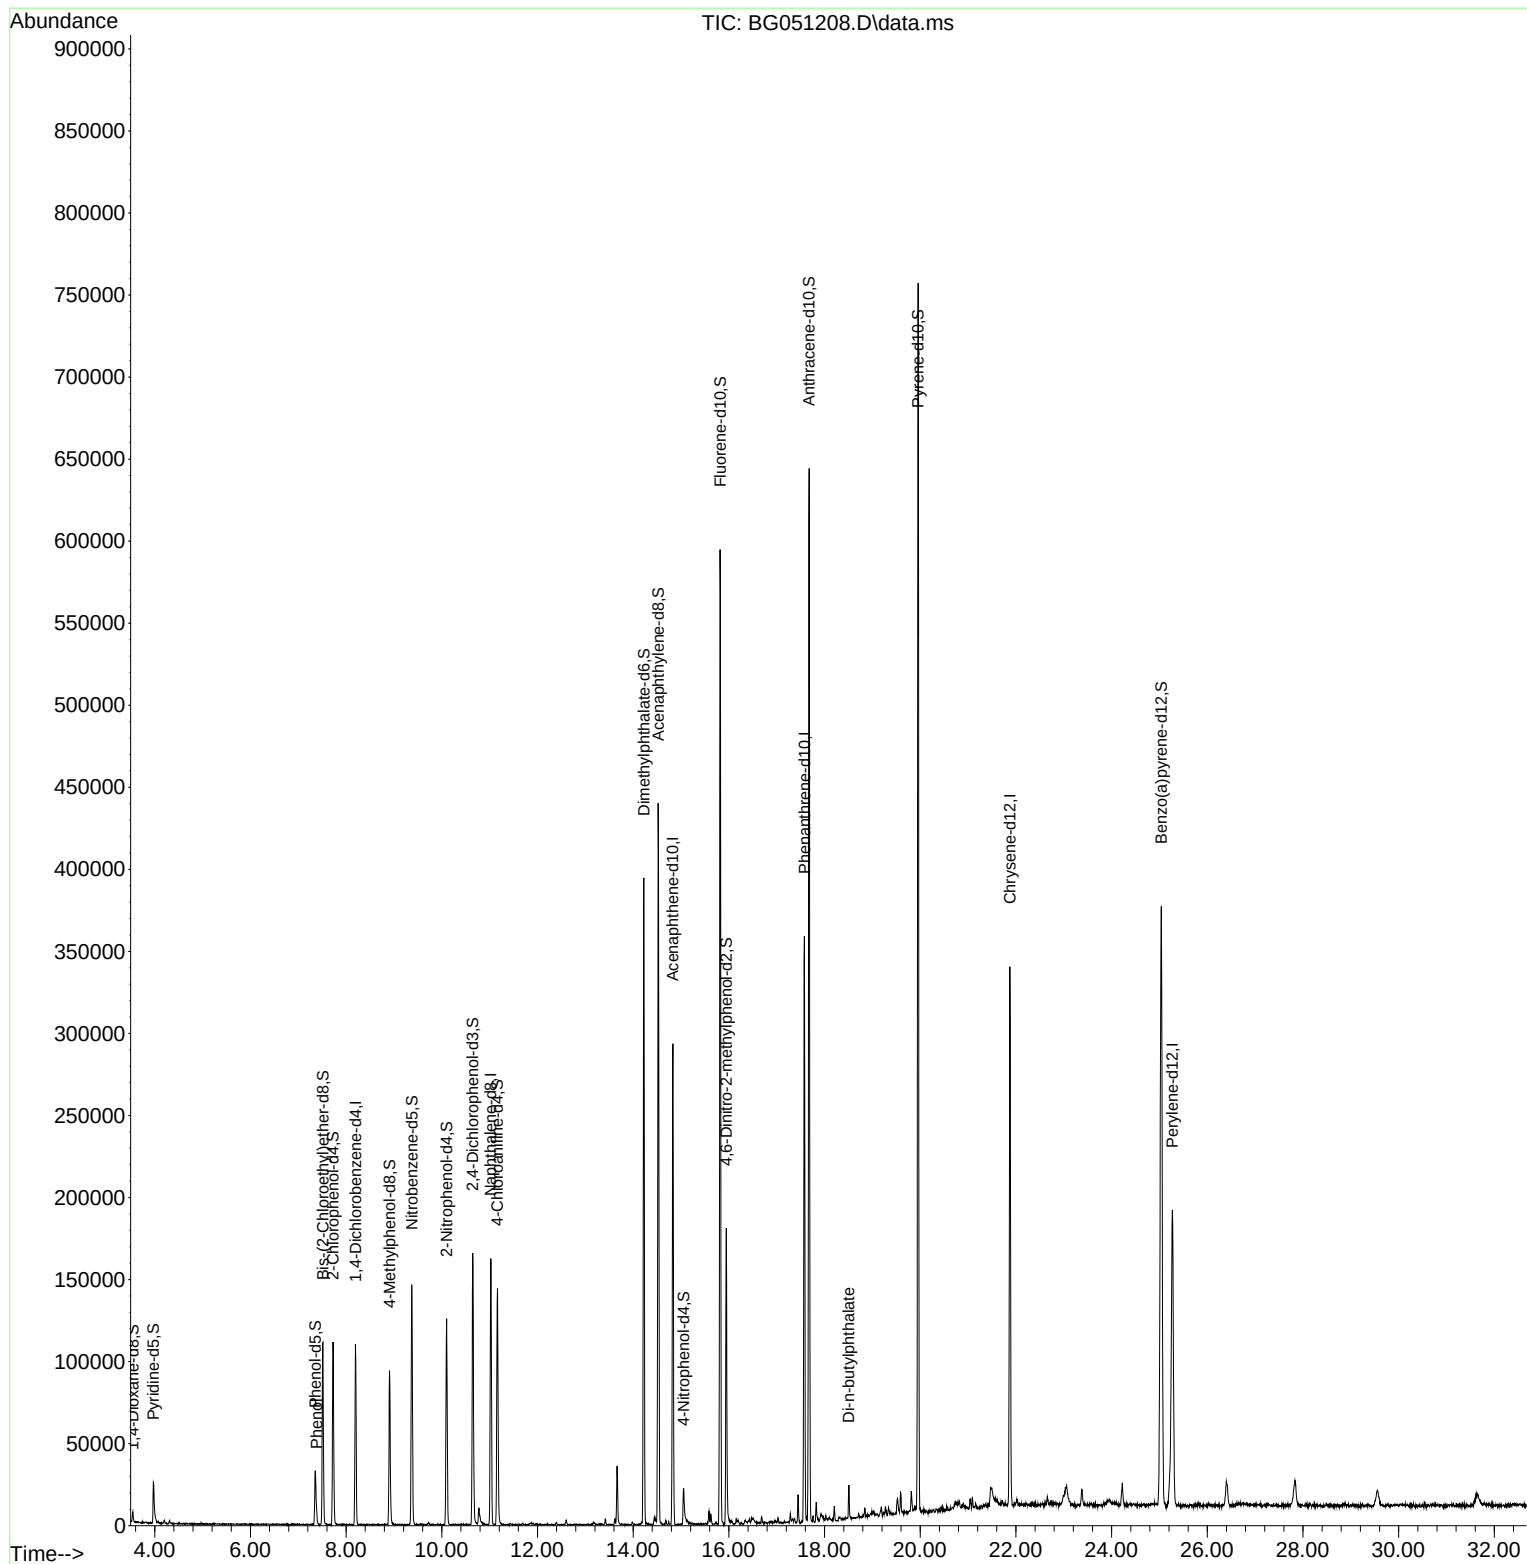


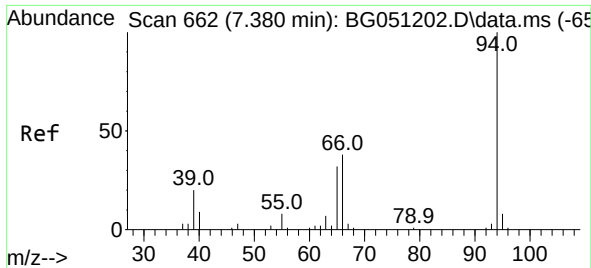

#8
Phenol
Concen: 1.045 ng/ul
RT: 7.386 min Scan# 662
Delta R.T. -0.000 min
Lab File: BG051208.D
Acq: 24 Nov 2021 12:05

Instrument :
BNA_G
ClientSampleId :
BG1X2

Tgt Ion: 94 Resp: 3261
Ion Ratio Lower Upper
94 100
65 24.7 25.1 37.7#
66 45.6 31.6 47.4

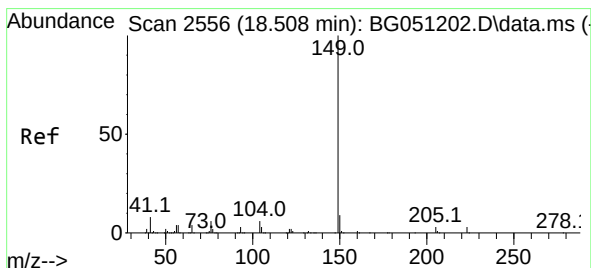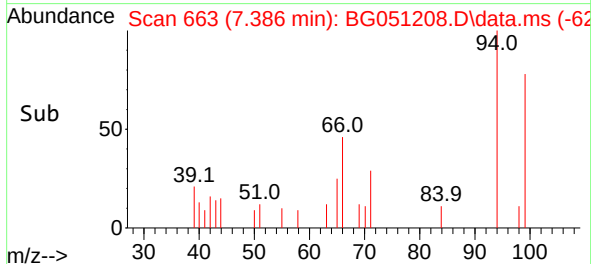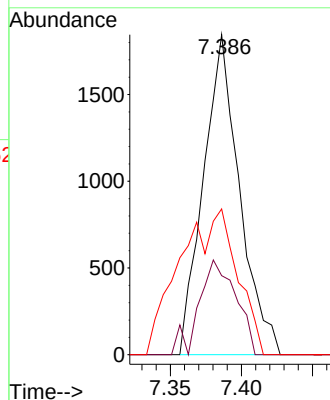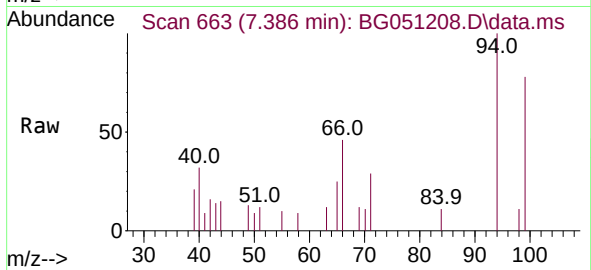

#78
Di-n-butylphthalate
Concen: 1.085 ng/ul
RT: 18.508 min Scan# 2556
Delta R.T. -0.006 min
Lab File: BG051208.D
Acq: 24 Nov 2021 12:05

Tgt Ion: 149 Resp: 15062
Ion Ratio Lower Upper
149 100
150 7.9 7.5 11.3
104 6.0 5.0 7.6

