

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051210.D
 Acq On : 24 Nov 2021 13:27
 Operator : CG/JU
 Sample : M4753-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A0010

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
 Supervised By :Sohil Jodhani 11/30/2021

Quant Time: Nov 24 14:31:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.199	152	28502	20.000	ng/u1	0.00
20) Naphthalene-d8	11.025	136	130204	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.827	164	93971	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.577	188	206624	20.000	ng/u1	0.00
79) Chrysene-d12	21.877	240	185966	20.000	ng/u1	0.00
88) Perylene-d12	25.268	264	184232	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.540	96	3337	4.069	ng/uL	0.00
4) Pyridine-d5	3.975	84	13733	5.706	ng/u1	0.00
7) Phenol-d5	7.353	99	14046	4.986	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.512	67	42605	24.082	ng/u1	0.00
11) 2-Chlorophenol-d4	7.729	132	38272	18.867	ng/u1	0.00
15) 4-Methylphenol-d8	8.910	113	27137	11.938	ng/u1	0.00
21) Nitrobenzene-d5	9.374	128	26163	23.804	ng/u1	0.00
24) 2-Nitrophenol-d4	10.103	143	29006	23.395	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.649	165	46238	21.980	ng/u1	0.00
31) 4-Chloroaniline-d4	11.161	131	65093	21.148	ng/u1	0.00
46) Dimethylphthalate-d6	14.222	166	186344	25.772	ng/u1	0.00
49) Acenaphthylene-d8	14.527	160	226399	24.831	ng/u1	0.00
54) 4-Nitrophenol-d4	15.068	143	5048m	4.313	ng/u1	0.02
60) Fluorene-d10	15.820	176	171881	26.398	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.949	200	30990	24.306	ng/u1	0.00
73) Anthracene-d10	17.676	188	307069	31.073	ng/u1	0.00
81) Pyrene-d10	19.956	212	346596	30.802	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.038	264	313046	31.816	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.383	94	3811	1.306	ng/u1	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051210.D
Acq On : 24 Nov 2021 13:27
Operator : CG/JU
Sample : M4753-01
Misc :
ALS Vial : 31 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
A0010

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
Supervised By :Sohil Jodhani 11/30/2021

Quant Time: Nov 24 14:31:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration

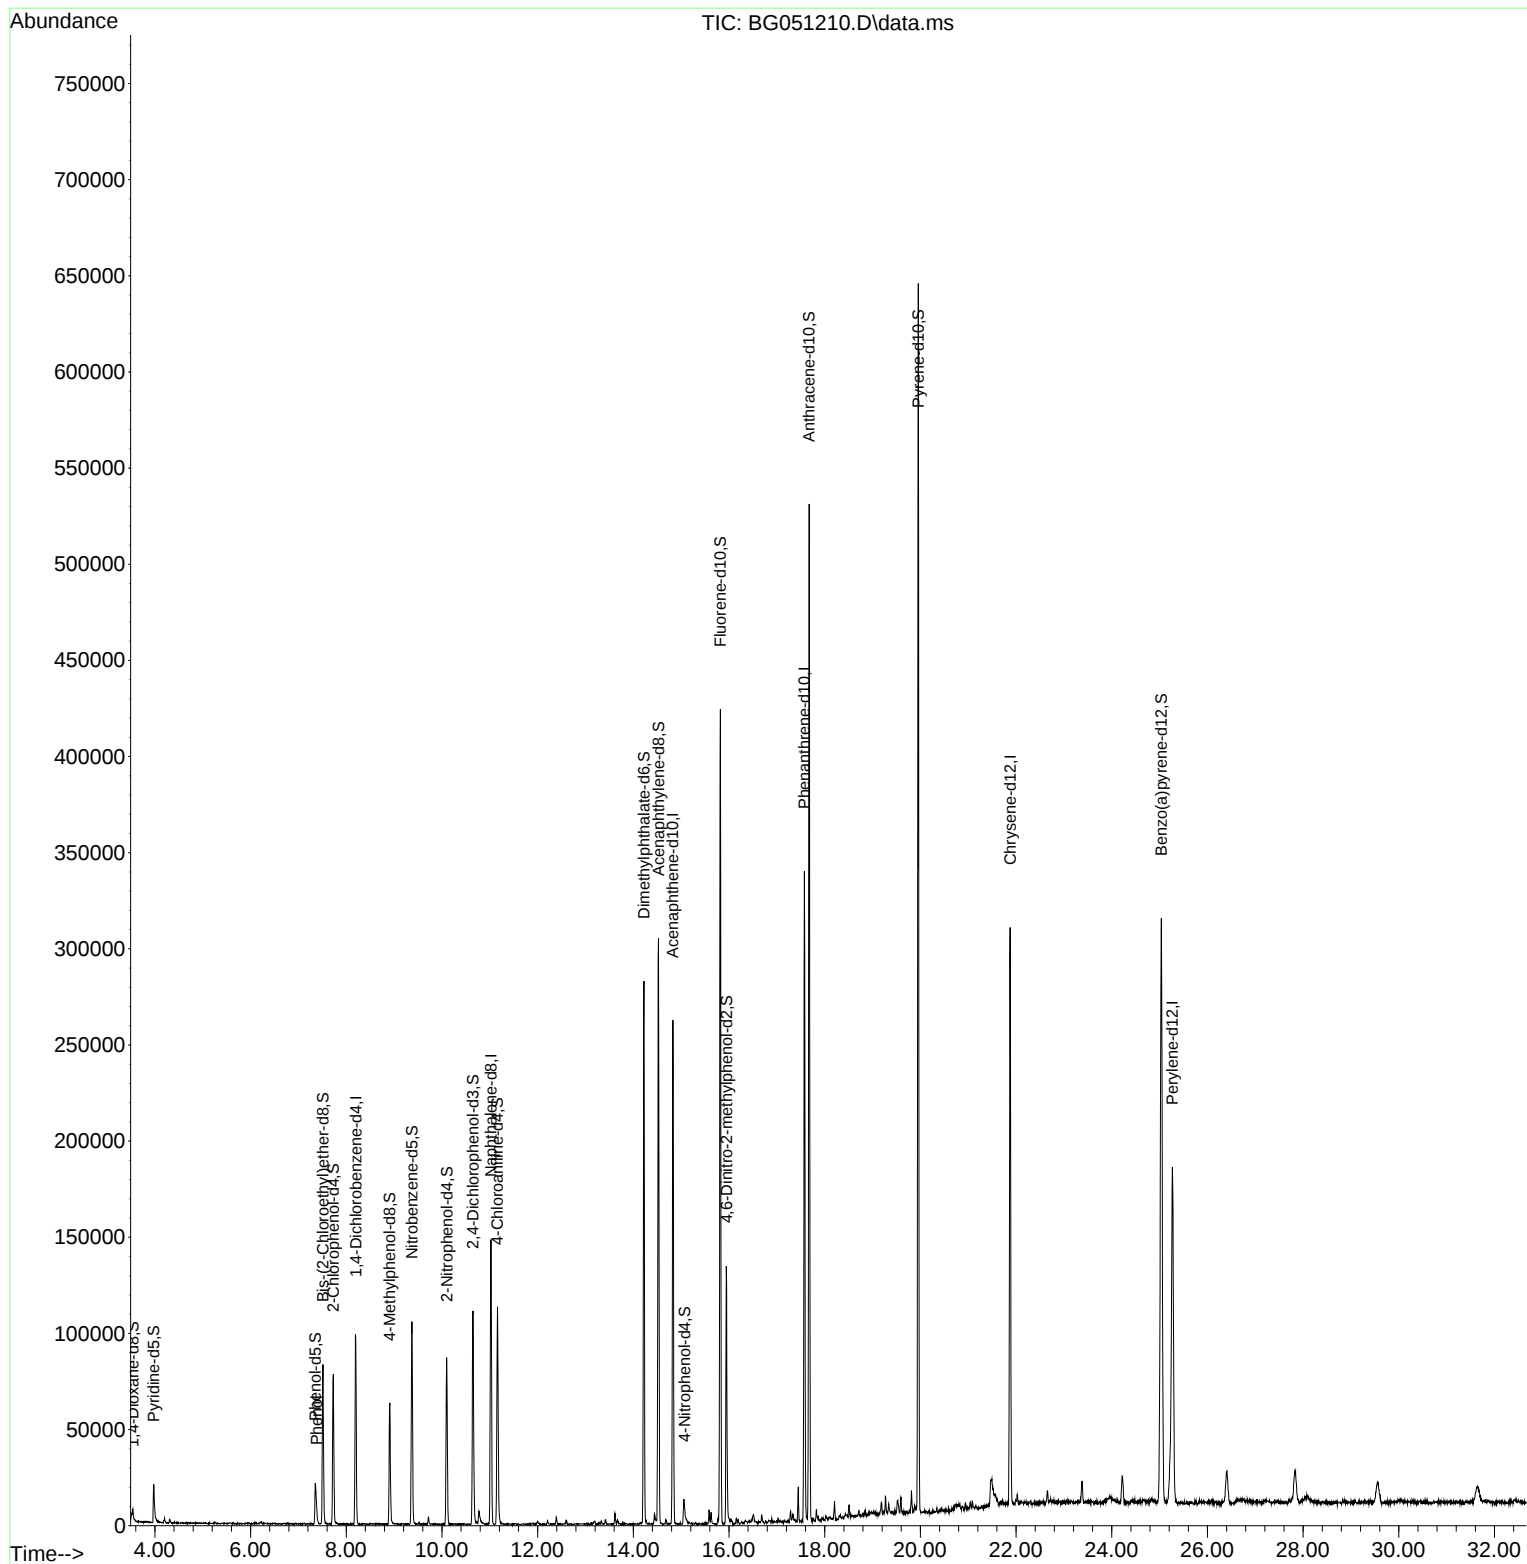

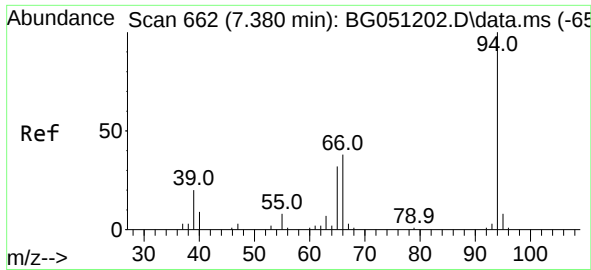

#8
Phenol
Concen: 1.306 ng/ul
RT: 7.383 min Scan# 60
Delta R.T. -0.004 min
Lab File: BG051210.D
Acq: 24 Nov 2021 13:27

Instrument :
BNA_G
ClientSampleId :
A0010

Tgt Ion: 94 Resp: 381
Ion Ratio Lower Upper
94 100
65 29.0 25.1 37.7
66 42.7 31.6 47.4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
Supervised By :Sohil Jodhani 11/30/2021

