

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051212.D
 Acq On : 24 Nov 2021 14:49
 Operator : CG/JU
 Sample : M4702-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLQ0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
 Supervised By :Sohil Jodhani 11/30/2021

Quant Time: Nov 24 17:06:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.194	152	29657	20.000	ng/u1	0.00
20) Naphthalene-d8	11.020	136	136867	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.828	164	95893	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.577	188	210904	20.000	ng/u1	0.00
79) Chrysene-d12	21.878	240	183728	20.000	ng/u1	0.00
88) Perylene-d12	25.268	264	181238	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.541	96	1988	2.329	ng/uL	0.00
4) Pyridine-d5	3.976	84	22630	9.037	ng/u1	0.00
7) Phenol-d5	7.354	99	36170	12.340	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.513	67	24267	13.182	ng/u1	0.00
11) 2-Chlorophenol-d4	7.724	132	27671	13.110	ng/u1	0.00
15) 4-Methylphenol-d8	8.911	113	28830	12.189	ng/u1	0.00
21) Nitrobenzene-d5	9.375	128	14667	12.695	ng/u1	0.00
24) 2-Nitrophenol-d4	10.104	143	16654	12.778	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.650	165	26531	11.998	ng/u1	0.00
31) 4-Chloroaniline-d4	11.167	131	36754	11.359	ng/u1	0.00
46) Dimethylphthalate-d6	14.222	166	97038	13.152	ng/u1	0.00
49) Acenaphthylene-d8	14.522	160	122976	13.217	ng/u1	0.00
54) 4-Nitrophenol-d4	15.045	143	10149m	8.498	ng/u1	0.00
60) Fluorene-d10	15.815	176	88058	13.253	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.950	200	12151	9.337	ng/u1	0.00
73) Anthracene-d10	17.677	188	130186	12.907	ng/u1	0.00
81) Pyrene-d10	19.957	212	155296	13.969	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.033	264	128782	13.305	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.720	149	39009	4.882	ng/u1	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051212.D
Acq On : 24 Nov 2021 14:49
Operator : CG/JU
Sample : M4702-15
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
DBLQ0

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
Supervised By :Sohil Jodhani 11/30/2021


Quant Time: Nov 24 17:06:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration

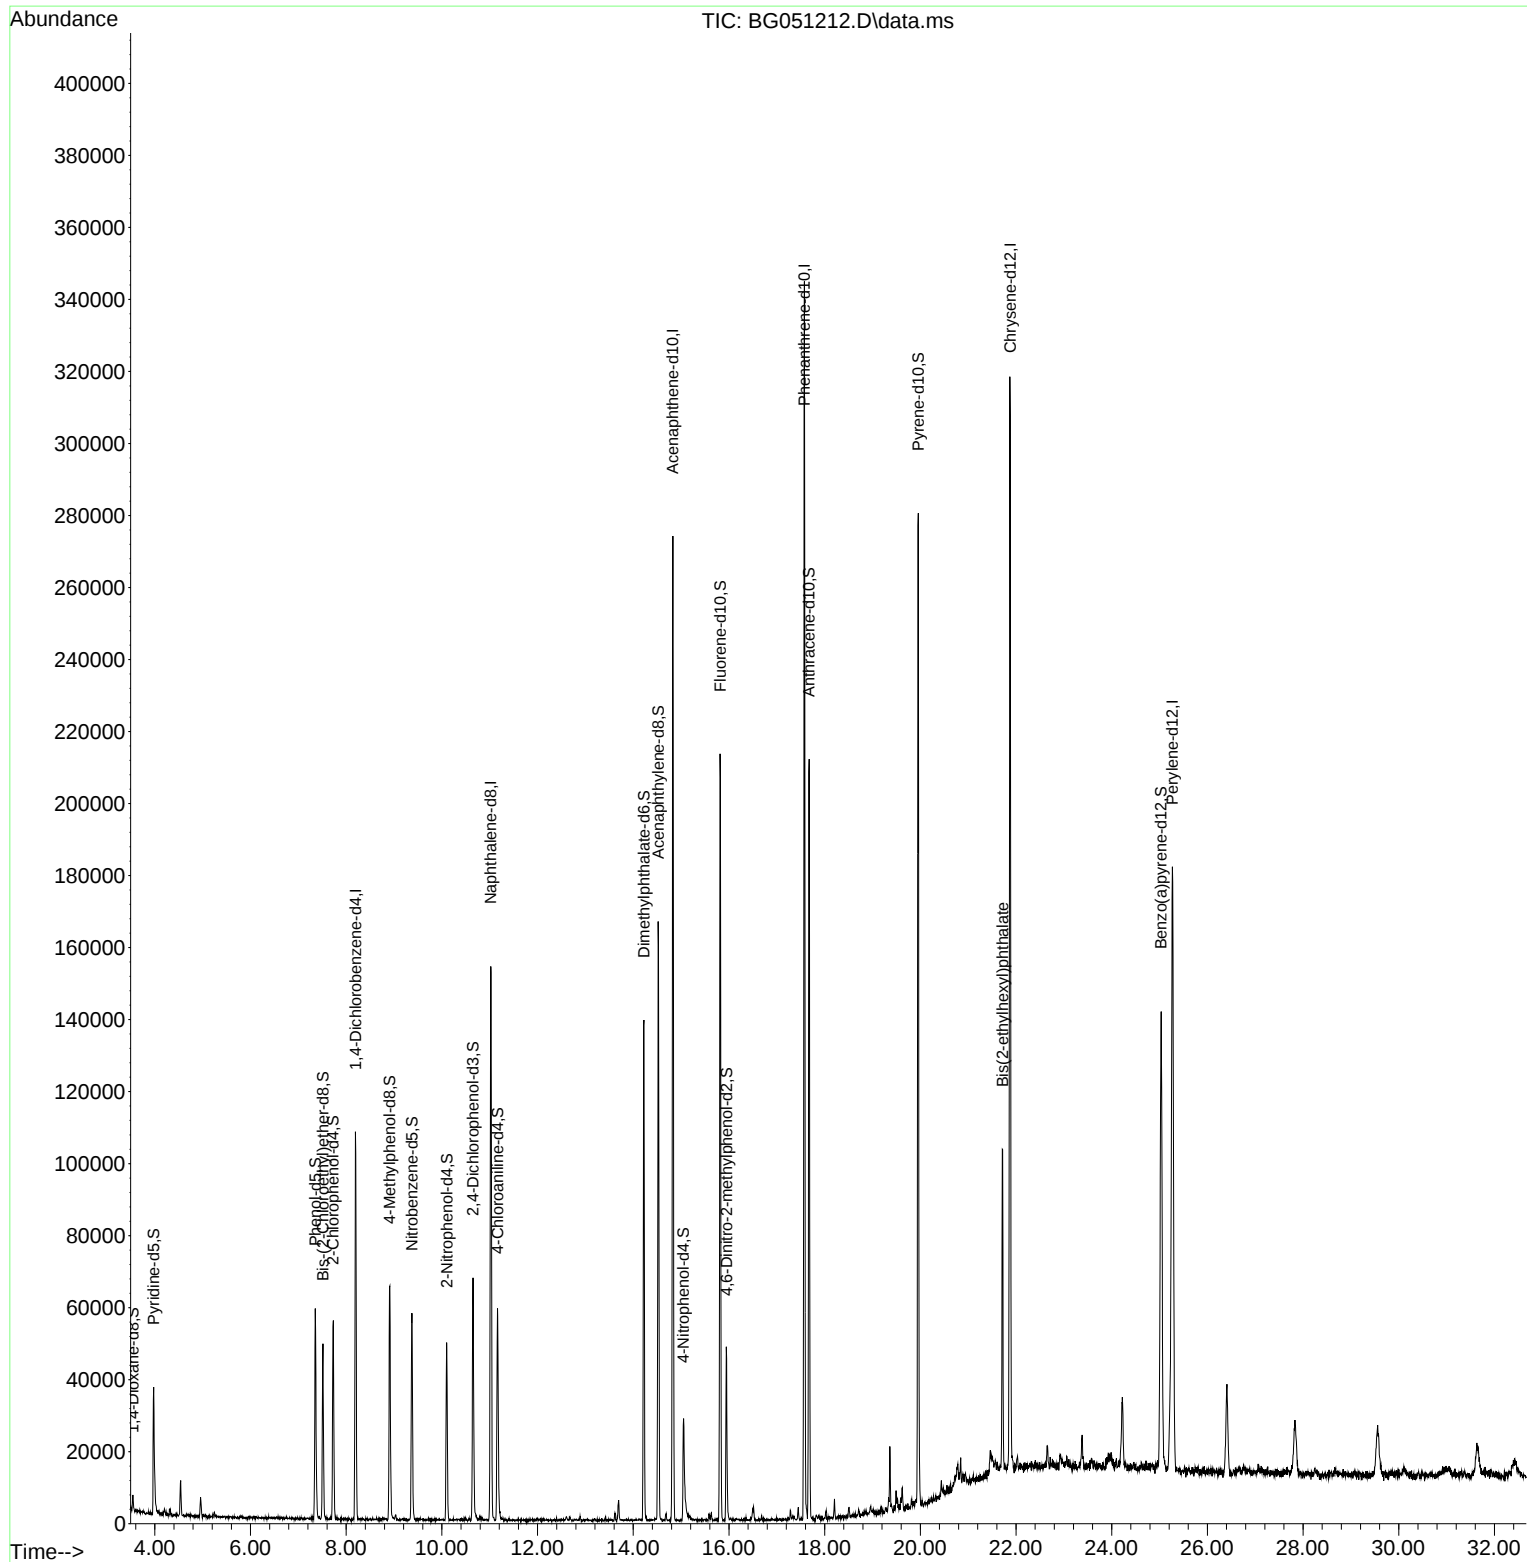

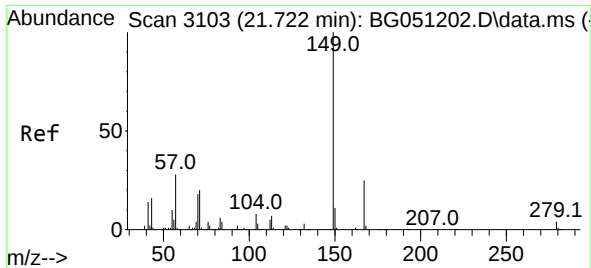

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 4.882 ng/ul
 RT: 21.720 min Scan# 3103
 Delta R.T. -0.003 min
 Lab File: BG051212.D
 Acq: 24 Nov 2021 14:49

Instrument :
 BNA_G
 ClientSampleId :
 DBLQ0

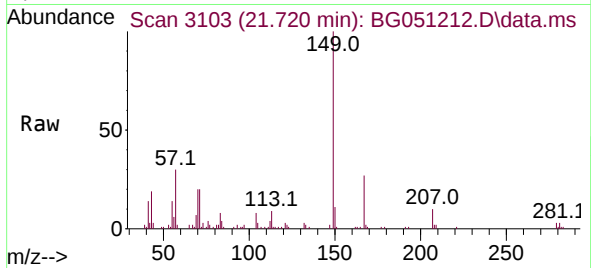

Tgt Ion:149 Resp: 39009
 Ion Ratio Lower Upper
 149 100
 167 26.6 21.1 31.7
 279 3.2 2.7 4.1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
 Supervised By :Sohil Jodhani 11/30/2021

