

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051225.D
 Acq On : 25 Nov 2021 00:21
 Operator : CG/JU
 Sample : M4725-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F4L00

Quant Time: Nov 25 04:21:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.200	152	32634	20.000	ng/u1	0.00
20) Naphthalene-d8	11.027	136	147484	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.828	164	99218	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.584	188	201919	20.000	ng/u1	0.00
79) Chrysene-d12	21.879	240	174607	20.000	ng/u1	0.00
88) Perylene-d12	25.286	264	174516	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.541	96	3714	3.955	ng/uL	0.00
4) Pyridine-d5	3.976	84	30649	11.122	ng/u1	0.00
7) Phenol-d5	7.360	99	18530	5.745	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.513	67	57681	28.475	ng/u1	0.00
11) 2-Chlorophenol-d4	7.730	132	43483	18.722	ng/u1	0.00
15) 4-Methylphenol-d8	8.911	113	33486	12.866	ng/u1	0.00
21) Nitrobenzene-d5	9.376	128	36257	29.123	ng/u1	0.00
24) 2-Nitrophenol-d4	10.104	143	32340	23.028	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.650	165	51508	21.617	ng/u1	0.00
31) 4-Chloroaniline-d4	11.168	131	77133	22.123	ng/u1	0.00
46) Dimethylphthalate-d6	14.223	166	232486	30.453	ng/u1	0.00
49) Acenaphthylene-d8	14.528	160	290019	30.127	ng/u1	0.00
54) 4-Nitrophenol-d4	15.063	143	7653	6.193	ng/u1	0.02
60) Fluorene-d10	15.821	176	208669	30.353	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.950	200	23170	18.596	ng/u1	0.00
73) Anthracene-d10	17.678	188	329493	34.119	ng/u1	0.00
81) Pyrene-d10	19.957	212	369976	35.019	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.045	264	328210	35.214	ng/u1	0.00
Target Compounds						Qvalue
8) Phenol	7.390	94	5501	1.646	ng/u1	92
59) Diethylphthalate	15.621	149	11557	1.425	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051225.D
Acq On : 25 Nov 2021 00:21
Operator : CG/JU
Sample : M4725-01
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
F4L00

Quant Time: Nov 25 04:21:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration




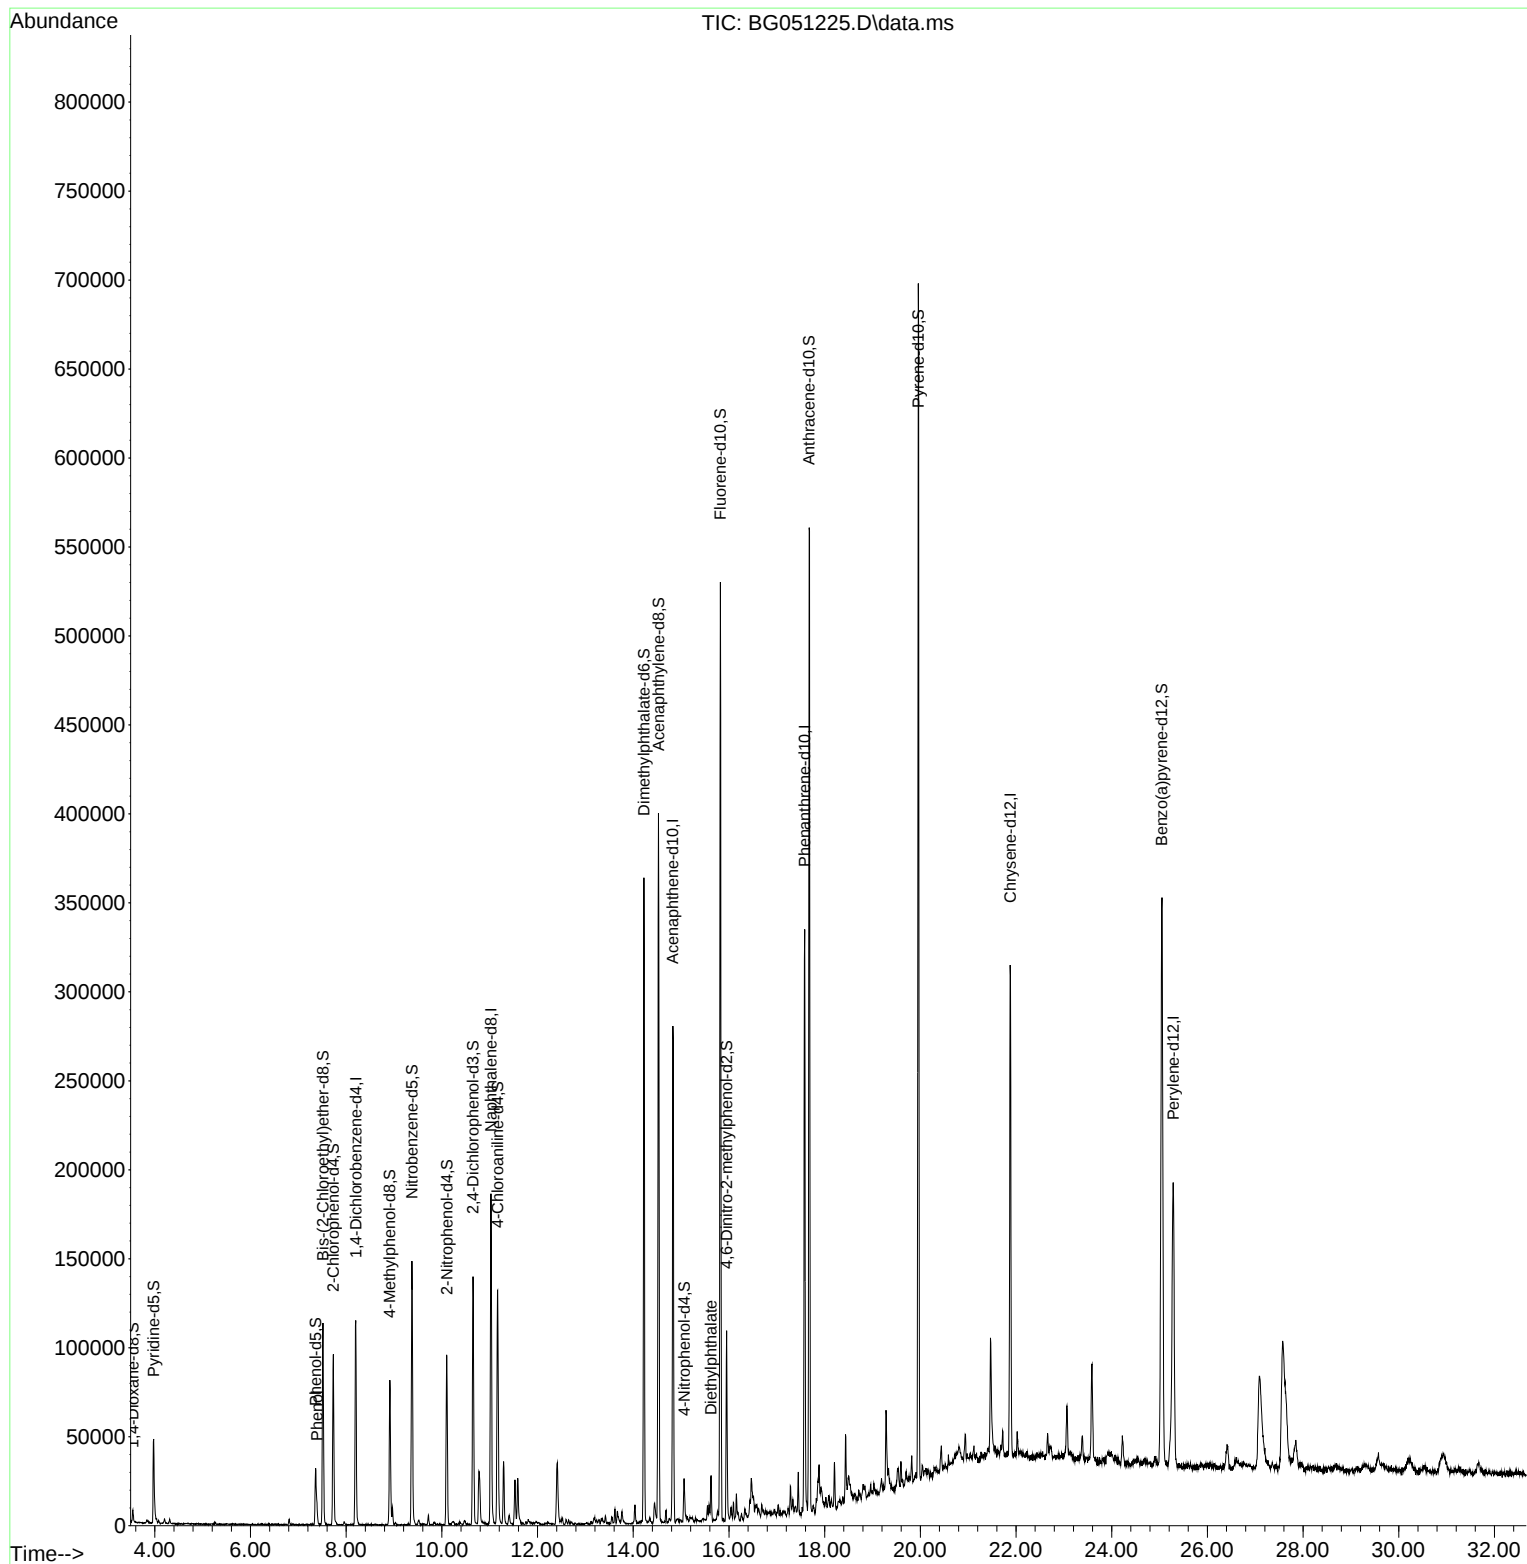


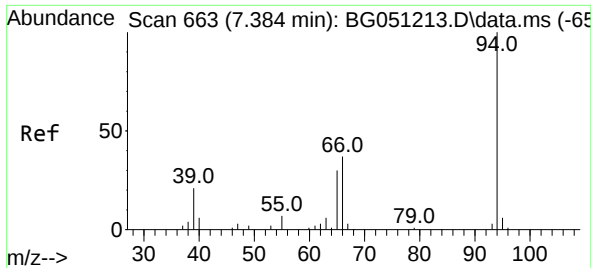

#8
Phenol
Concen: 1.646 ng/ul
RT: 7.390 min Scan# 60
Delta R.T. 0.003 min
Lab File: BG051225.D
Acq: 25 Nov 2021 00:21

Instrument :
BNA_G
ClientSampleId :
F4L00

Tgt Ion: 94	Resp:	5501
Ion Ratio	Lower	Upper
94	100	
65	35.3	25.1 37.7
66	45.2	31.6 47.4

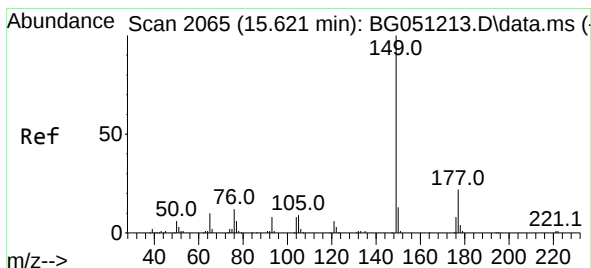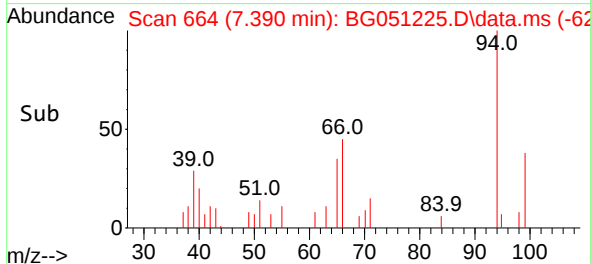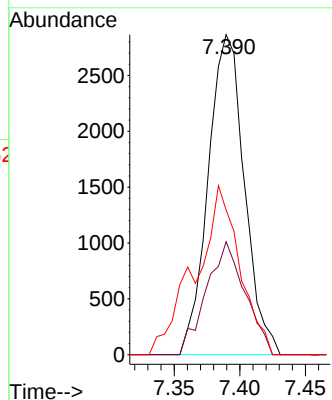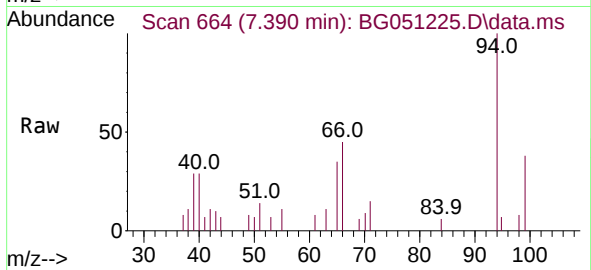

#59
Diethylphthalate
Concen: 1.425 ng/ul
RT: 15.621 min Scan# 2065
Delta R.T. -0.003 min
Lab File: BG051225.D
Acq: 25 Nov 2021 00:21

Tgt Ion: 149	Resp:	11557
Ion Ratio	Lower	Upper
149	100	
177	21.7	16.8 25.2
150	10.8	10.1 15.1

