

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051232.D
 Acq On : 25 Nov 2021 5:45
 Operator : CG/JU
 Sample : M4725-07
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F4L13

Quant Time: Nov 25 06:37:41 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.200	152	26903	20.000	ng/u1	0.00
20) Naphthalene-d8	11.026	136	122524	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.828	164	83914	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.577	188	178673	20.000	ng/u1	0.00
79) Chrysene-d12	21.878	240	153737	20.000	ng/u1	0.00
88) Perylene-d12	25.280	264	152701	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.541	96	3216	4.154	ng/uL	0.00
4) Pyridine-d5	3.976	84	15982	7.035	ng/u1	0.00
7) Phenol-d5	7.360	99	21185	7.968	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.513	67	58539	35.055	ng/u1	0.00
11) 2-Chlorophenol-d4	7.730	132	53526	27.956	ng/u1	0.00
15) 4-Methylphenol-d8	8.911	113	40118	18.697	ng/u1	0.00
21) Nitrobenzene-d5	9.375	128	36597	35.384	ng/u1	0.00
24) 2-Nitrophenol-d4	10.104	143	41284	35.385	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.650	165	65929	33.305	ng/u1	0.00
31) 4-Chloroaniline-d4	11.161	131	75205	25.964	ng/u1	0.00
46) Dimethylphthalate-d6	14.222	166	237224	36.741	ng/u1	0.00
49) Acenaphthylene-d8	14.528	160	306088	37.595	ng/u1	0.00
54) 4-Nitrophenol-d4	15.057	143	6224	5.955	ng/u1	0.00
60) Fluorene-d10	15.821	176	213491	36.718	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.950	200	33260	30.167	ng/u1	0.00
73) Anthracene-d10	17.677	188	335509	39.262	ng/u1	0.00
81) Pyrene-d10	19.957	212	379711	40.819	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.045	264	334865	41.061	ng/u1	0.00
Target Compounds						Qvalue
8) Phenol	7.389	94	3850	1.398	ng/u1	97
78) Di-n-butylphthalate	18.511	149	18184	1.640	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051232.D
Acq On : 25 Nov 2021 5:45
Operator : CG/JU
Sample : M4725-07
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
F4L13

Quant Time: Nov 25 06:37:41 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration




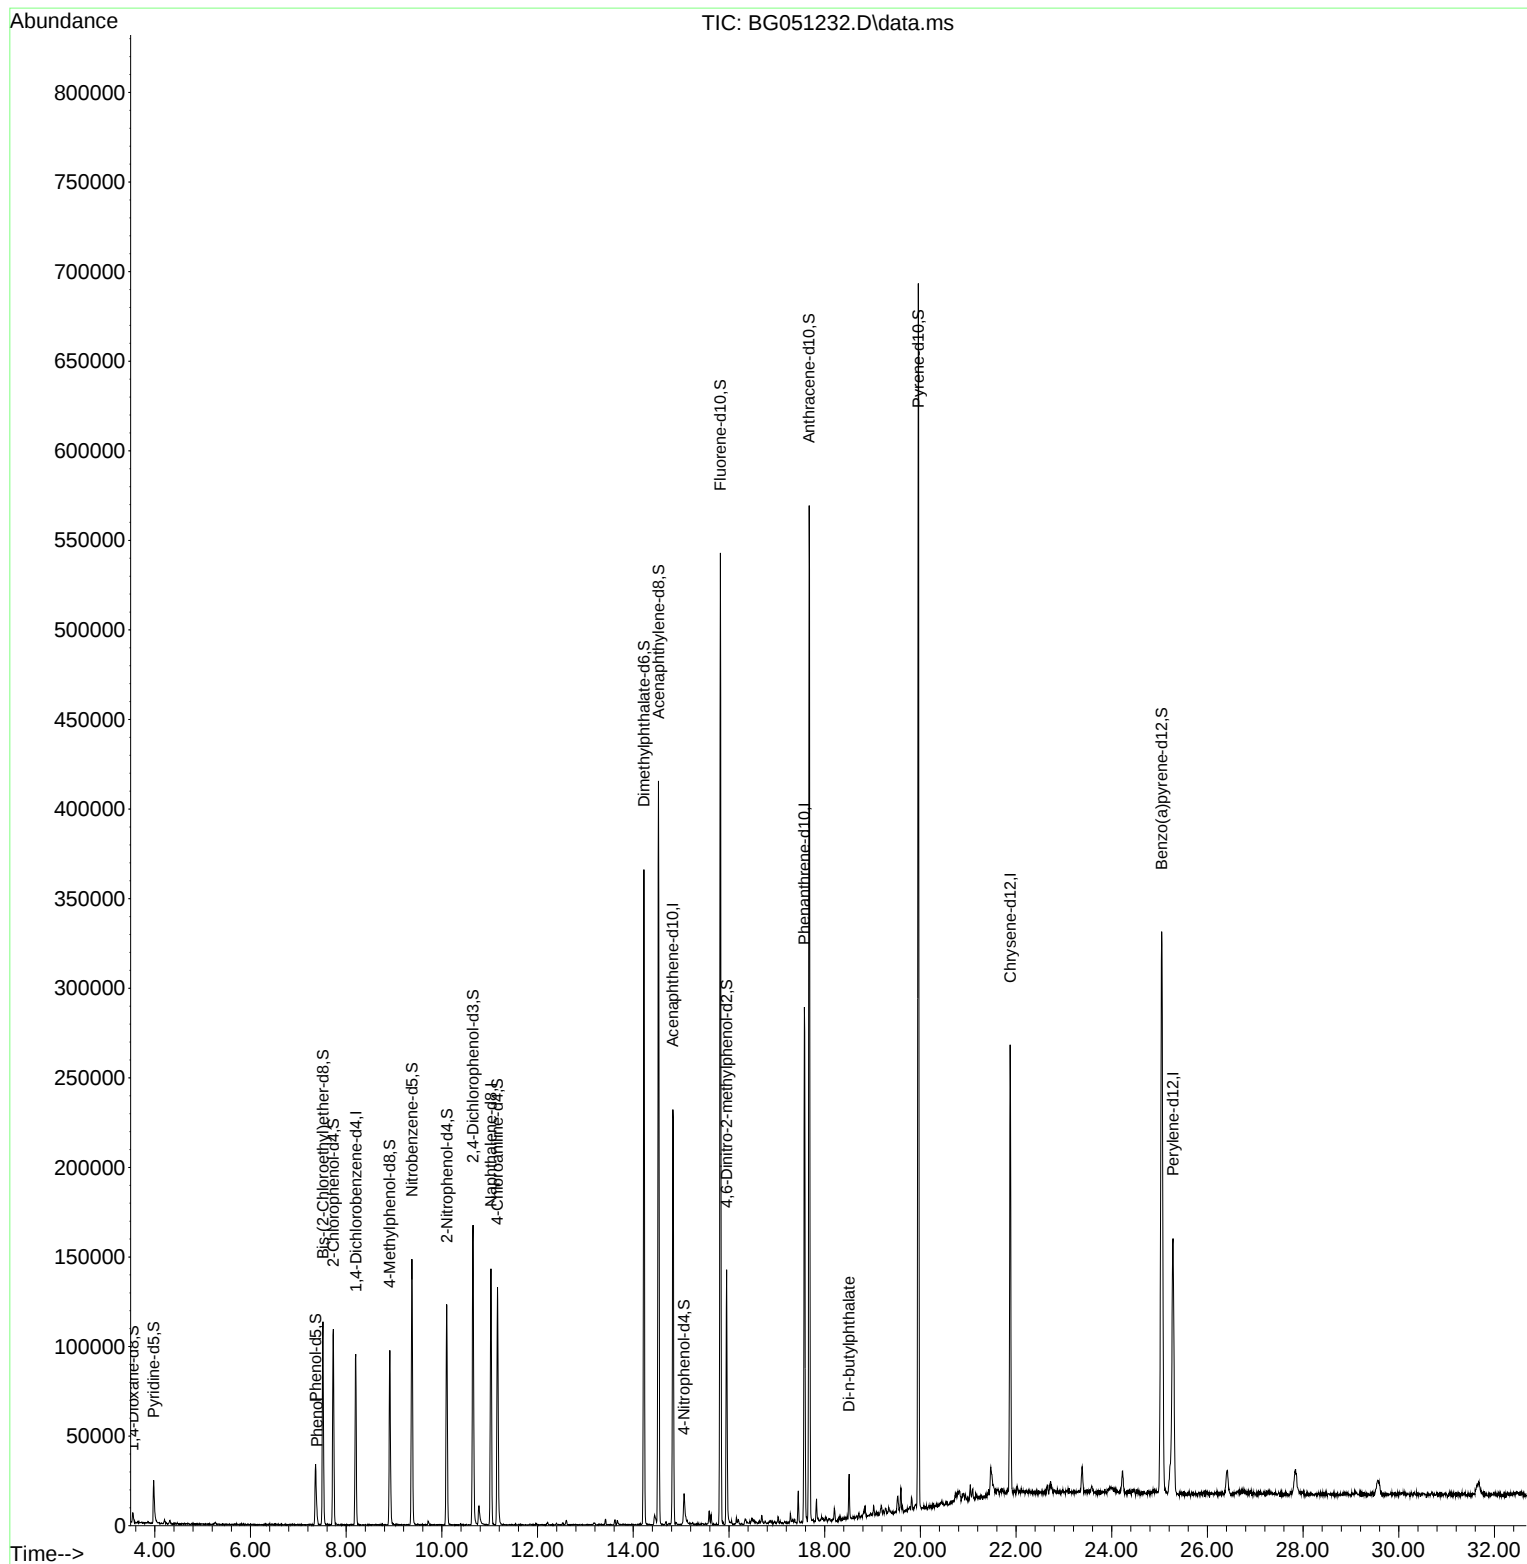


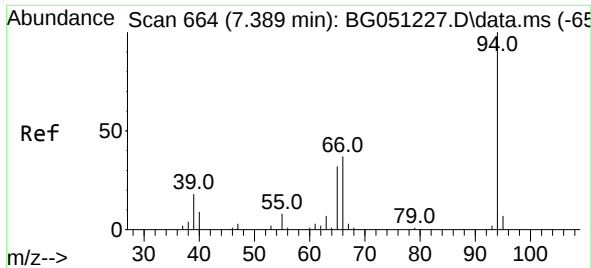

#8
Phenol
Concen: 1.398 ng/ul
RT: 7.389 min Scan# 664
Delta R.T. 0.003 min
Lab File: BG051232.D
Acq: 25 Nov 2021 5:45

Instrument :
BNA_G
ClientSampleId :
F4L13

Tgt Ion: 94	Resp:	3850
Ion Ratio	Lower	Upper
94	100	
65	28.3	25.1 37.7
66	40.5	31.6 47.4

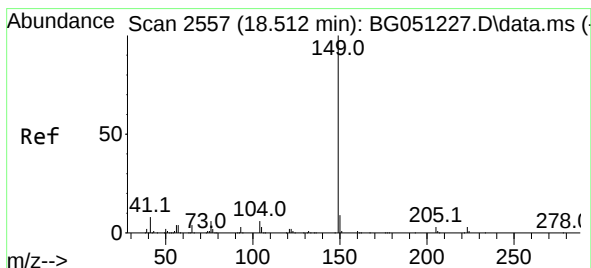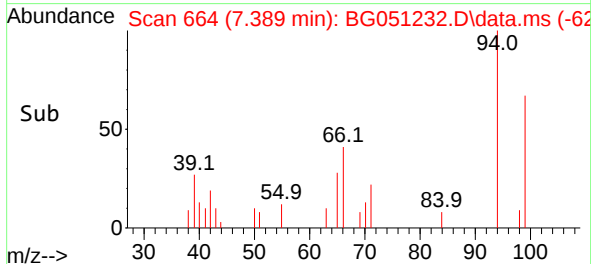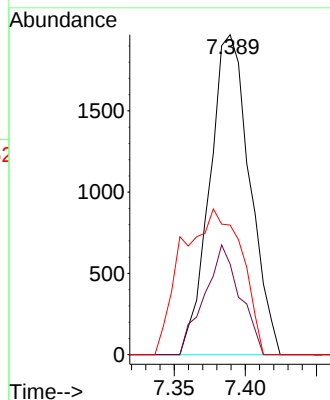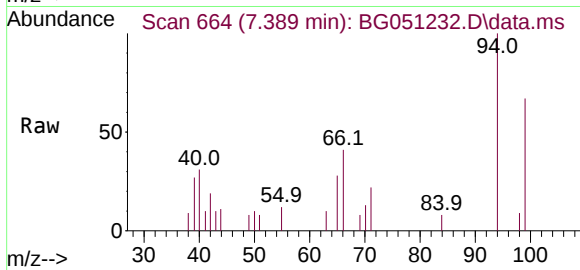

#78
Di-n-butylphthalate
Concen: 1.640 ng/ul
RT: 18.511 min Scan# 2557
Delta R.T. -0.003 min
Lab File: BG051232.D
Acq: 25 Nov 2021 5:45

Tgt Ion: 149	Resp:	18184
Ion Ratio	Lower	Upper
149	100	
150	9.9	7.5 11.3
104	6.0	5.0 7.6

