

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051237.D
 Acq On : 25 Nov 2021 9:07
 Operator : CG/JU
 Sample : M4779-03
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F4L05

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
 Supervised By :Sohil Jodhani 11/30/2021

Quant Time: Nov 26 00:38:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.196	152	27227	20.000	ng/u1	0.00
20) Naphthalene-d8	11.022	136	124574	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.830	164	85555	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.579	188	174002	20.000	ng/u1	0.00
79) Chrysene-d12	21.880	240	152939	20.000	ng/u1	0.00
88) Perylene-d12	25.282	264	151406	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.537	96	3302	4.214	ng/uL	0.00
4) Pyridine-d5	3.978	84	13411	5.833	ng/u1	0.00
7) Phenol-d5	7.362	99	20348	7.562	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.515	67	55157	32.637	ng/u1	0.00
11) 2-Chlorophenol-d4	7.732	132	49843	25.722	ng/u1	0.00
15) 4-Methylphenol-d8	8.913	113	38132	17.560	ng/u1	0.00
21) Nitrobenzene-d5	9.377	128	34643	32.944	ng/u1	0.00
24) 2-Nitrophenol-d4	10.100	143	37424	31.549	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.652	165	60098	29.860	ng/u1	0.00
31) 4-Chloroaniline-d4	11.163	131	63843	21.679	ng/u1	0.00
46) Dimethylphthalate-d6	14.224	166	226652	34.430	ng/u1	0.00
49) Acenaphthylene-d8	14.530	160	286770	34.546	ng/u1	0.00
54) 4-Nitrophenol-d4	15.065	143	6820m	6.400	ng/u1	0.02
60) Fluorene-d10	15.823	176	203425	34.316	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.952	200	30570	28.471	ng/u1	0.00
73) Anthracene-d10	17.679	188	325532	39.118	ng/u1	0.00
81) Pyrene-d10	19.959	212	359122	38.807	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.047	264	320692	39.660	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.385	94	2849	1.022	ng/u1#	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051237.D
Acq On : 25 Nov 2021 9:07
Operator : CG/JU
Sample : M4779-03
Misc :
ALS Vial : 60 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
F4L05

Quant Time: Nov 26 00:38:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/30/2021
Supervised By :Sohil Jodhani 11/30/2021

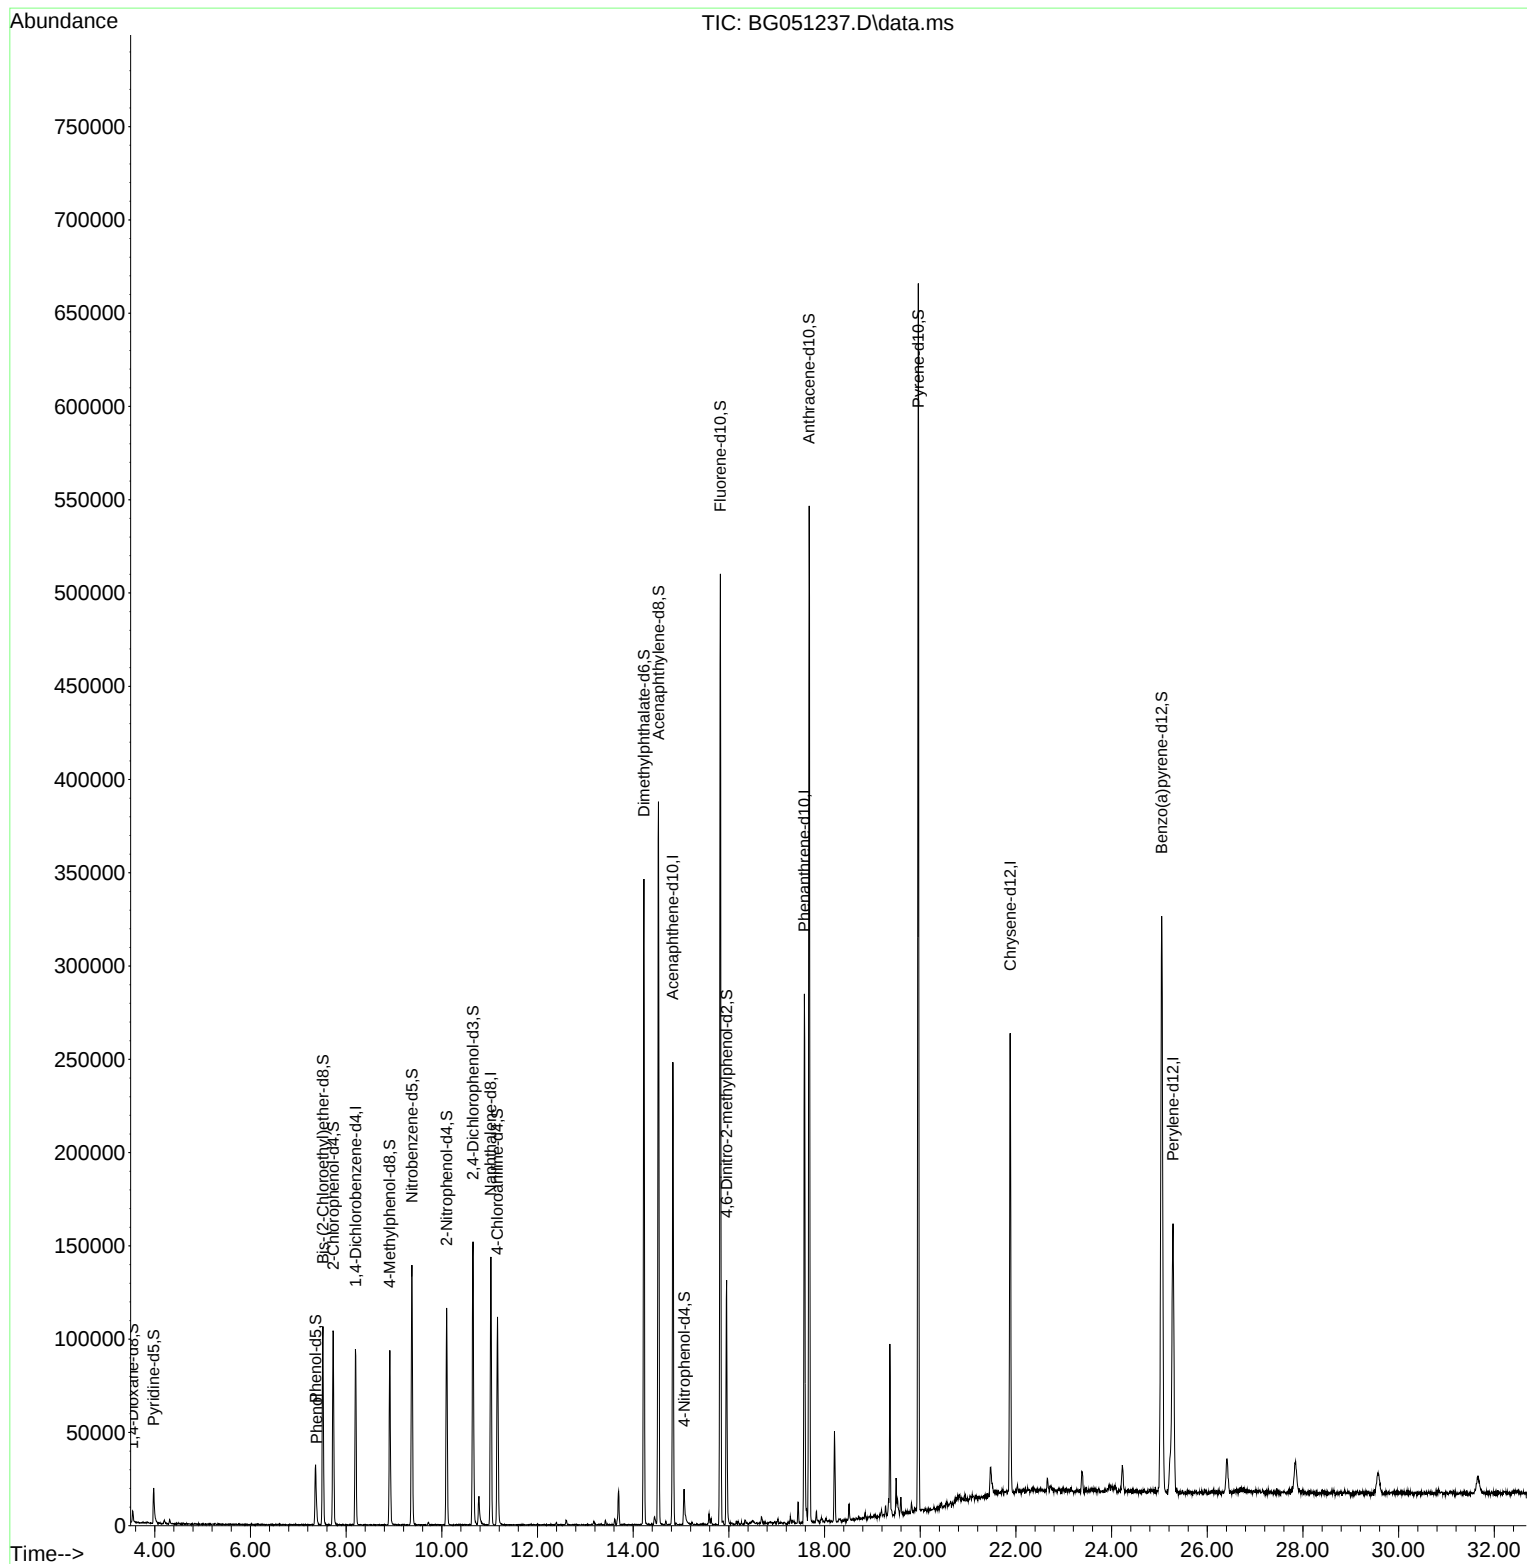

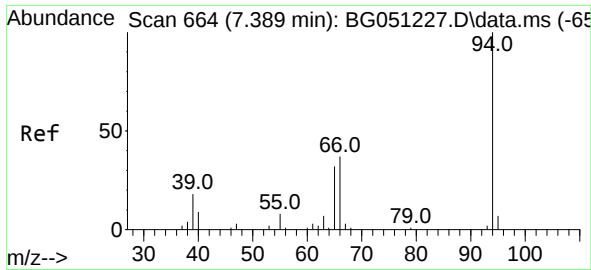

#8
Phenol
Concen: 1.022 ng/ul
RT: 7.385 min Scan# 60
Delta R.T. -0.001 min
Lab File: BG051237.D
Acq: 25 Nov 2021 9:07

Instrument :
BNA_G
ClientSampleId :
F4L05

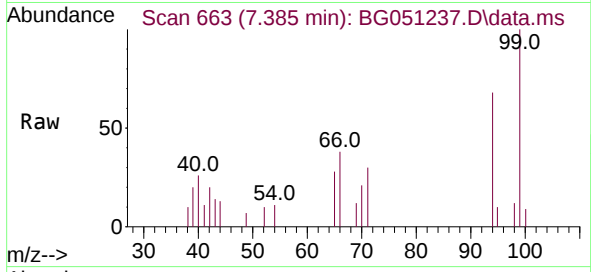

Tgt Ion: 94 Resp: 2849
Ion Ratio Lower Upper
94 100
65 41.1 25.1 37.7
66 55.5 31.6 47.4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
Supervised By :Sohil Jodhani 11/30/2021

