

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051238.D
 Acq On : 25 Nov 2021 9:48
 Operator : CG/JU
 Sample : M4779-02
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F4L04

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
 Supervised By :Sohil Jodhani 11/30/2021

Quant Time: Nov 26 00:42:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.199	152	30082	20.000	ng/u1	0.00
20) Naphthalene-d8	11.025	136	137359	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.833	164	94242	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.582	188	193354	20.000	ng/u1	0.00
79) Chrysene-d12	21.883	240	170543	20.000	ng/u1	0.00
88) Perylene-d12	25.285	264	167936	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.540	96	3477	4.017	ng/uL	0.00
4) Pyridine-d5	3.975	84	26774	10.540	ng/u1	0.00
7) Phenol-d5	7.359	99	19193	6.456	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.512	67	57835	30.973	ng/u1	0.00
11) 2-Chlorophenol-d4	7.729	132	52952	24.733	ng/u1	0.00
15) 4-Methylphenol-d8	8.910	113	38374	15.994	ng/u1	0.00
21) Nitrobenzene-d5	9.374	128	36065	31.104	ng/u1	0.00
24) 2-Nitrophenol-d4	10.103	143	42075	32.168	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.649	165	65709	29.609	ng/u1	0.00
31) 4-Chloroaniline-d4	11.166	131	81596	25.128	ng/u1	0.00
46) Dimethylphthalate-d6	14.222	166	238433	32.881	ng/u1	0.00
49) Acenaphthylene-d8	14.527	160	295386	32.304	ng/u1	0.00
54) 4-Nitrophenol-d4	15.103	143	387m	0.330	ng/u1	0.06
60) Fluorene-d10	15.820	176	205721	31.504	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.961	200	3563	2.986	ng/u1	0.00
73) Anthracene-d10	17.682	188	336443	36.382	ng/u1	0.00
81) Pyrene-d10	19.962	212	366506	35.517	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.050	264	327954	36.565	ng/u1	0.00
Target Compounds					Qvalue	
8) Phenol	7.388	94	4246	1.379	ng/u1	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051238.D
Acq On : 25 Nov 2021 9:48
Operator : CG/JU
Sample : M4779-02
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
F4L04

Quant Time: Nov 26 00:42:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/30/2021
Supervised By :Sohil Jodhani 11/30/2021

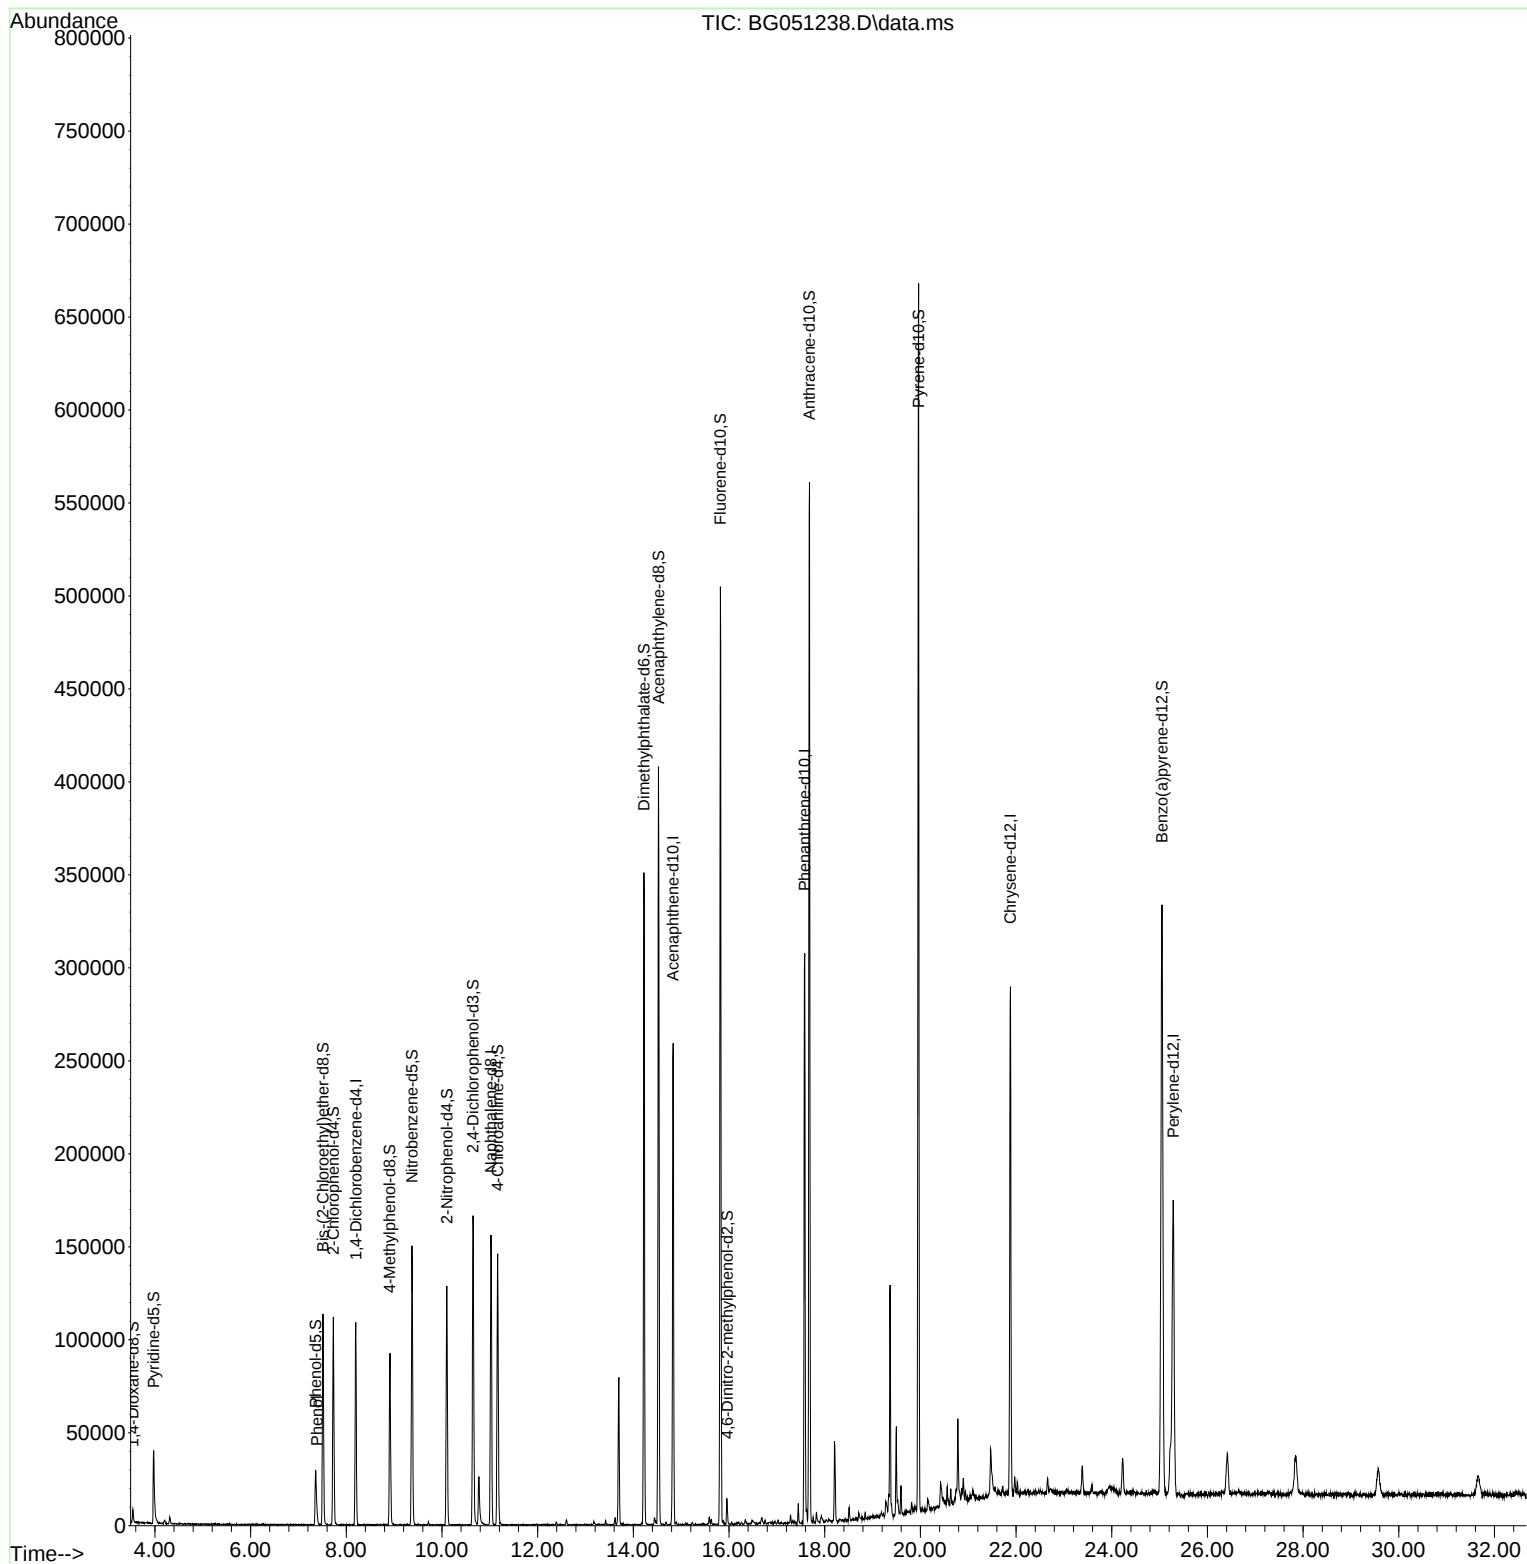

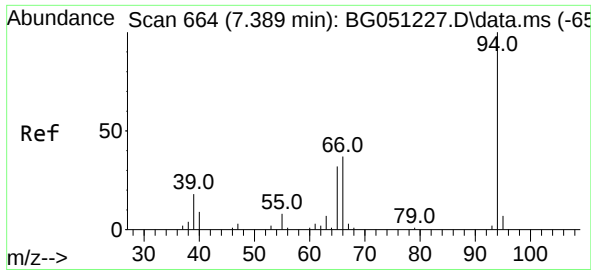

#8
Phenol
Concen: 1.379 ng/ul
RT: 7.388 min Scan# 664
Delta R.T. 0.002 min
Lab File: BG051238.D
Acq: 25 Nov 2021 9:48

Instrument :
BNA_G
ClientSampleId :
F4L04

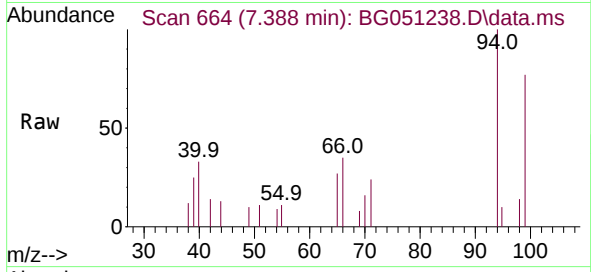

Tgt Ion: 94 Resp: 4240
Ion Ratio Lower Upper
94 100
65 27.2 25.1 37.7
66 35.1 31.6 47.4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/30/2021
Supervised By :Sohil Jodhani 11/30/2021

