

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051205.D
 Acq On : 24 Nov 2021 10:02
 Operator : CG/JU
 Sample : PB140904BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK904

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.537	4	8	19	rVB2	8595	12686	1.52%	0.145%
2	3.966	77	81	99	rVV	91572	167386	20.10%	1.909%
3	4.307	136	139	146	rVB6	1671	2489	0.30%	0.028%
4	4.771	216	218	225	rVB3	646	1283	0.15%	0.015%
5	5.359	313	318	319	rBV2	967	1076	0.13%	0.012%
6	5.523	343	346	349	rBV2	669	980	0.12%	0.011%
7	5.717	374	379	381	rBV3	664	833	0.10%	0.009%
8	5.993	423	426	428	rVB2	946	936	0.11%	0.011%
9	6.105	440	445	447	rBV3	661	937	0.11%	0.011%
10	7.227	631	636	637	rBV4	667	991	0.12%	0.011%
11	7.351	651	657	667	rBV	116196	212415	25.51%	2.422%
12	7.515	678	685	694	rVB	94043	163485	19.63%	1.864%
13	7.727	714	721	731	rBV	110862	201633	24.21%	2.299%
14	7.938	753	757	761	rBV2	561	938	0.11%	0.011%
15	8.197	794	801	809	rBV	86225	146578	17.60%	1.671%
16	8.637	873	876	882	rVB3	587	1039	0.12%	0.012%
17	8.908	915	922	940	rBV	145716	268834	32.28%	3.065%
18	9.372	994	1001	1013	rBV	117671	219314	26.33%	2.501%
19	10.100	1118	1125	1133	rBV	104953	187132	22.47%	2.134%
20	10.647	1211	1218	1230	rBV	138157	261675	31.42%	2.984%
21	11.023	1273	1282	1290	rBV	131483	240449	28.87%	2.742%
22	11.164	1297	1306	1319	rBV	142546	279261	33.53%	3.184%
23	12.374	1510	1512	1517	rVB2	738	946	0.11%	0.011%
24	12.609	1548	1552	1557	rVB	2212	3650	0.44%	0.042%
25	14.219	1820	1826	1836	rBV	296419	449366	53.96%	5.124%
26	14.525	1871	1878	1891	rVB	345827	552692	66.36%	6.302%
27	14.830	1923	1930	1937	rVB	232985	366691	44.03%	4.181%
28	15.042	1960	1966	1981	rBV	86498	181629	21.81%	2.071%
29	15.817	2091	2098	2110	rVB	442803	690180	82.87%	7.870%
30	15.946	2114	2120	2135	rBV	113621	185380	22.26%	2.114%
31	16.058	2135	2139	2142	rVB3	1387	1686	0.20%	0.019%
32	17.368	2358	2362	2365	rVB3	809	1106	0.13%	0.013%
33	17.580	2389	2398	2406	rBV	287288	455440	54.69%	5.193%
34	17.680	2408	2415	2426	rVB	472348	748421	89.87%	8.534%
35	17.797	2433	2435	2442	rVB3	645	906	0.11%	0.010%
36	18.150	2491	2495	2500	rVB3	744	1320	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051205.D
 Acq On : 24 Nov 2021 10:02
 Operator : CG/JU
 Sample : PB140904BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK904

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	19.084	2652	2654	2658	rBV2	739	876	0.11%	0.010%
38	19.219	2674	2677	2680	rVB2	961	1162	0.14%	0.013%
39	19.284	2684	2688	2690	rVB3	887	1083	0.13%	0.012%
40	19.431	2709	2713	2717	rVB2	664	881	0.11%	0.010%
41	19.489	2721	2723	2725	rBV2	1031	938	0.11%	0.011%
42	19.525	2725	2729	2732	rVB3	5842	8398	1.01%	0.096%
43	19.595	2737	2741	2745	rVV	5543	8177	0.98%	0.093%
44	19.654	2747	2751	2752	rVV2	945	959	0.12%	0.011%
45	19.666	2752	2753	2755	rVV2	1336	839	0.10%	0.010%
46	19.789	2771	2774	2776	rBV3	646	990	0.12%	0.011%
47	19.877	2787	2789	2794	rBV3	1139	1259	0.15%	0.014%
48	19.953	2796	2802	2813	rBV	566364	832807	100.00%	9.496%
49	20.065	2817	2821	2822	rBV3	934	1173	0.14%	0.013%
50	20.136	2831	2833	2835	rBV3	1318	1201	0.14%	0.014%
51	20.230	2845	2849	2850	rBV3	1122	1074	0.13%	0.012%
52	20.247	2850	2852	2856	rVV3	861	1027	0.12%	0.012%
53	20.288	2856	2859	2860	rVB2	1319	1145	0.14%	0.013%
54	20.406	2877	2879	2881	rBV2	1488	1277	0.15%	0.015%
55	20.576	2907	2908	2911	rBV2	1343	1620	0.19%	0.018%
56	20.664	2921	2923	2925	rBV3	1277	1266	0.15%	0.014%
57	20.700	2927	2929	2930	rBV2	913	844	0.10%	0.010%
58	20.717	2930	2932	2933	rBV	1409	843	0.10%	0.010%
59	20.941	2969	2970	2971	rBV	2201	1015	0.12%	0.012%
60	21.134	3001	3003	3005	rBV3	2560	2223	0.27%	0.025%
61	21.193	3011	3013	3015	rBV3	1476	1308	0.16%	0.015%
62	21.434	3052	3054	3056	rBV3	1565	1320	0.16%	0.015%
63	21.616	3083	3085	3087	rBV3	1627	1394	0.17%	0.016%
64	21.693	3096	3098	3100	rBV3	1576	1322	0.16%	0.015%
65	21.751	3106	3108	3111	rBV3	2096	2698	0.32%	0.031%
66	21.875	3122	3129	3137	rBV	261360	445405	53.48%	5.079%
67	22.404	3217	3219	3220	rBV2	1746	1215	0.15%	0.014%
68	22.451	3226	3227	3229	rBV2	2830	1836	0.22%	0.021%
69	22.656	3259	3262	3265	rVB4	3751	4980	0.60%	0.057%
70	23.032	3324	3326	3327	rBV2	2012	1439	0.17%	0.016%
71	23.379	3380	3385	3390	rVB5	7768	12993	1.56%	0.148%
72	24.219	3523	3528	3536	rVB4	10655	21078	2.53%	0.240%
73	24.542	3581	3583	3586	rVB4	2833	3070	0.37%	0.035%
74	25.036	3656	3667	3681	rVB2	263026	771279	92.61%	8.795%
75	25.265	3691	3706	3721	rVB2	146154	484534	58.18%	5.525%
76	25.423	3731	3733	3734	rVB2	2258	1390	0.17%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051205.D
 Acq On : 24 Nov 2021 10:02
 Operator : CG/JU
 Sample : PB140904BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK904

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

77	25.435	3734	3735	3739	rBV4	2090	3139	0.38%	0.036%
78	26.405	3893	3900	3908	rVB2	14797	39811	4.78%	0.454%
79	27.832	4133	4143	4154	rVB6	14579	47842	5.74%	0.546%
80	28.479	4251	4253	4254	rBV2	1913	1405	0.17%	0.016%
81	29.566	4430	4438	4446	rVB10	8612	28837	3.46%	0.329%
82	30.776	4642	4644	4647	rBV4	1925	1807	0.22%	0.021%
83	31.334	4737	4739	4740	rBV	2051	1497	0.18%	0.017%
84	31.563	4776	4778	4779	rBV2	1911	1171	0.14%	0.013%
85	31.887	4831	4833	4837	rVB5	2267	2190	0.26%	0.025%




Sum of corrected areas: 8769800

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051205.D
Acq On : 24 Nov 2021 10:02
Operator : CG/JU
Sample : PB140904BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK904

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

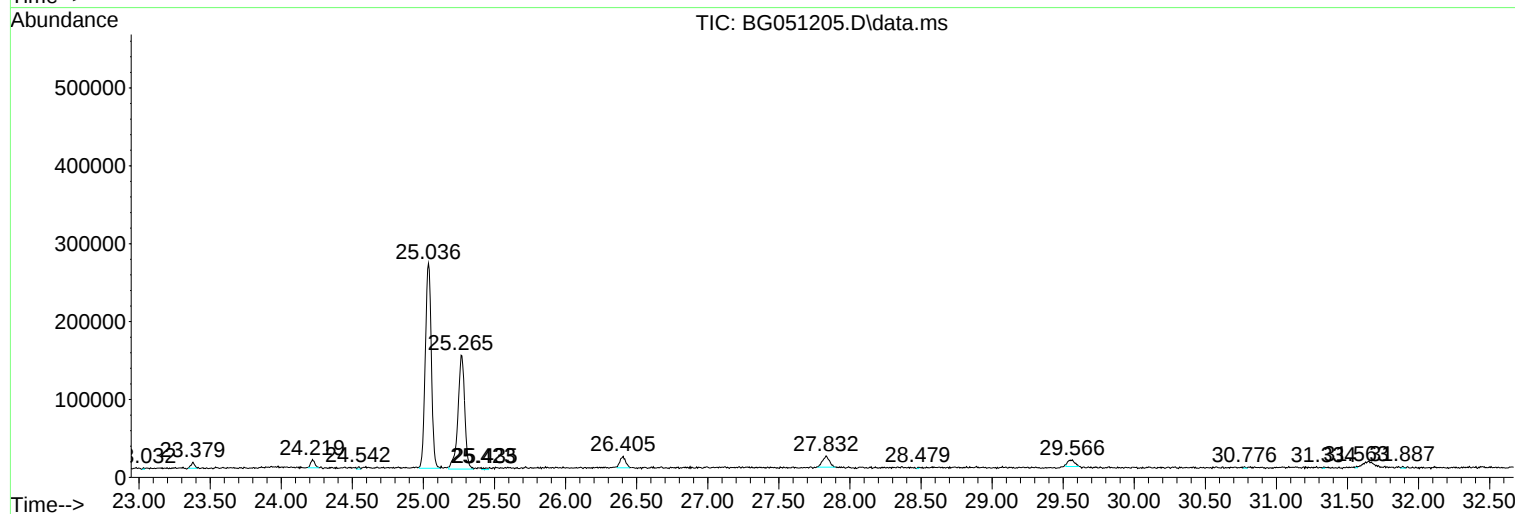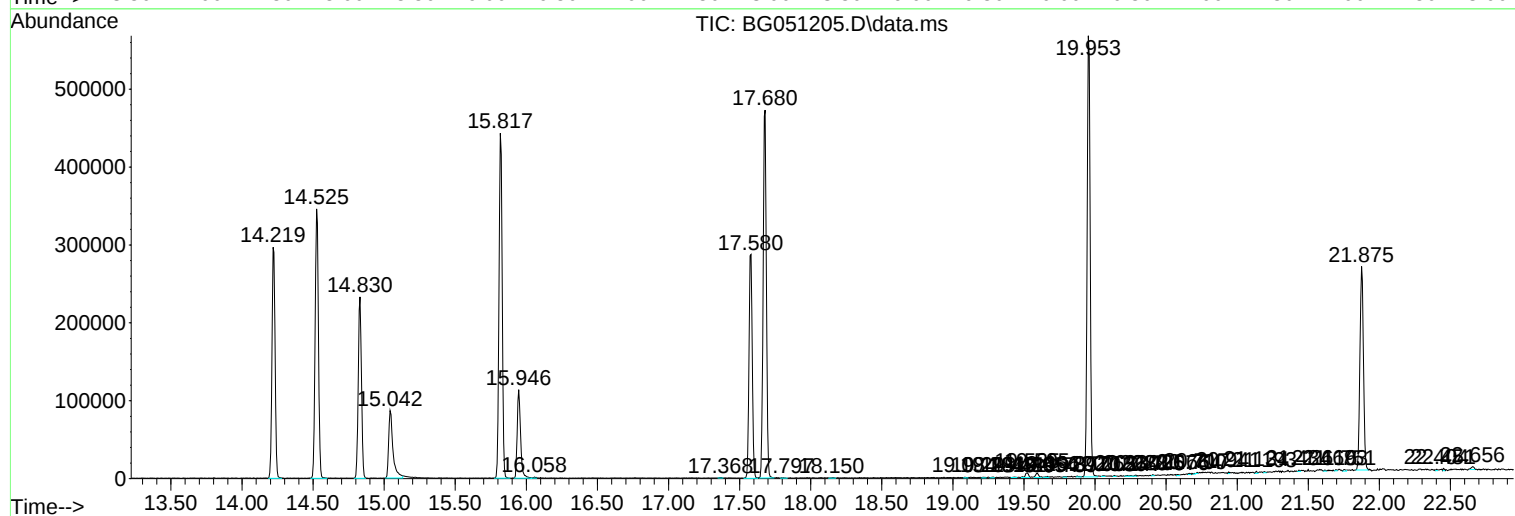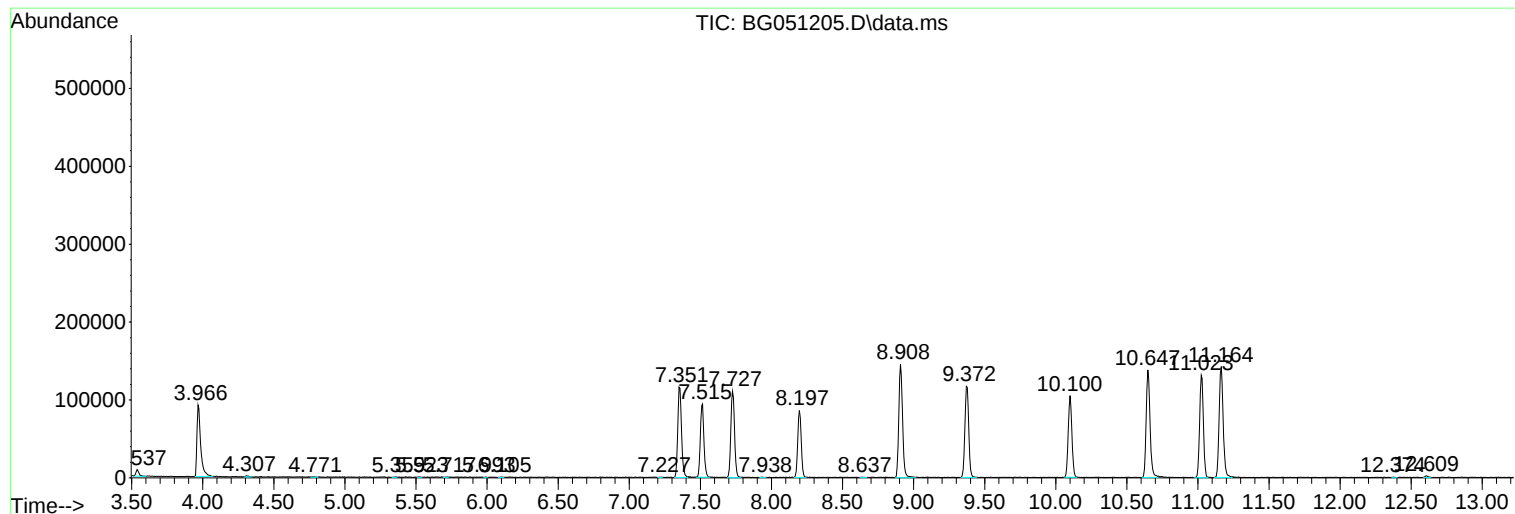

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051205.D
Acq On : 24 Nov 2021 10:02
Operator : CG/JU
Sample : PB140904BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK904

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051205.D
Acq On : 24 Nov 2021 10:02
Operator : CG/JU
Sample : PB140904BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK904

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc