

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051214.D
 Acq On : 24 Nov 2021 16:11
 Operator : CG/JU
 Sample : PB140870BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK870

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.544	4	9	16	rVB	8125	12853	1.60%	0.151%
2	3.967	77	81	95	rBV	98346	178394	22.18%	2.094%
3	4.055	95	96	100	rVB3	1639	1238	0.15%	0.015%
4	4.302	137	138	140	rBV	1324	1253	0.16%	0.015%
5	4.666	198	200	204	rVB2	687	826	0.10%	0.010%
6	5.089	270	272	277	rVB3	721	900	0.11%	0.011%
7	5.271	300	303	305	rVB2	702	823	0.10%	0.010%
8	5.312	305	310	312	rBV2	558	1058	0.13%	0.012%
9	6.305	475	479	481	rBV	605	847	0.11%	0.010%
10	6.341	483	485	488	rVB2	715	818	0.10%	0.010%
11	6.981	589	594	599	rVV3	421	923	0.11%	0.011%
12	7.351	650	657	670	rVV	116110	218368	27.15%	2.564%
13	7.510	677	684	693	rBV	94107	163516	20.33%	1.920%
14	7.727	714	721	730	rBV	119516	210428	26.16%	2.470%
15	8.197	792	801	809	rVB	95226	165380	20.56%	1.942%
16	8.855	910	913	915	rVV	615	910	0.11%	0.011%
17	8.908	915	922	932	rVV	145994	263519	32.76%	3.094%
18	8.996	936	937	942	rVB2	959	1252	0.16%	0.015%
19	9.372	993	1001	1010	rBV	121471	216075	26.87%	2.537%
20	10.101	1118	1125	1132	rBV	99871	185088	23.01%	2.173%
21	10.647	1212	1218	1231	rBV	133761	256141	31.85%	3.007%
22	11.023	1273	1282	1291	rBV	143547	252953	31.45%	2.970%
23	11.164	1298	1306	1320	rBV	137492	271165	33.71%	3.183%
24	12.610	1547	1552	1557	rVB2	1867	3624	0.45%	0.043%
25	13.009	1616	1620	1623	rBV3	474	812	0.10%	0.010%
26	14.220	1819	1826	1835	rBV	279670	427306	53.13%	5.017%
27	14.525	1871	1878	1888	rBV	331680	523398	65.08%	6.145%
28	14.831	1922	1930	1937	rBB	234508	367816	45.73%	4.318%
29	15.042	1960	1966	1981	rBV2	80010	166933	20.76%	1.960%
30	15.818	2091	2098	2108	rVB	420144	647147	80.46%	7.597%
31	15.947	2115	2120	2131	rBV	109101	175680	21.84%	2.062%
32	16.053	2136	2138	2140	rBV	1276	1338	0.17%	0.016%
33	17.357	2358	2360	2365	rBV	888	1171	0.15%	0.014%
34	17.574	2391	2397	2407	rBV	292129	453187	56.35%	5.320%
35	17.674	2407	2414	2423	rBV2	465009	703883	87.52%	8.264%
36	18.203	2499	2504	2507	rBV2	531	1056	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051214.D
 Acq On : 24 Nov 2021 16:11
 Operator : CG/JU
 Sample : PB140870BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK870

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	18.938	2626	2629	2634	rVB2	566	921	0.11%	0.011%
38	18.990	2634	2638	2640	rBV3	626	921	0.11%	0.011%
39	19.037	2642	2646	2648	rBV3	695	1043	0.13%	0.012%
40	19.137	2659	2663	2667	rBV3	613	985	0.12%	0.012%

41	19.525	2722	2729	2734	rBV3	5561	8293	1.03%	0.097%
42	19.596	2734	2741	2746	rBV2	5337	8828	1.10%	0.104%
43	19.678	2751	2755	2758	rVB3	891	882	0.11%	0.010%
44	19.731	2762	2764	2766	rBV2	1013	1135	0.14%	0.013%
45	19.836	2780	2782	2786	rVB4	1088	1175	0.15%	0.014%

46	19.954	2794	2802	2813	rVV	563019	804296	100.00%	9.442%
47	20.030	2813	2815	2817	rVV3	1267	949	0.12%	0.011%
48	20.071	2820	2822	2826	rBV3	764	859	0.11%	0.010%
49	20.118	2826	2830	2831	rBV3	1430	1426	0.18%	0.017%
50	20.248	2848	2852	2854	rBV4	1243	2019	0.25%	0.024%

51	20.289	2857	2859	2861	rBV2	1054	894	0.11%	0.010%
52	20.412	2878	2880	2881	rVB2	1569	1059	0.13%	0.012%
53	20.430	2881	2883	2885	rBV2	1270	1541	0.19%	0.018%
54	20.518	2897	2898	2900	rBV2	1184	1024	0.13%	0.012%
55	20.618	2913	2915	2917	rBV3	1142	1243	0.15%	0.015%

56	20.671	2922	2924	2925	rBV	1472	1494	0.19%	0.018%
57	20.730	2927	2934	2935	rBV5	7156	11613	1.44%	0.136%
58	20.935	2966	2969	2971	rBV4	1919	2276	0.28%	0.027%
59	20.982	2974	2977	2979	rBV4	1298	1565	0.19%	0.018%
60	21.188	3010	3012	3014	rBV3	1482	1155	0.14%	0.014%

61	21.299	3030	3031	3034	rBV3	1453	1642	0.20%	0.019%
62	21.452	3055	3057	3058	rBV2	1549	829	0.10%	0.010%
63	21.581	3074	3079	3081	rBV4	2749	4777	0.59%	0.056%
64	21.875	3122	3129	3137	rVB	262421	457813	56.92%	5.375%
65	22.222	3187	3188	3193	rBV5	2978	3659	0.45%	0.043%

66	22.263	3193	3195	3199	rVV5	2604	2912	0.36%	0.034%
67	23.379	3380	3385	3390	rVB6	4183	8039	1.00%	0.094%
68	23.703	3438	3440	3442	rBV3	1938	1142	0.14%	0.013%
69	23.844	3462	3464	3466	rBV3	1874	1887	0.23%	0.022%
70	24.220	3522	3528	3535	rBV7	6700	15779	1.96%	0.185%

71	24.854	3633	3636	3638	rBV4	2634	2792	0.35%	0.033%
72	25.036	3655	3667	3680	rVB2	254869	743173	92.40%	8.725%
73	25.148	3682	3686	3690	rBV6	1947	3206	0.40%	0.038%
74	25.265	3692	3706	3721	rVB2	151960	473439	58.86%	5.558%
75	25.465	3738	3740	3741	rBV2	2135	1629	0.20%	0.019%

76	25.506	3745	3747	3748	rBV2	1933	1094	0.14%	0.013%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051214.D
 Acq On : 24 Nov 2021 16:11
 Operator : CG/JU
 Sample : PB140870BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK870

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

77	25.912	3814	3816	3820	rBV4	1779	2530	0.31%	0.030%
78	26.158	3856	3858	3859	rBV	1776	1024	0.13%	0.012%
79	26.299	3880	3882	3884	rBV3	1633	1131	0.14%	0.013%
80	26.405	3891	3900	3909	rBV6	9903	29814	3.71%	0.350%
81	27.304	4050	4053	4054	rBV2	2413	2760	0.34%	0.032%
82	28.397	4237	4239	4241	rBV3	1781	1674	0.21%	0.020%
83	28.738	4295	4297	4300	rBV4	1852	1705	0.21%	0.020%
84	29.408	4409	4411	4414	rBV4	2104	2880	0.36%	0.034%
85	29.490	4421	4425	4426	rBV4	2342	3128	0.39%	0.037%
86	30.354	4570	4572	4573	rBV	2296	1381	0.17%	0.016%
87	30.495	4592	4596	4599	rBV5	1894	2733	0.34%	0.032%
88	30.706	4630	4632	4633	rBV2	1643	1111	0.14%	0.013%
89	30.876	4658	4661	4662	rBV3	2113	2667	0.33%	0.031%
90	31.605	4781	4785	4786	rBV3	3338	3950	0.49%	0.046%




Sum of corrected areas: 8517975

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051214.D
Acq On : 24 Nov 2021 16:11
Operator : CG/JU
Sample : PB140870BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK870

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

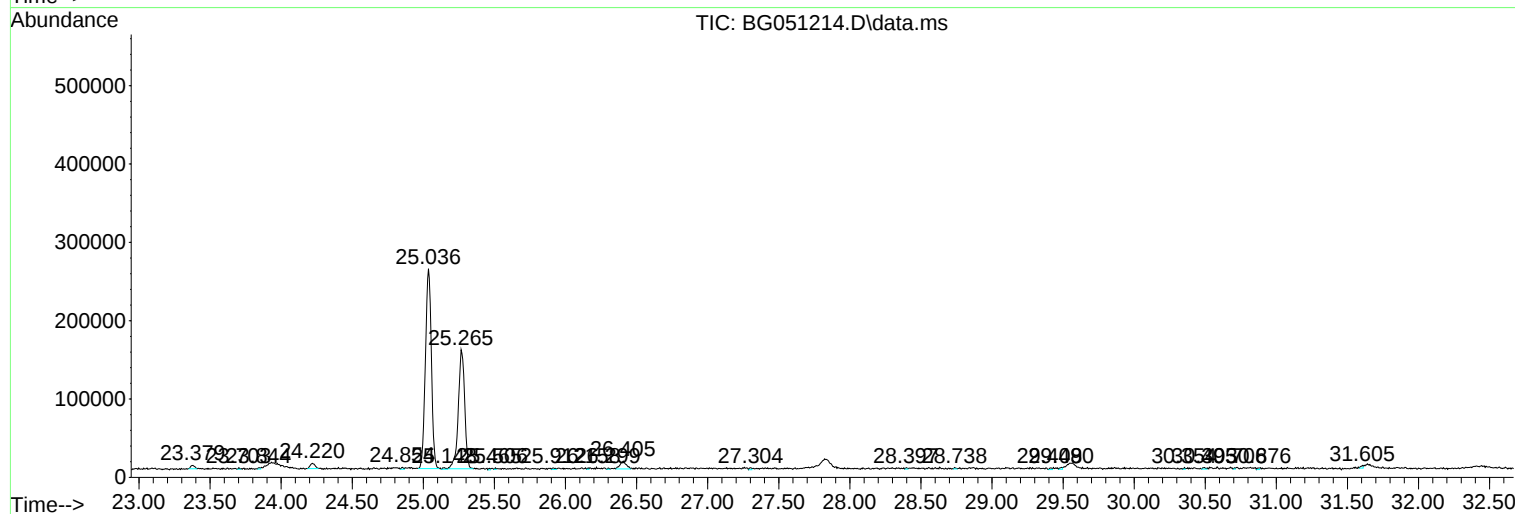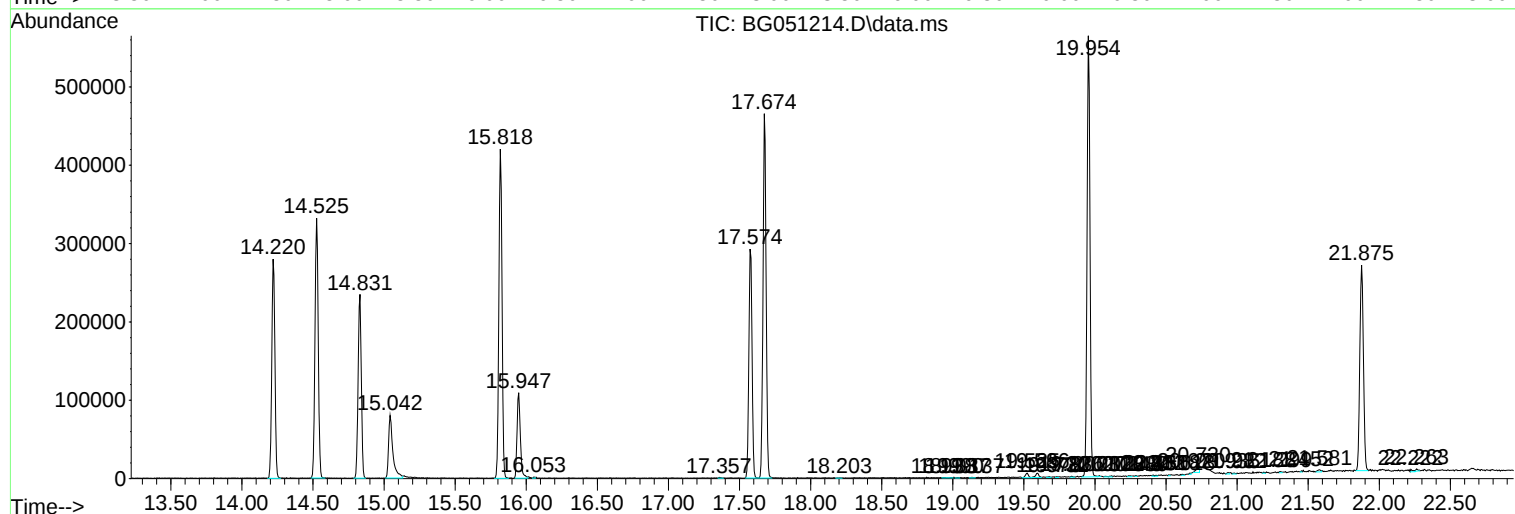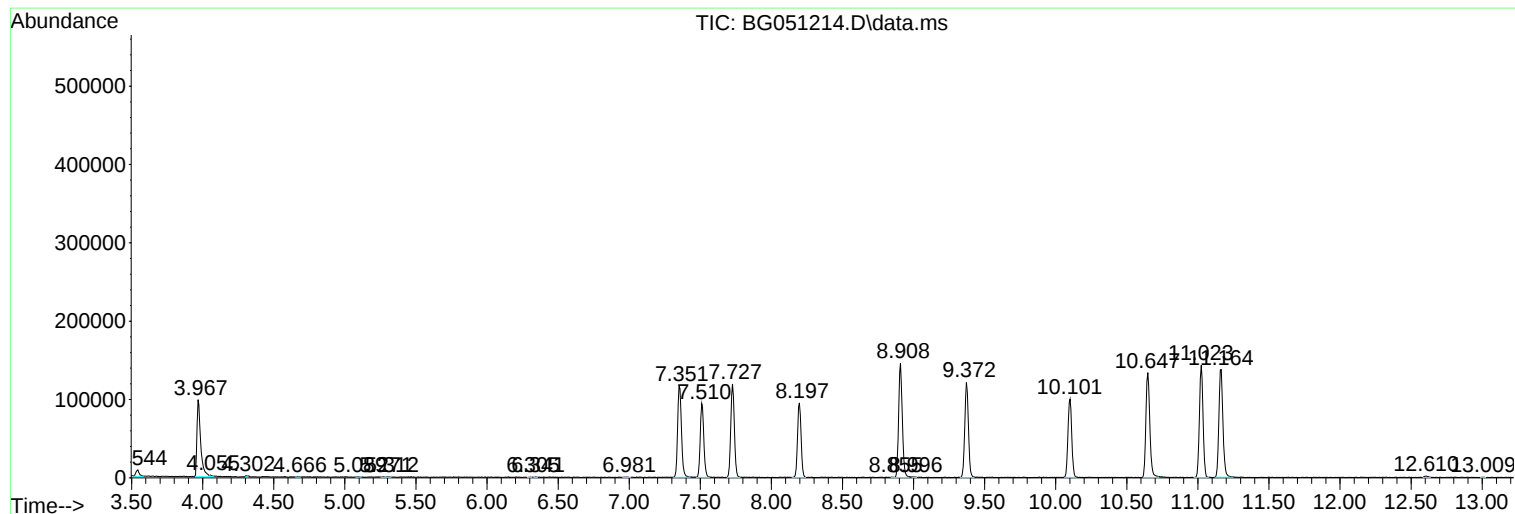

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051214.D
Acq On : 24 Nov 2021 16:11
Operator : CG/JU
Sample : PB140870BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK870

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051214.D
Acq On : 24 Nov 2021 16:11
Operator : CG/JU
Sample : PB140870BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK870

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc