

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051241.D
 Acq On : 25 Nov 2021 12:32
 Operator : CG/JU
 Sample : PB140983BL
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK983

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.541	5	9	18	rVB	10002	14744	1.65%	0.150%
2	3.970	77	82	102	rVB	106994	196235	21.92%	1.997%
3	4.310	135	140	151	rVB	13063	22224	2.48%	0.226%
4	4.804	220	224	225	rBV	629	920	0.10%	0.009%
5	5.762	384	387	390	rBV2	605	981	0.11%	0.010%
6	5.814	392	396	400	rVB2	549	986	0.11%	0.010%
7	6.249	467	470	473	rBV	565	958	0.11%	0.010%
8	7.089	612	613	618	rVB3	704	1022	0.11%	0.010%
9	7.360	652	659	672	rBV	151183	273096	30.51%	2.779%
10	7.512	677	685	693	rVV	115895	197942	22.11%	2.014%
11	7.730	715	722	731	rBV	146306	258447	28.87%	2.630%
12	8.200	793	802	814	rBV	109237	191447	21.39%	1.948%
13	8.911	916	923	936	rBV	185009	334682	37.39%	3.406%
14	9.375	995	1002	1012	rBV	146122	267002	29.83%	2.717%
15	10.104	1118	1126	1138	rVB	132085	238292	26.62%	2.425%
16	10.650	1212	1219	1231	rBV	178941	334640	37.38%	3.405%
17	11.026	1274	1283	1295	rBV	166813	302950	33.84%	3.083%
18	11.167	1299	1307	1317	rVV	179318	340250	38.01%	3.463%
19	11.249	1319	1321	1326	rVV3	914	1599	0.18%	0.016%
20	11.314	1329	1332	1336	rVB2	577	1010	0.11%	0.010%
21	12.606	1544	1552	1557	rBV3	3034	5431	0.61%	0.055%
22	14.222	1821	1827	1835	rBV	329942	506021	56.53%	5.149%
23	14.528	1871	1879	1892	rBV	390585	640234	71.52%	6.515%
24	14.833	1924	1931	1939	rBV	272537	434358	48.52%	4.420%
25	15.051	1961	1968	1987	rBV	91759	198116	22.13%	2.016%
26	15.820	2092	2099	2107	rBV	499843	774360	86.51%	7.880%
27	15.950	2116	2121	2136	rVV	114611	180582	20.17%	1.838%
28	16.061	2136	2140	2143	rVB2	1743	2484	0.28%	0.025%
29	17.583	2392	2399	2407	rBV	316193	503939	56.30%	5.128%
30	17.683	2409	2416	2428	rVB	518966	800673	89.45%	8.148%
31	18.411	2536	2540	2543	rVB2	682	987	0.11%	0.010%
32	19.522	2725	2729	2734	rBV3	5825	8801	0.98%	0.090%
33	19.592	2737	2741	2746	rBV2	6213	9207	1.03%	0.094%
34	19.663	2750	2753	2756	rBV3	889	1041	0.12%	0.011%
35	19.769	2768	2771	2772	rBV3	954	989	0.11%	0.010%
36	19.957	2797	2803	2812	rBV	586944	895123	100.00%	9.109%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
 Data File : BG051241.D
 Acq On : 25 Nov 2021 12:32
 Operator : CG/JU
 Sample : PB140983BL
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK983

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	20.227	2847	2849	2852	rVV2	1199	1549	0.17%	0.016%
38	20.274	2855	2857	2861	rVB3	1391	1432	0.16%	0.015%
39	20.333	2861	2867	2870	rBV4	1683	2743	0.31%	0.028%
40	20.738	2930	2936	2939	rBV6	10032	21552	2.41%	0.219%
41	21.044	2983	2988	2991	rBV6	1651	3243	0.36%	0.033%
42	21.091	2995	2996	2999	rVB3	2209	1763	0.20%	0.018%
43	21.243	3020	3022	3023	rBV2	1862	1154	0.13%	0.012%
44	21.572	3076	3078	3082	rVB4	2218	2497	0.28%	0.025%
45	21.614	3084	3085	3086	rBV	2570	992	0.11%	0.010%
46	21.784	3112	3114	3117	rBV3	1925	2337	0.26%	0.024%
47	21.884	3124	3131	3139	rVB2	280662	495761	55.38%	5.045%
48	22.994	3318	3320	3322	rBV3	2284	1015	0.11%	0.010%
49	23.306	3371	3373	3376	rBV4	2139	2311	0.26%	0.024%
50	23.376	3382	3385	3387	rBV3	6138	8290	0.93%	0.084%
51	24.551	3584	3585	3586	rVB	2789	983	0.11%	0.010%
52	25.051	3658	3670	3685	rBV2	279725	819570	91.56%	8.340%
53	25.286	3697	3710	3723	rVB3	163632	510728	57.06%	5.197%
54	26.161	3857	3859	3860	rBV2	2286	930	0.10%	0.009%
55	26.984	3997	3999	4000	rBV2	2232	1519	0.17%	0.015%
56	27.654	4111	4113	4115	rBV3	2483	1759	0.20%	0.018%
57	31.079	4694	4696	4697	rBV2	2383	1141	0.13%	0.012%
58	31.572	4778	4780	4781	rBV2	2123	1609	0.18%	0.016%




Sum of corrected areas: 9826651

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051241.D
Acq On : 25 Nov 2021 12:32
Operator : CG/JU
Sample : PB140983BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK983

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

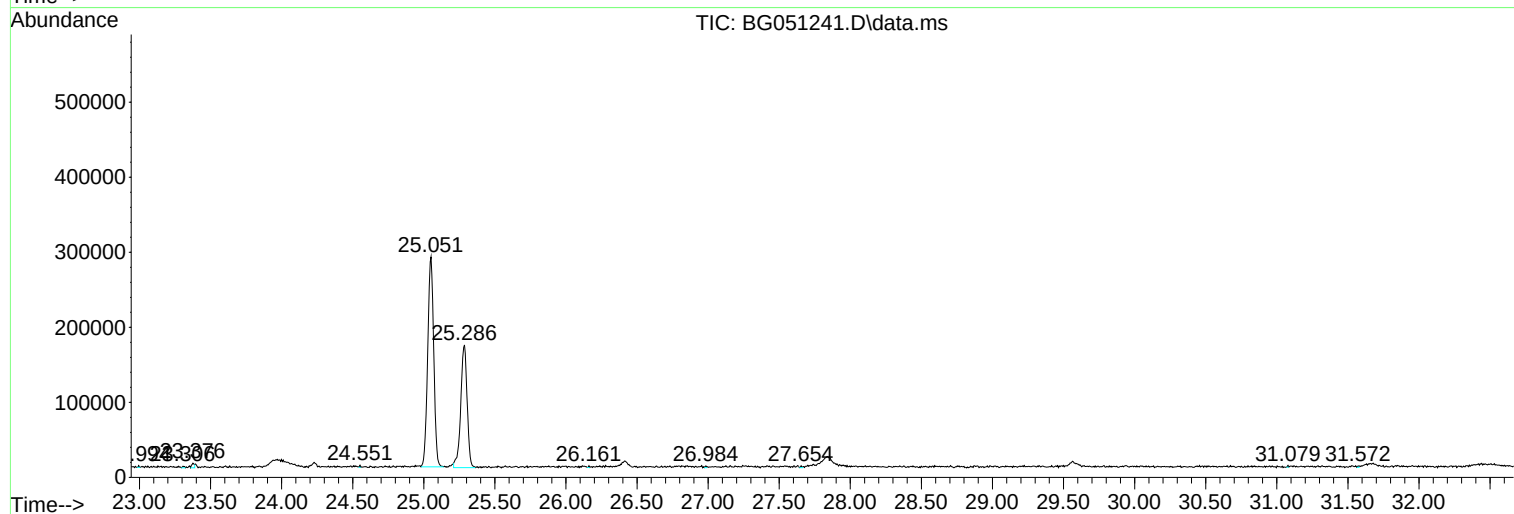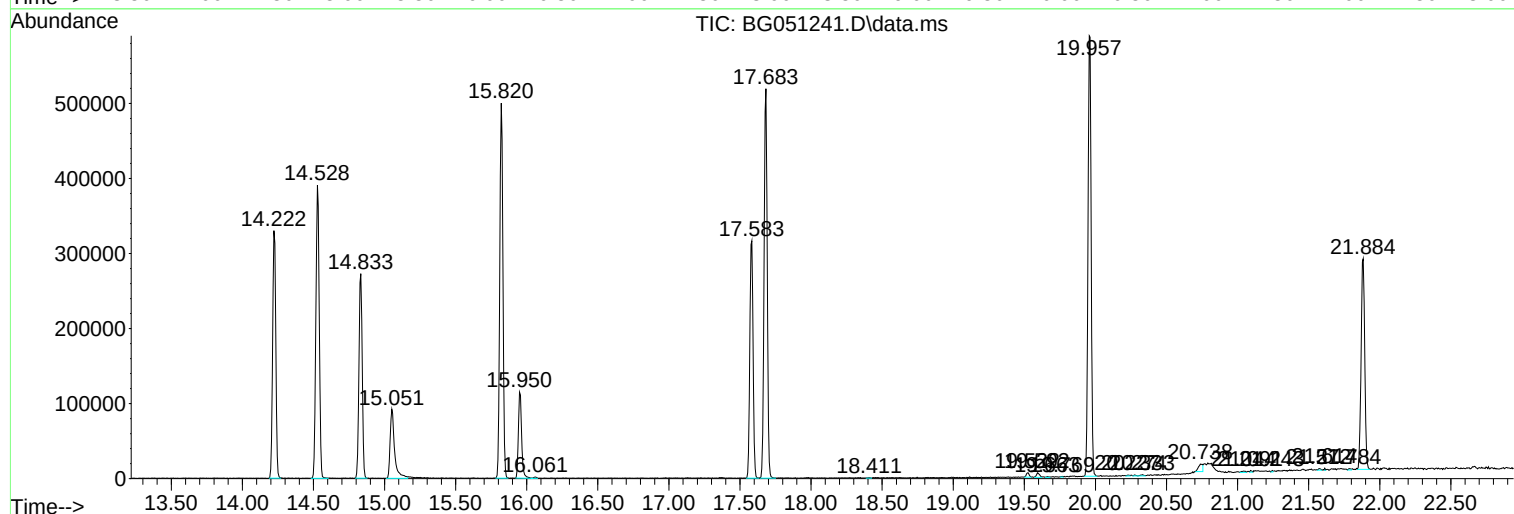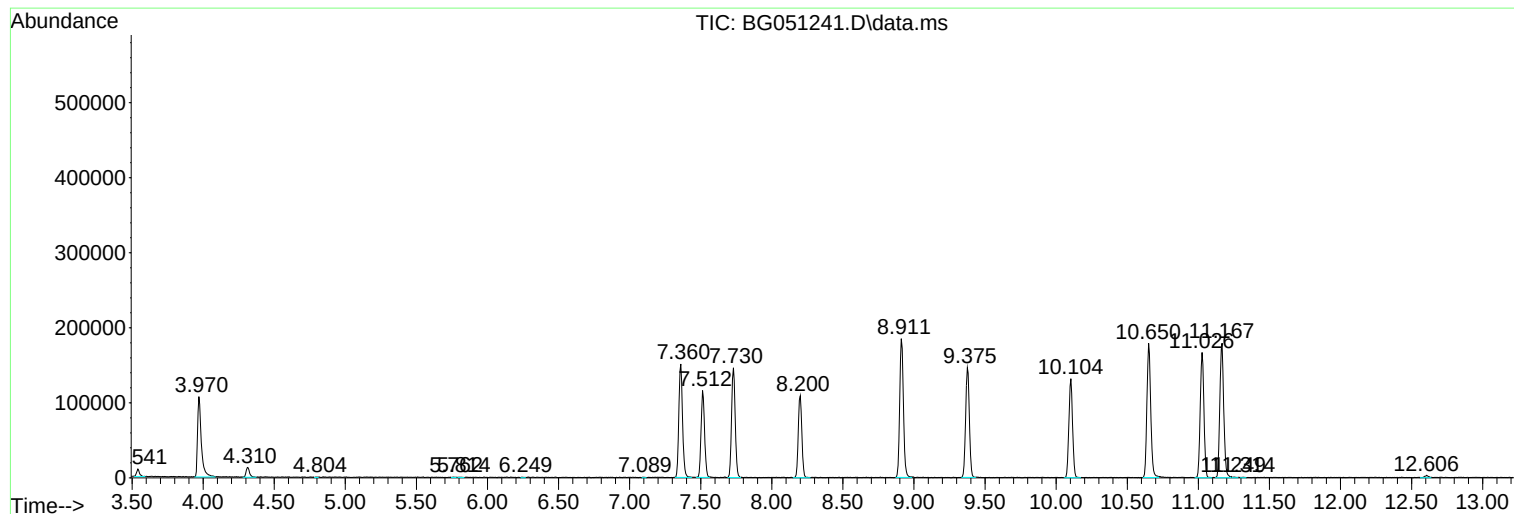

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051241.D
Acq On : 25 Nov 2021 12:32
Operator : CG/JU
Sample : PB140983BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK983










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Spiro[2,4]hepta-4,6-diene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.310	2.32 ng/ul	22224	1,4-Dichlorobenzene-d4	8.200

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Toluene	92	C7H8	000108-88-3	86
2			Toluene	92	C7H8	000108-88-3	80
3			Spiro[2,4]hepta-4,6-diene	92	C7H8	000765-46-8	80
4			Toluene	92	C7H8	000108-88-3	80
5			1,3,5-Cycloheptatriene	92	C7H8	000544-25-2	80

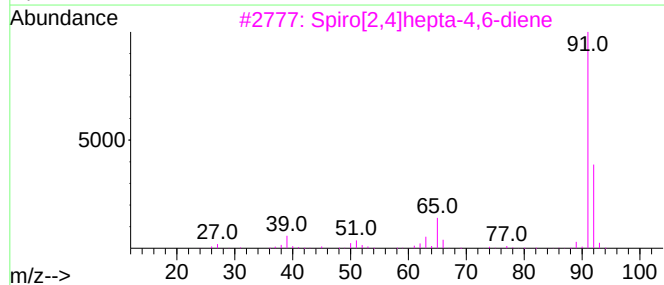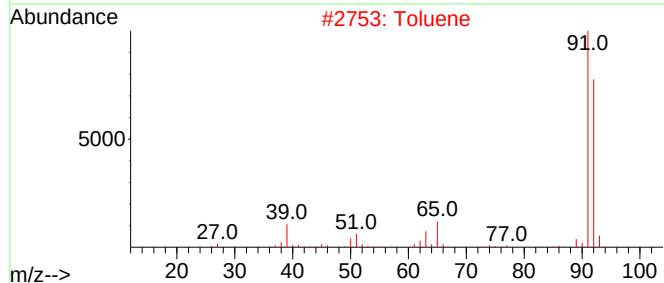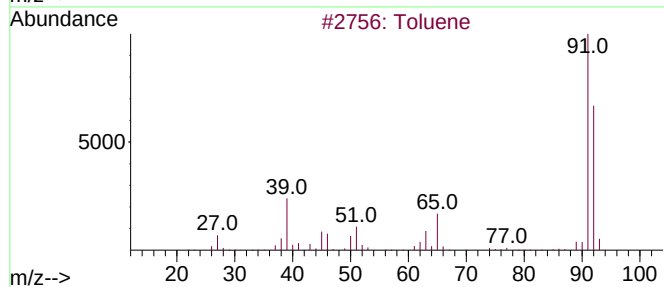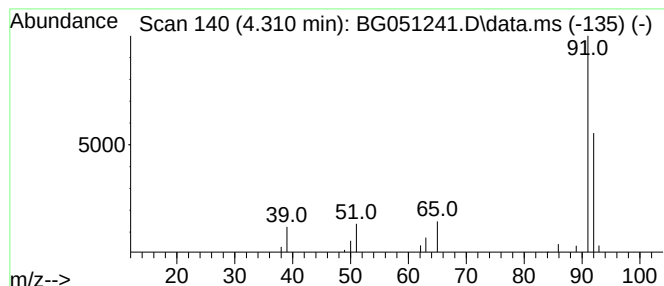

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112321\
Data File : BG051241.D
Acq On : 25 Nov 2021 12:32
Operator : CG/JU
Sample : PB140983BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK983

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Spiro[2,4]hepta...	4.310	2.3	ng/u1	22224	1	8.200	191447	20.0