
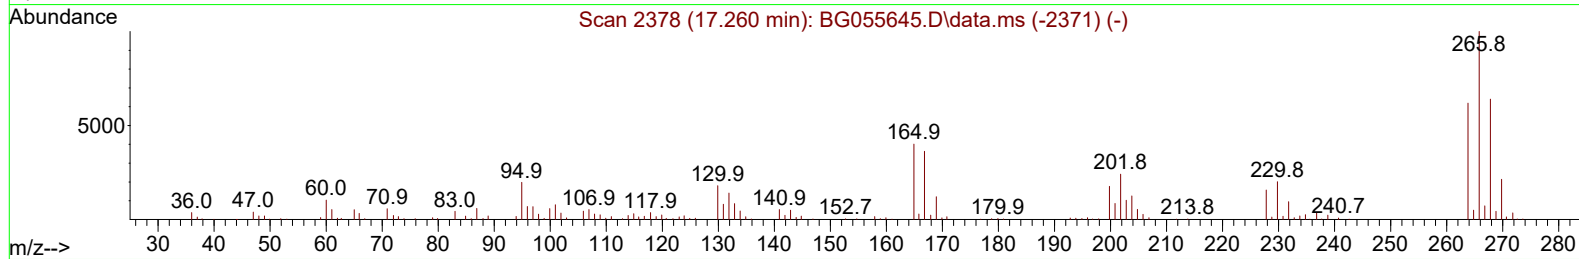
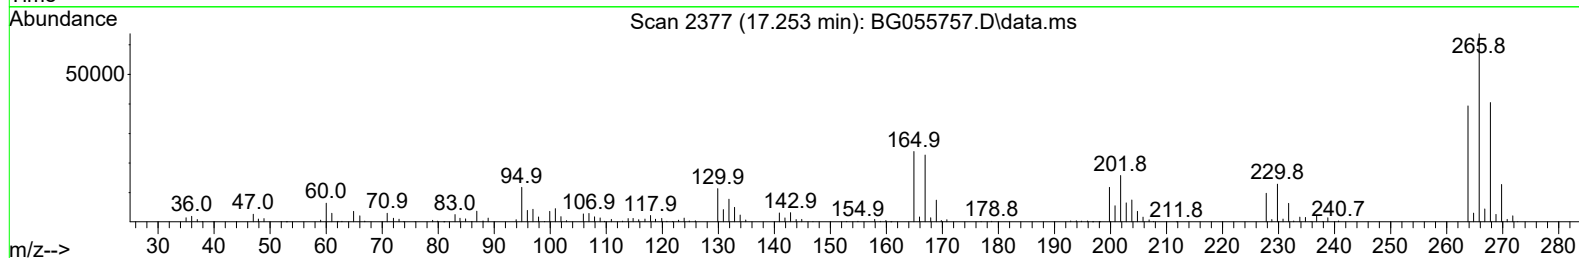


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112322\
Data File : BG055757.D
Acq On : 23 Nov 2022 16:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 17:23:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:35:20 2022
Response via : Initial Calibration

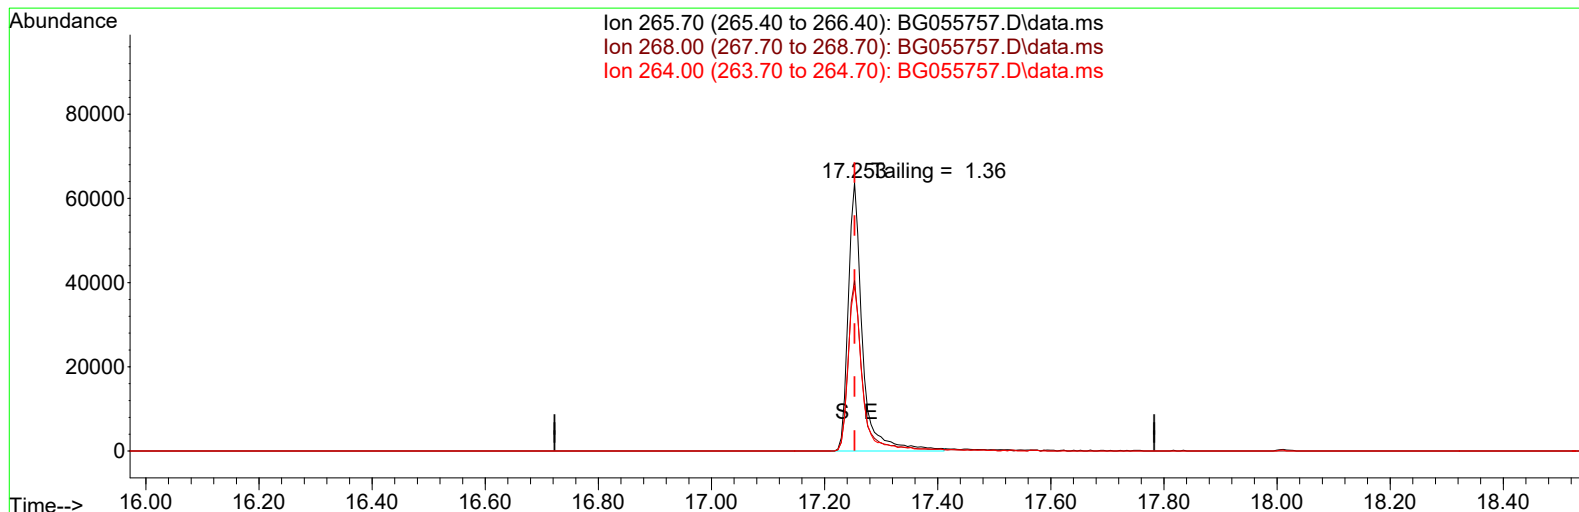

TIC: BG055757.D\data.ms

(70) Pentachlorophenol (C)




17.253min (-0.000) 27124.37 ng

response 112782

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.45
264.00	61.90	61.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112322\
Data File : BG055757.D
Acq On : 23 Nov 2022 16:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 17:23:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:35:20 2022
Response via : Initial Calibration

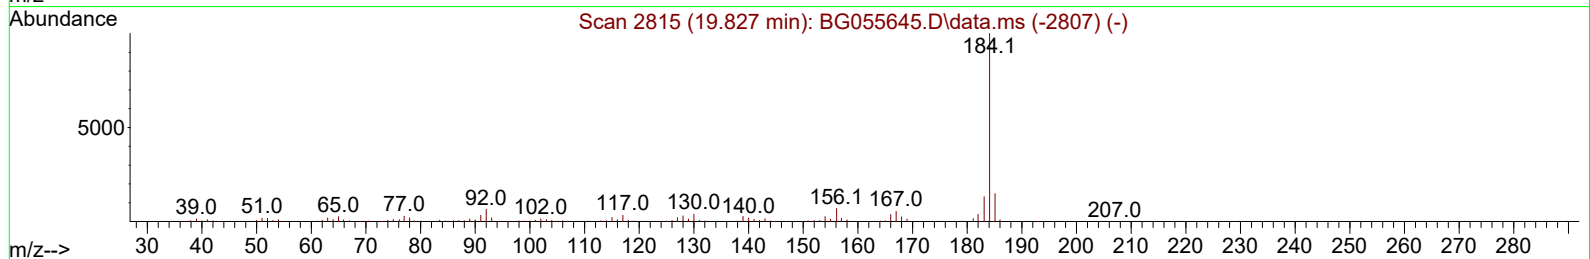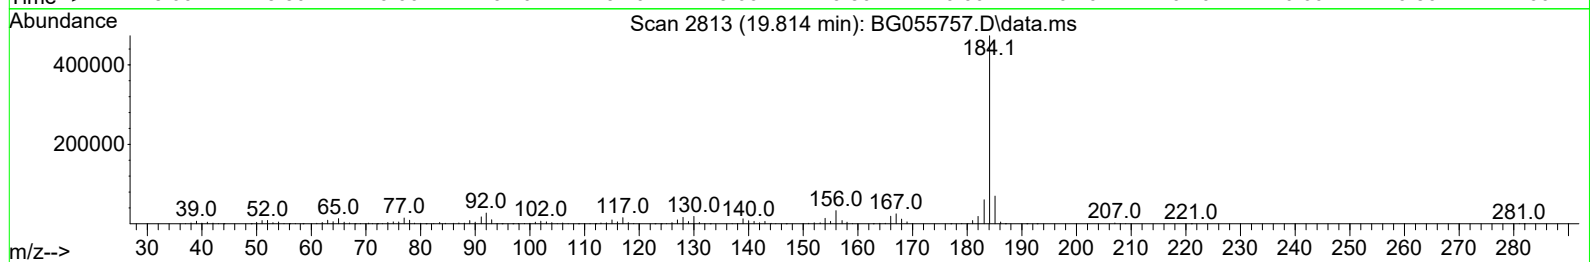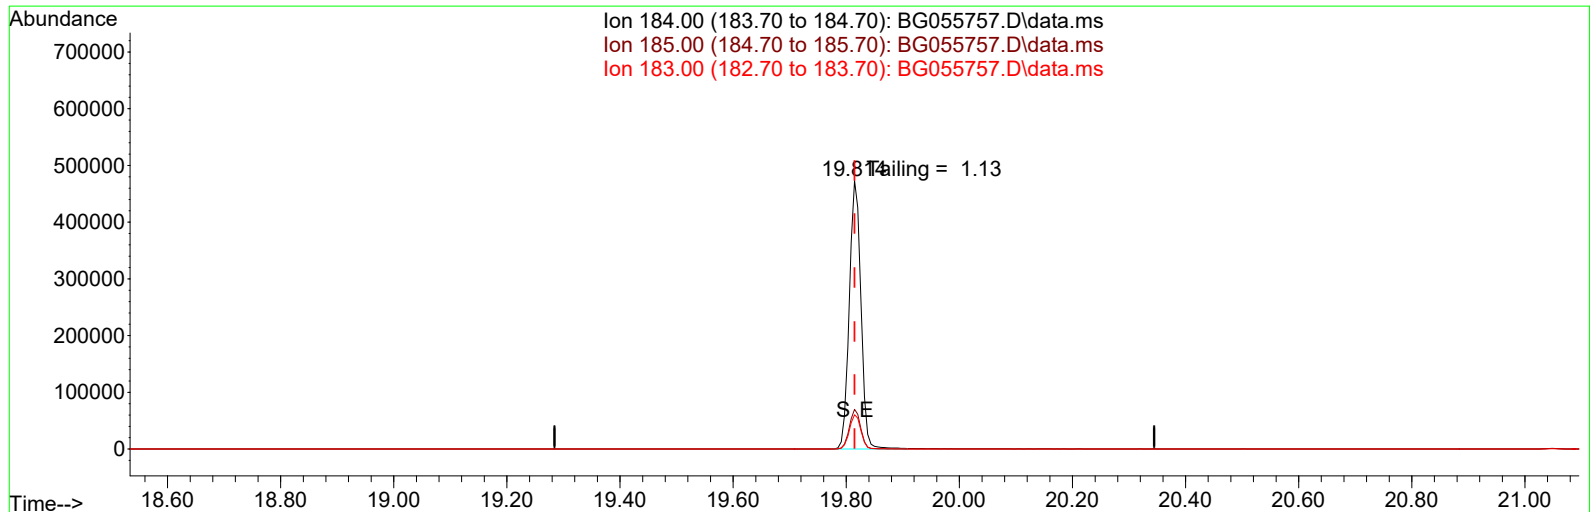

TIC: BG055757.D\data.ms

(77) Benzidine**19.814min (-0.000) 264009.81 ng****response 677958**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.78
183.00	13.20	12.78
0.00	0.00	0.00