
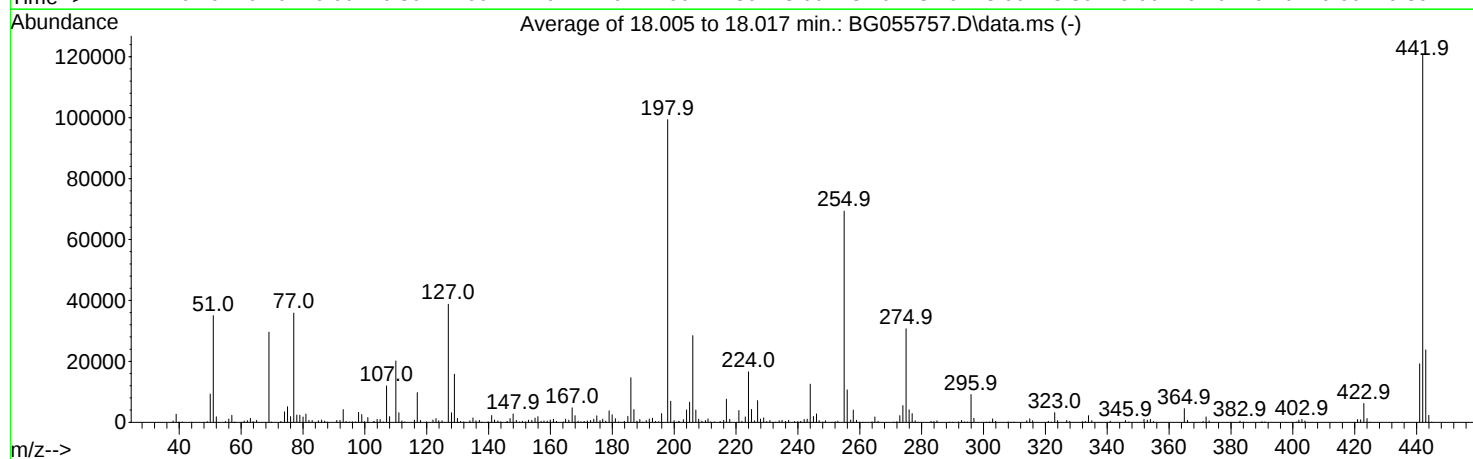


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112322\
 Data File : BG055757.D
 Acq On : 23 Nov 2022 16:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 24 06:05:02 2022

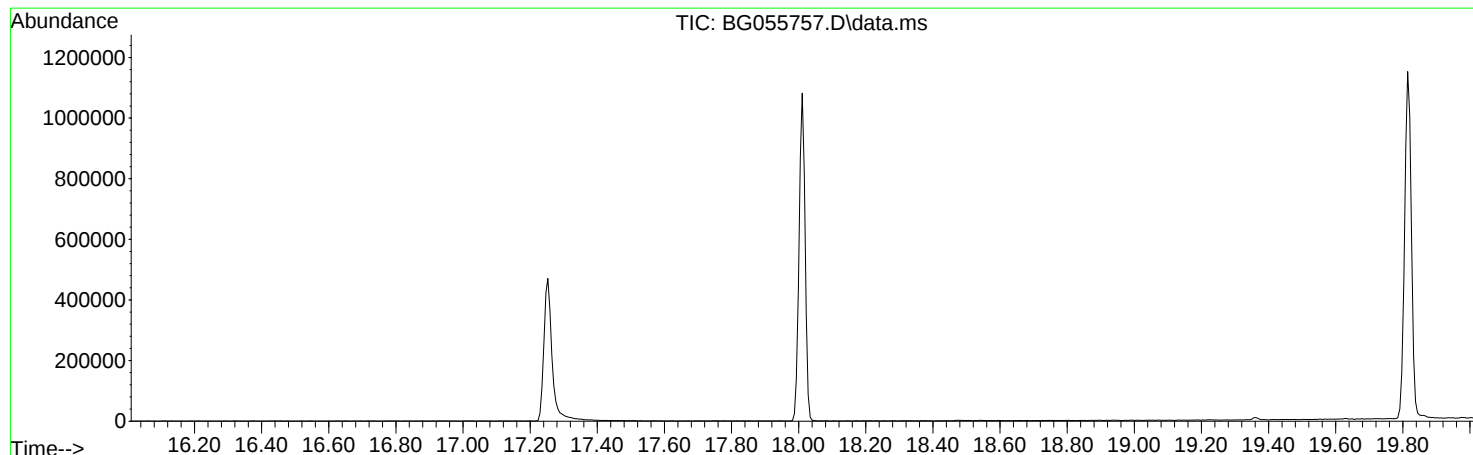




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	35000	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.8	29581	PASS
70	69	0.00	2	0.2	60	PASS
127	198	10	80	39.0	38765	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99360	PASS
199	198	5	9	6.9	6893	PASS
275	198	10	60	30.9	30683	PASS
365	198	1	100	4.5	4472	PASS
441	198	0.01	100	19.3	19205	PASS
442	442	50	100	100.0	120763	PASS
443	442	15	24	19.7	23752	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112322\
Data File : BG055757.D
Acq On : 23 Nov 2022 16:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 23 17:23:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:35:20 2022
Response via : Initial Calibration

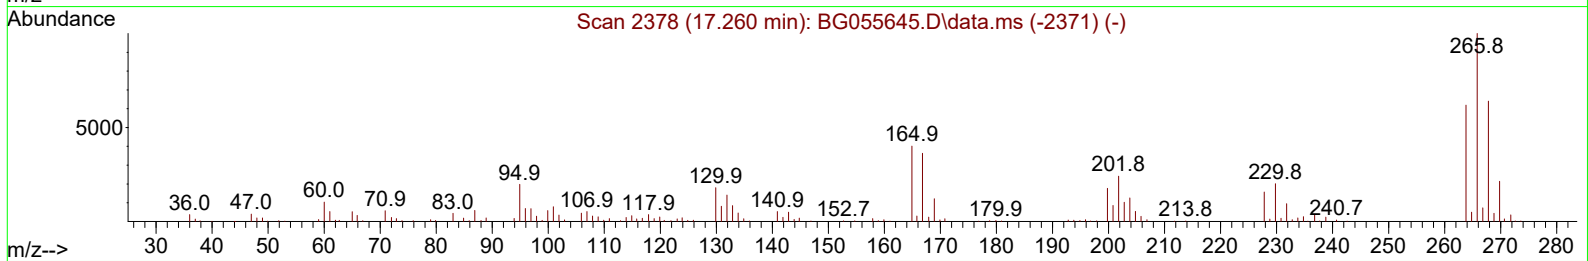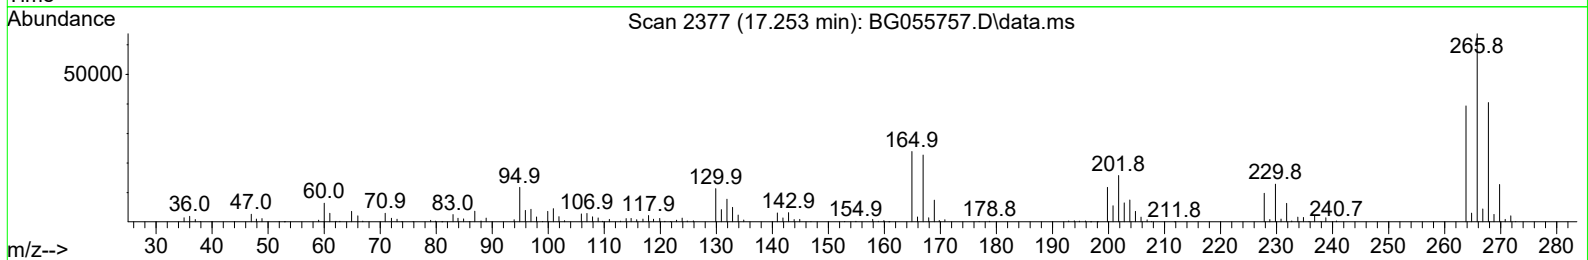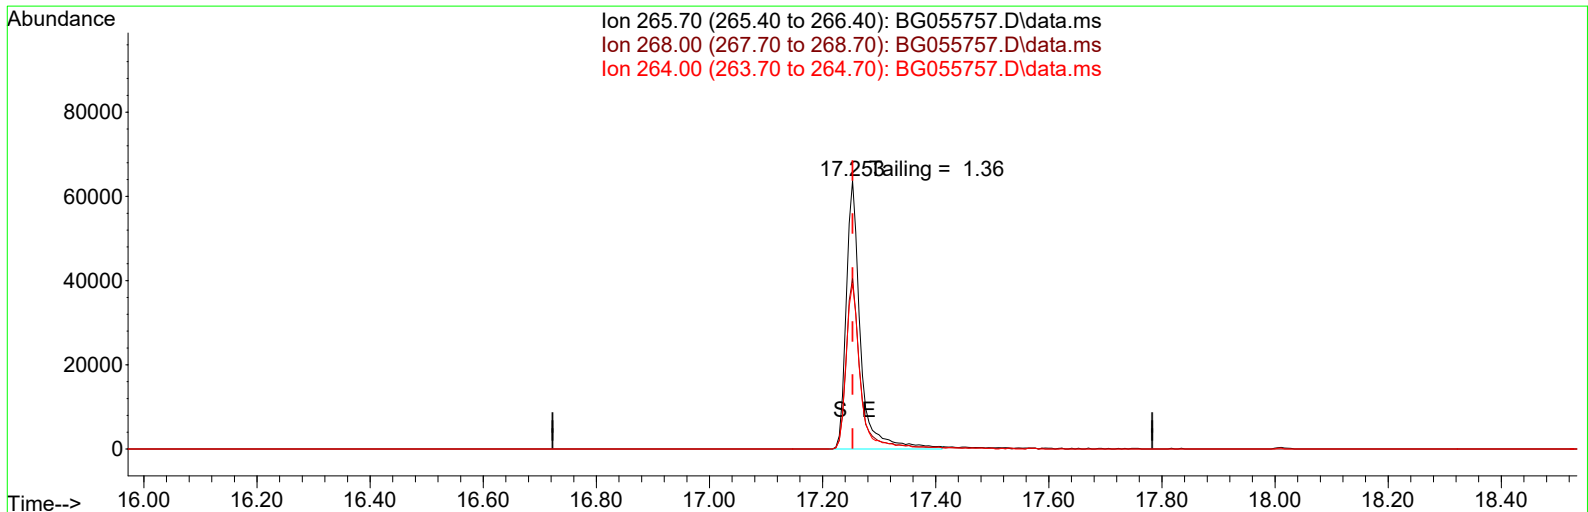

TIC: BG055757.D\data.ms

(70) Pentachlorophenol (C)

17.253min (-0.000) 27124.37 ng




response 112782

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.45
264.00	61.90	61.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112322\
 Data File : BG055757.D
 Acq On : 23 Nov 2022 16:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 23 17:23:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 23 01:35:20 2022
 Response via : Initial Calibration

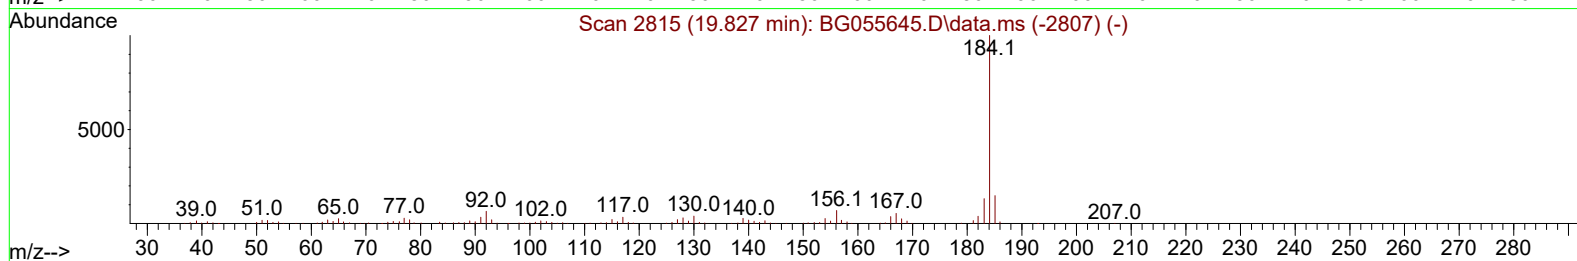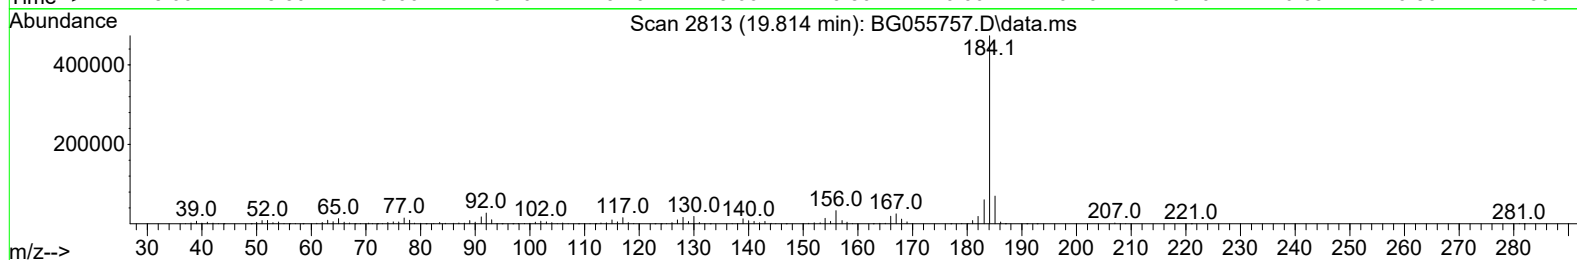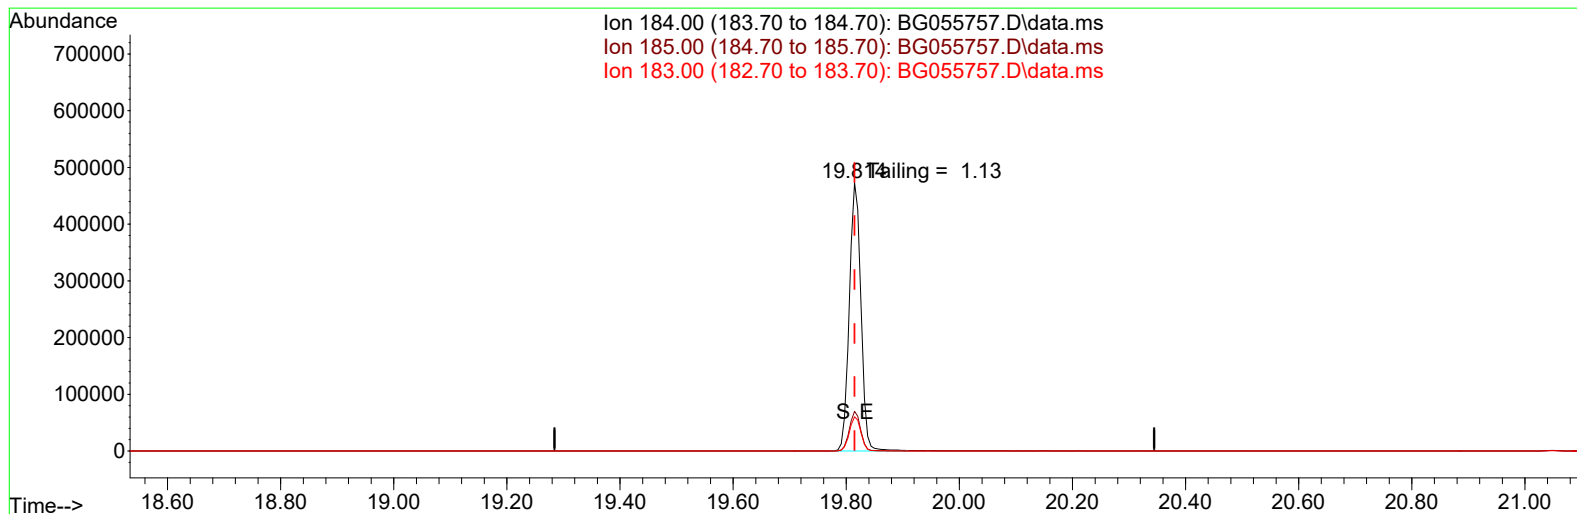

TIC: BG055757.D\data.ms

(77) Benzidine

19.814min (-0.000) 264009.81 ng

response 677958

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.78
183.00	13.20	12.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/23/2022	BNA_G	<u>BG055757.D</u>
Compound Name	Response	Retention Time
DDT	335197	21.048
DDD	10475	20.596
DDE	313	20.097
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10788	345985	3.12

Instrument :
BNA_G
ClientSampleId :
DFTPP