
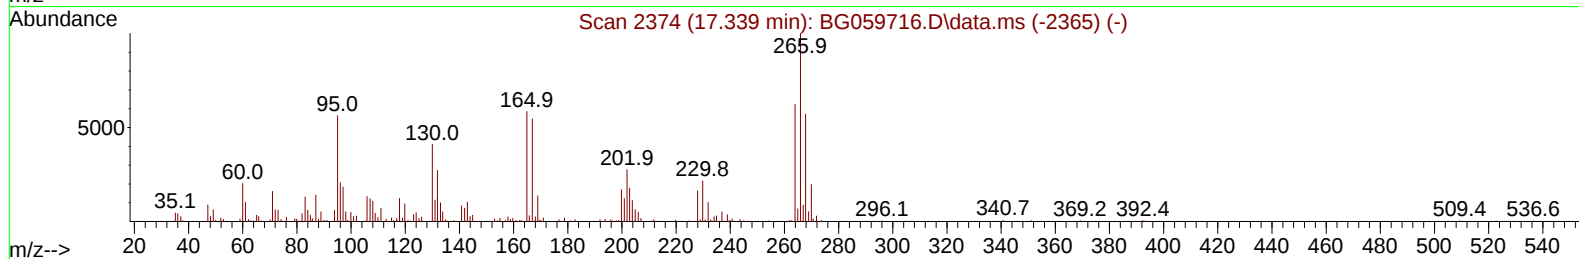
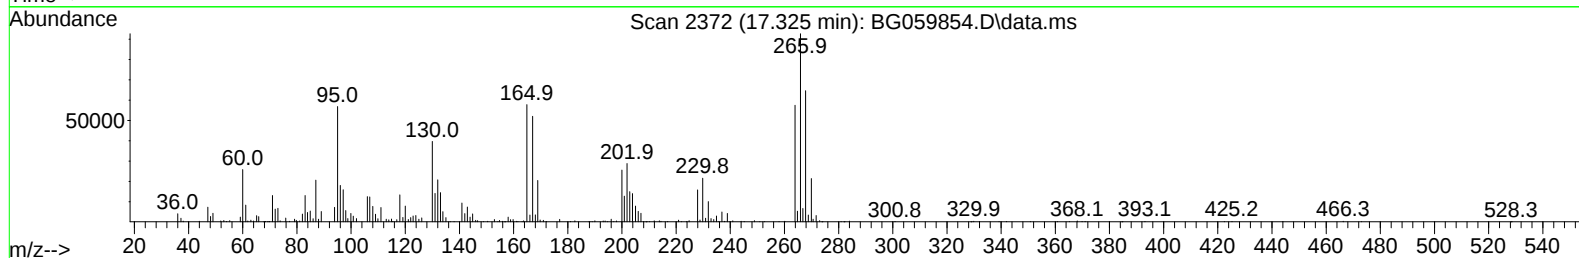


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059854.D
Acq On : 24 Nov 2023 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 13:30:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

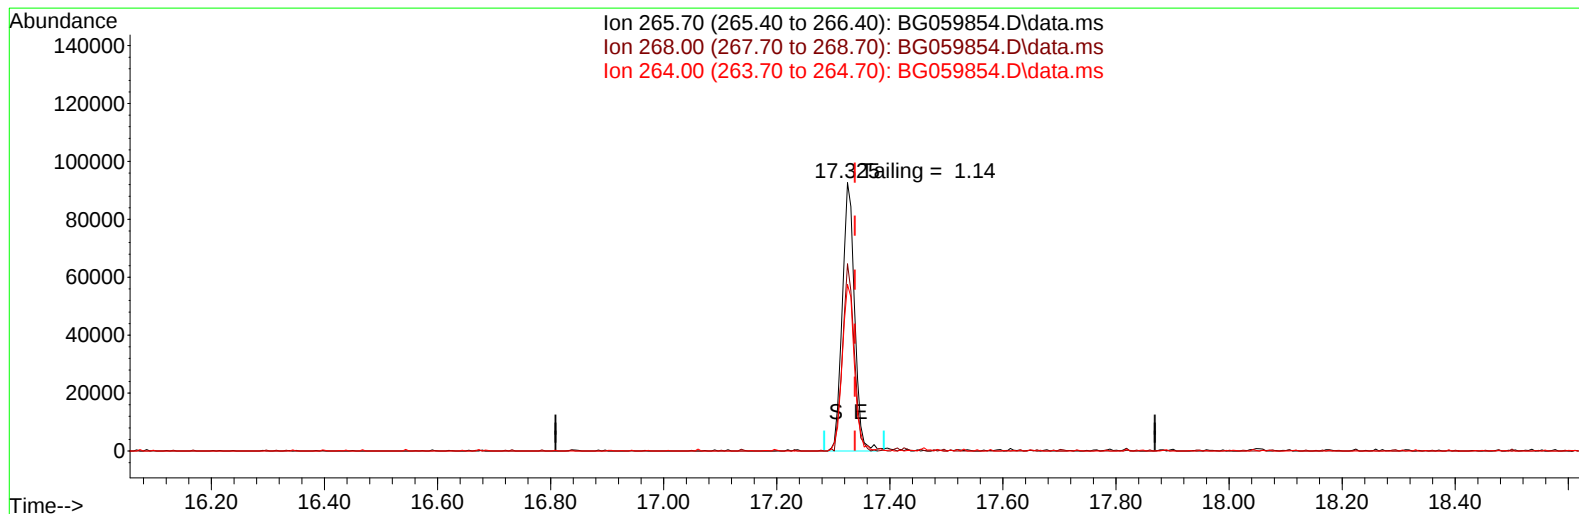

TIC: BG059854.D\data.ms

(70) Pentachlorophenol (C)




17.325min (-0.014) 24563.53 ng

response 140363

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	69.78#
264.00	62.30	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059854.D
Acq On : 24 Nov 2023 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 13:30:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

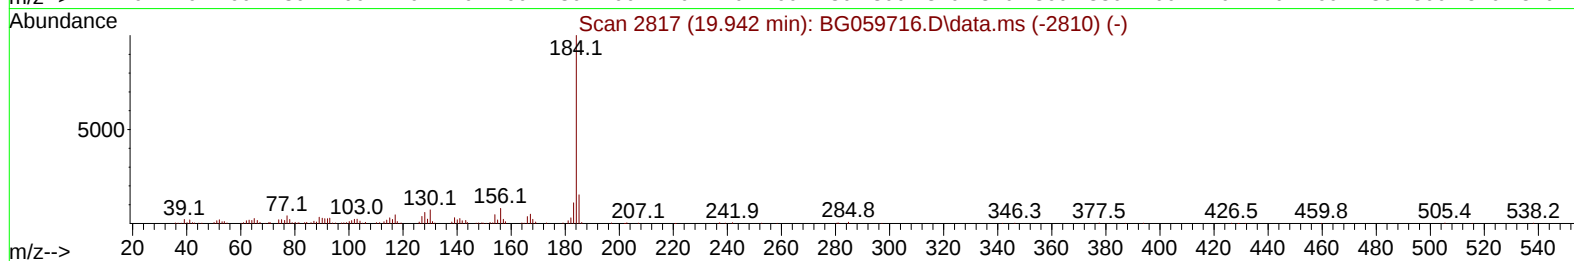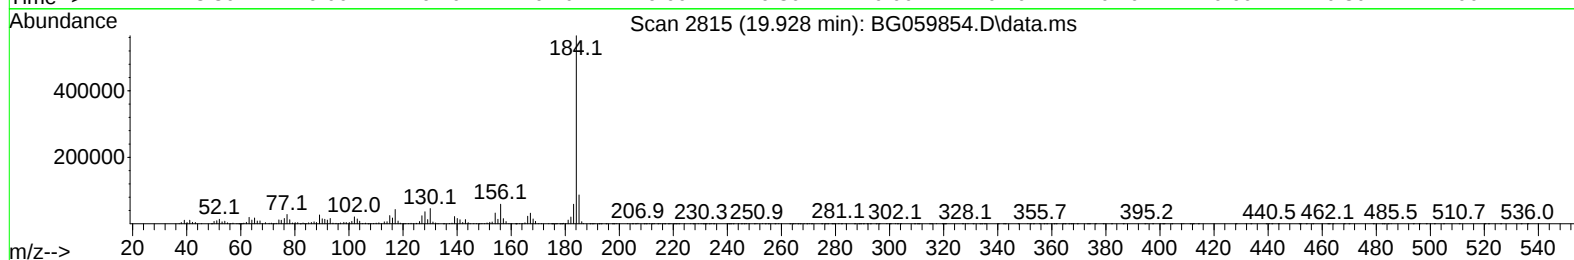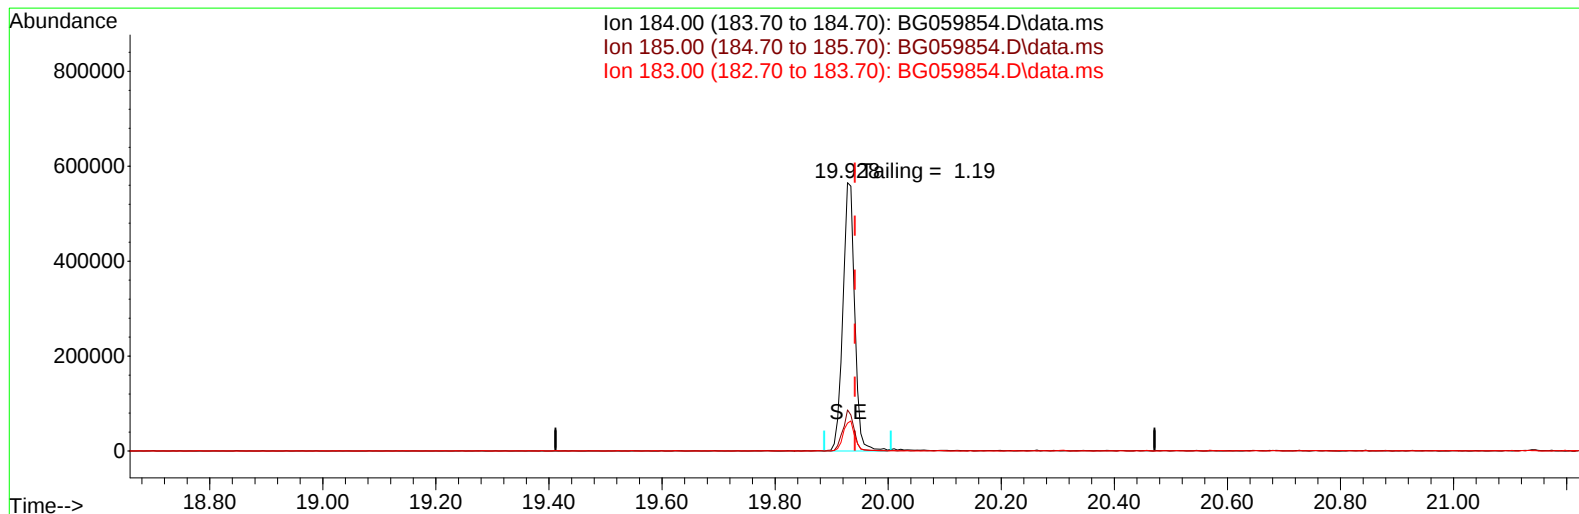

TIC: BG059854.D\data.ms

(77) Benzidine**19.928min (-0.014) 29495.18 ng****response 820649**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.37
183.00	11.00	10.39
0.00	0.00	0.00