
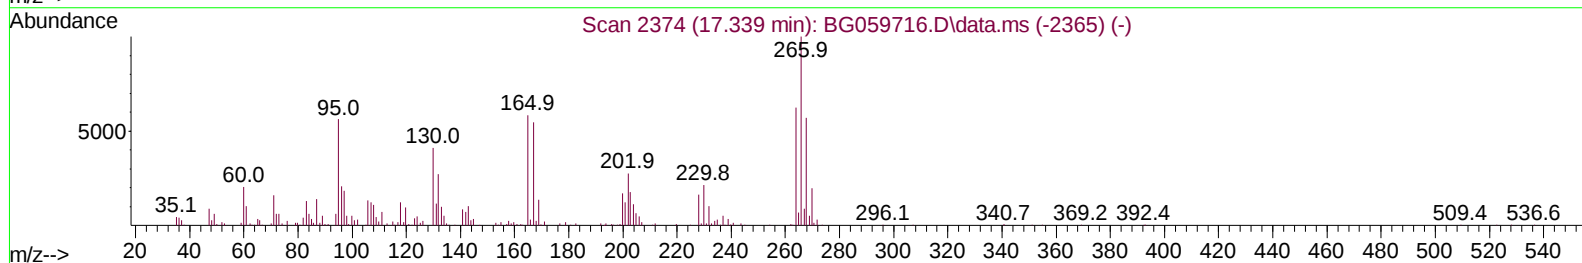
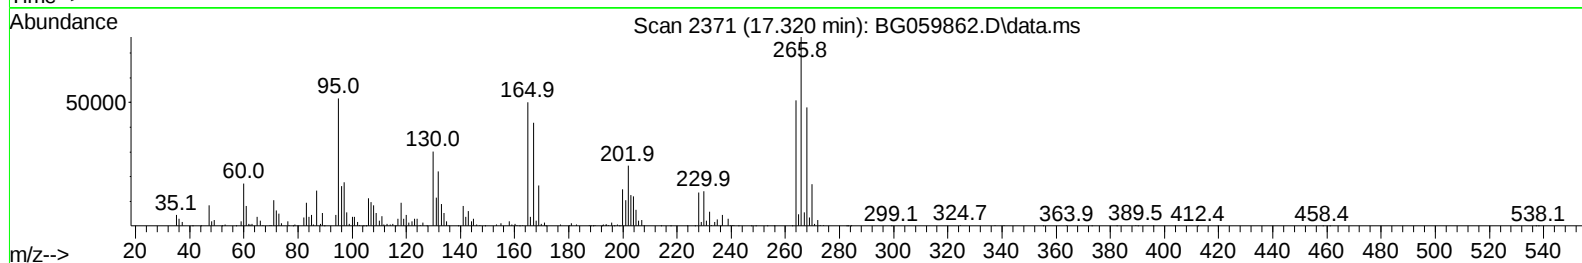


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
 Data File : BG059862.D
 Acq On : 24 Nov 2023 17:24
 Operator : MA/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 00:25:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 15:11:07 2023
 Response via : Initial Calibration

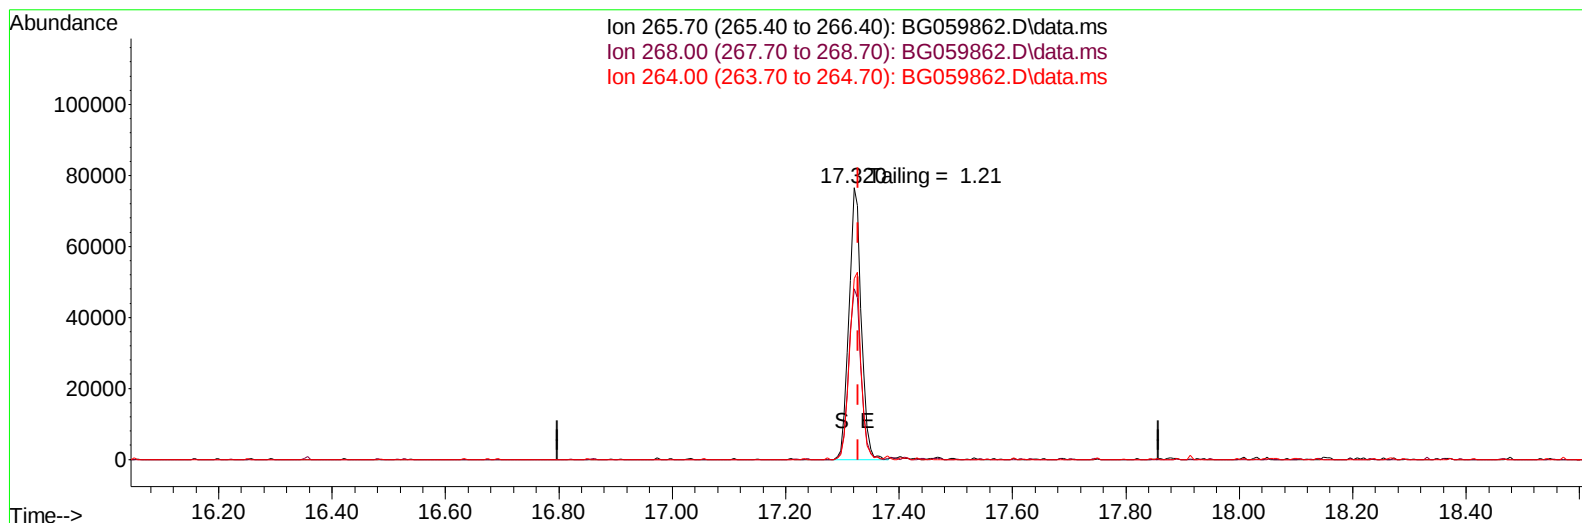




TIC: BG059862.D\data.ms

(70) Pentachlorophenol (C)**17.320min (-0.007) 54473.83 ng****response 114594**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	62.80
264.00	62.30	66.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059862.D
Acq On : 24 Nov 2023 17:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 00:25:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:11:07 2023
Response via : Initial Calibration

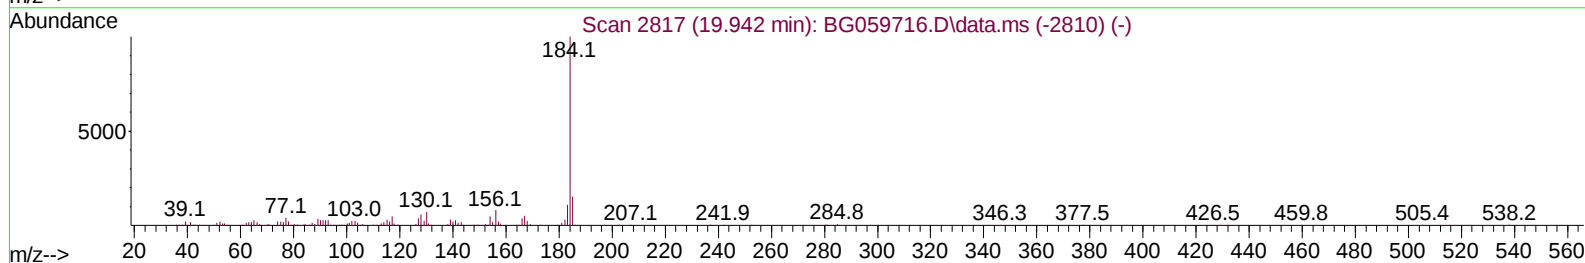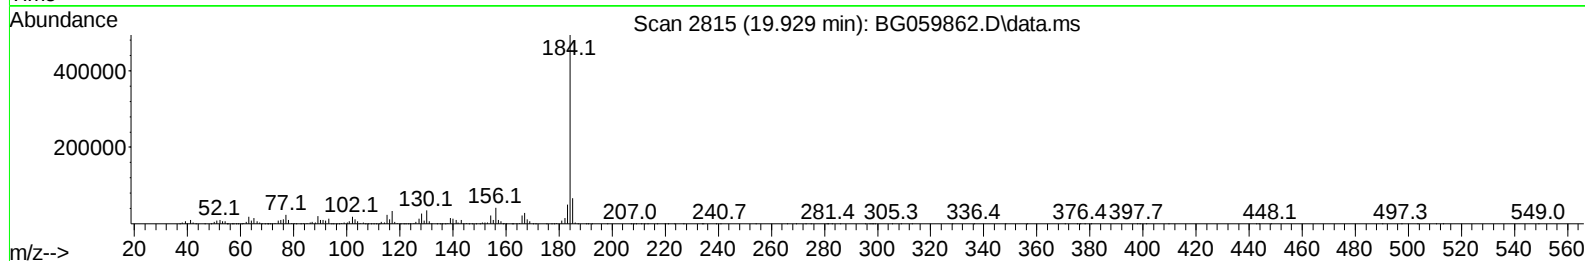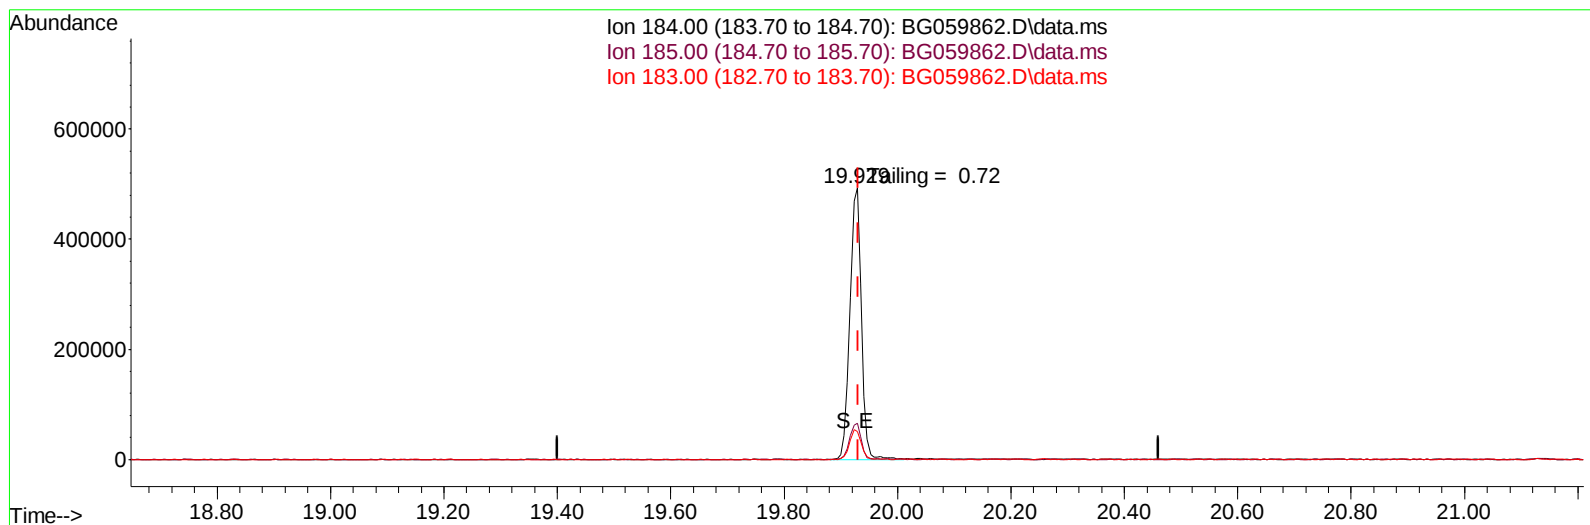

TIC: BG059862.D\data.ms

(77) Benzidine**19.929min (-0.001) 267351.38 ng****response 691113**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.45
183.00	11.00	10.21
0.00	0.00	0.00