
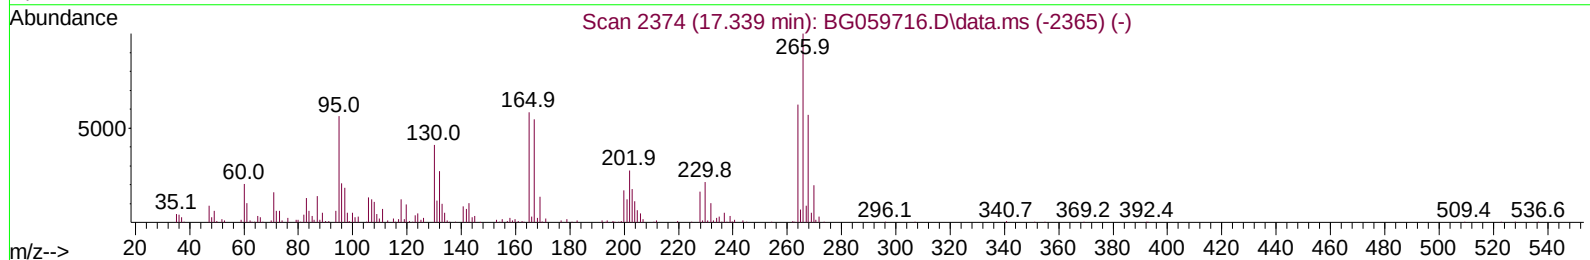
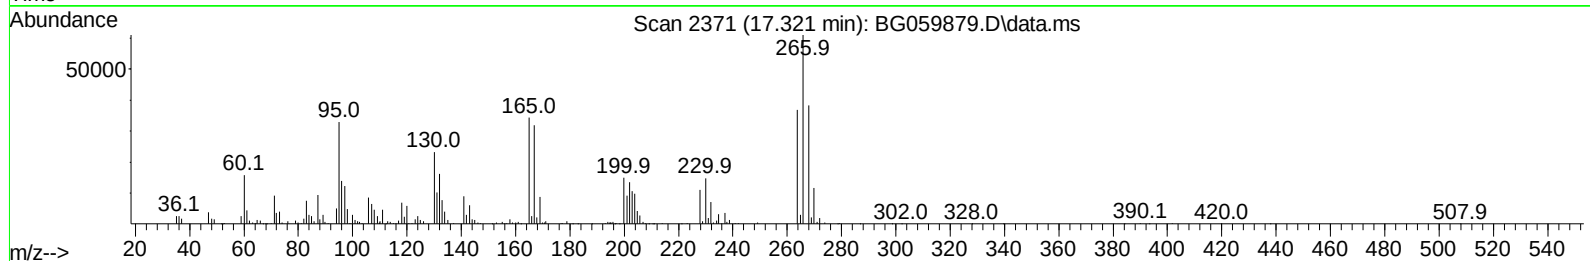


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059879.D
Acq On : 25 Nov 2023 5:50
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 06:29:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:11:07 2023
Response via : Initial Calibration

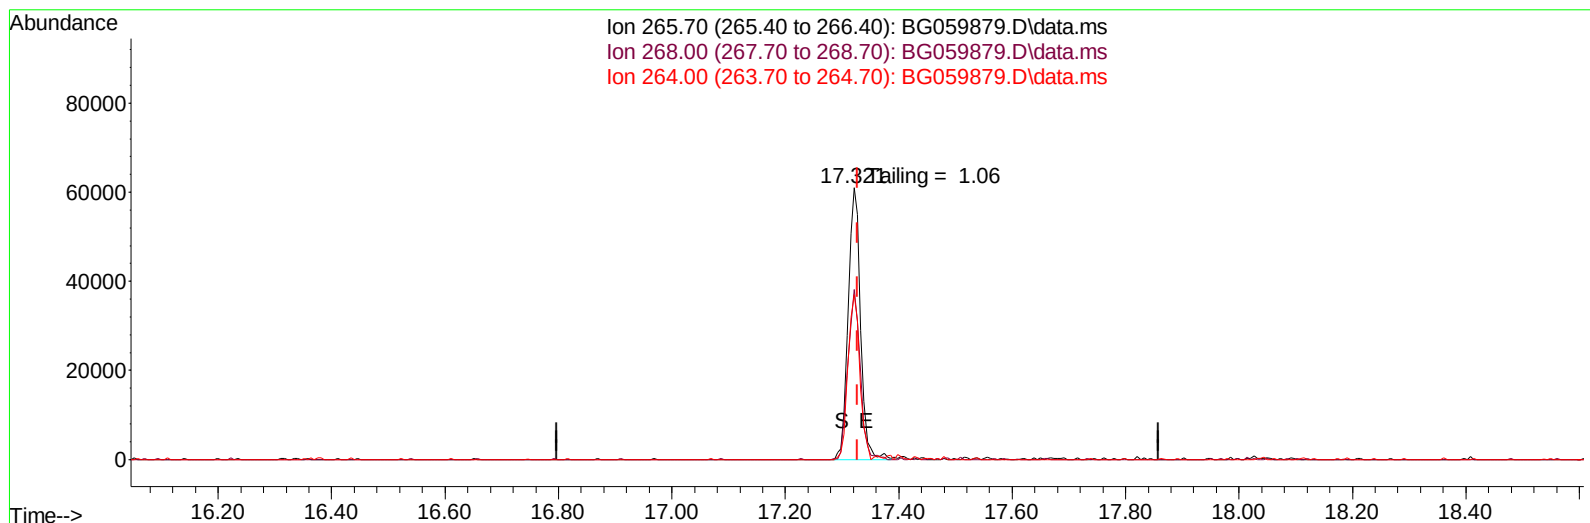

TIC: BG059879.D\data.ms

(70) Pentachlorophenol (C)




17.321min (-0.006) 109416.85 ng

response 91233

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	62.72
264.00	62.30	60.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059879.D
Acq On : 25 Nov 2023 5:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 06:29:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:11:07 2023
Response via : Initial Calibration

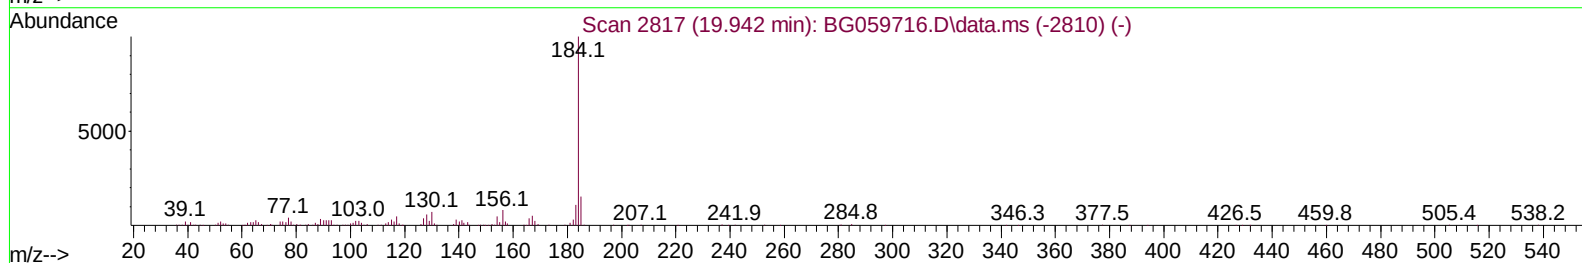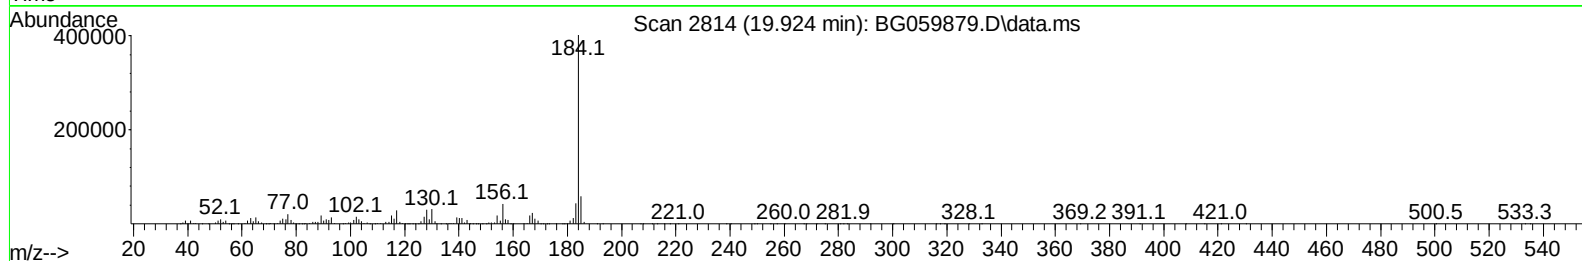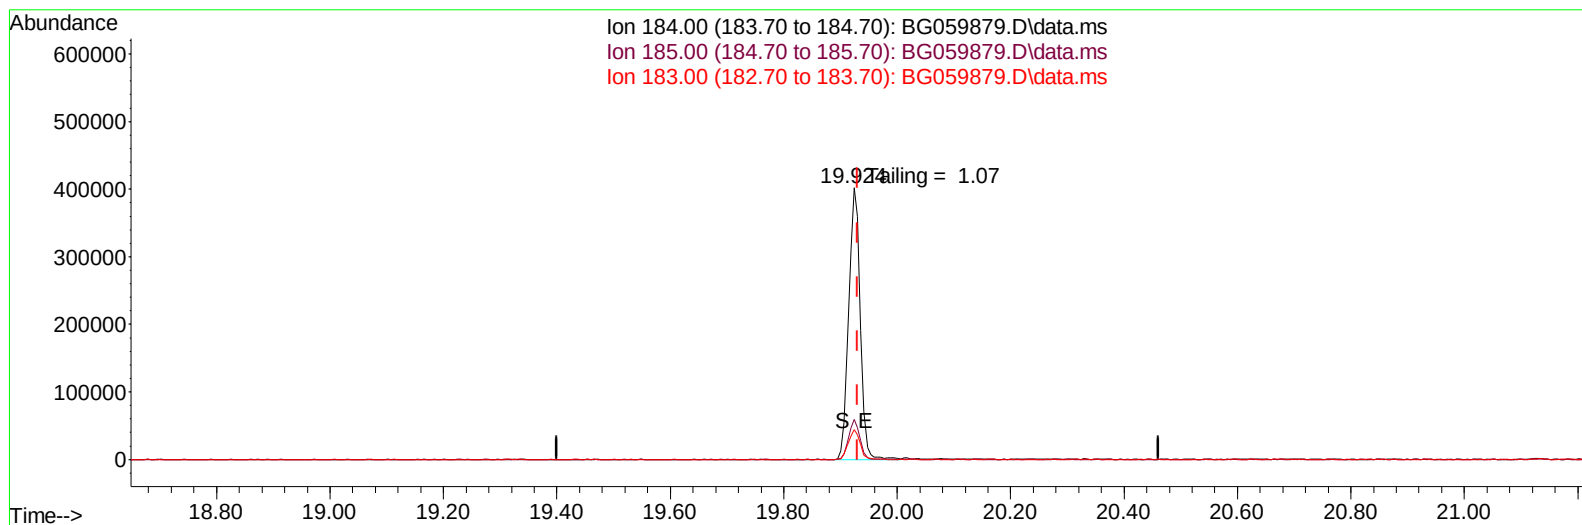

TIC: BG059879.D\data.ms

(77) Benzidine**19.924min (-0.006) 71201.58 ng****response 569936**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.64
183.00	11.00	11.05
0.00	0.00	0.00