

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
 Data File : BG059864.D
 Acq On : 24 Nov 2023 19:02
 Operator : MA/JU
 Sample : PB157019BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB157019BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG059864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.808	405	412	422	rBV	544555	886212	17.32%	5.898%
2	7.442	683	690	699	rVB	519317	914793	17.88%	6.088%
3	8.317	833	839	845	rVB3	87891	149402	2.92%	0.994%
4	9.516	1035	1043	1051	rBV2	336603	632631	12.37%	4.210%
5	11.167	1316	1324	1332	rVB	121013	213335	4.17%	1.420%
6	13.570	1725	1733	1742	rBV	1626899	2446961	47.83%	16.286%
7	14.951	1961	1968	1975	rVB2	294280	463707	9.06%	3.086%
8	16.437	2213	2221	2231	rBV	1527366	2285968	44.68%	15.214%
9	17.700	2429	2436	2445	rBV	465749	695509	13.59%	4.629%
10	20.280	2868	2875	2880	rBV	4048835	5116168	100.00%	34.051%
11	22.025	3165	3172	3179	rVB	362688	638903	12.49%	4.252%
12	25.585	3769	3778	3788	rBV3	180594	581506	11.37%	3.870%




Sum of corrected areas: 15025095

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059864.D
Acq On : 24 Nov 2023 19:02
Operator : MA/JU
Sample : PB157019BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157019BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

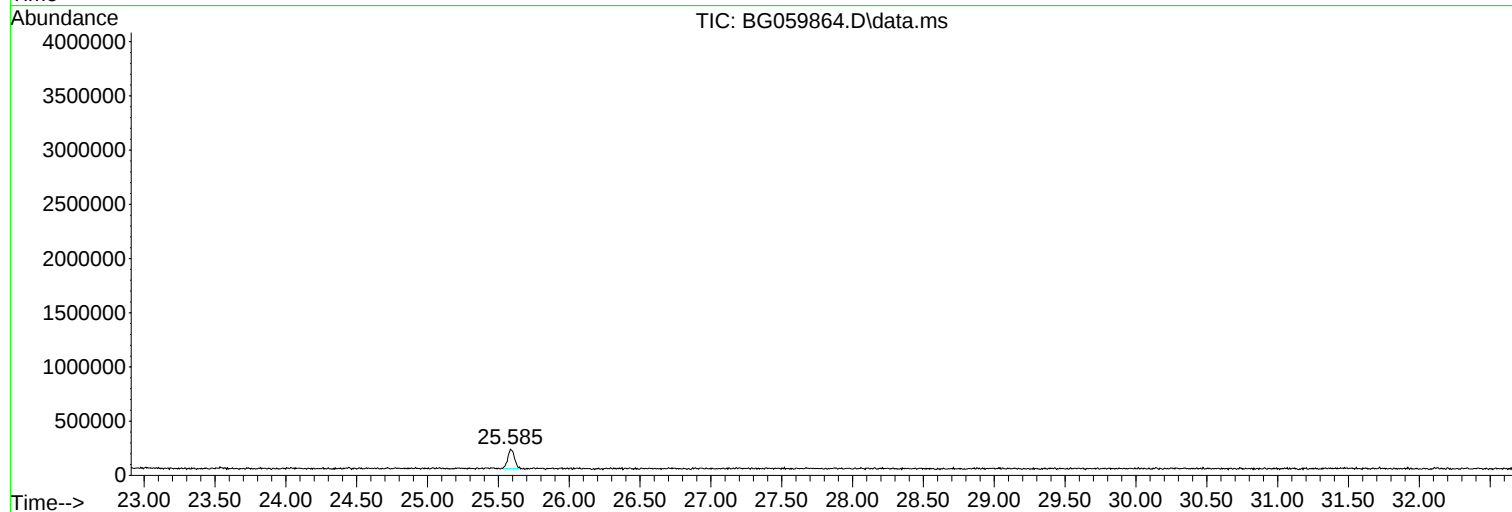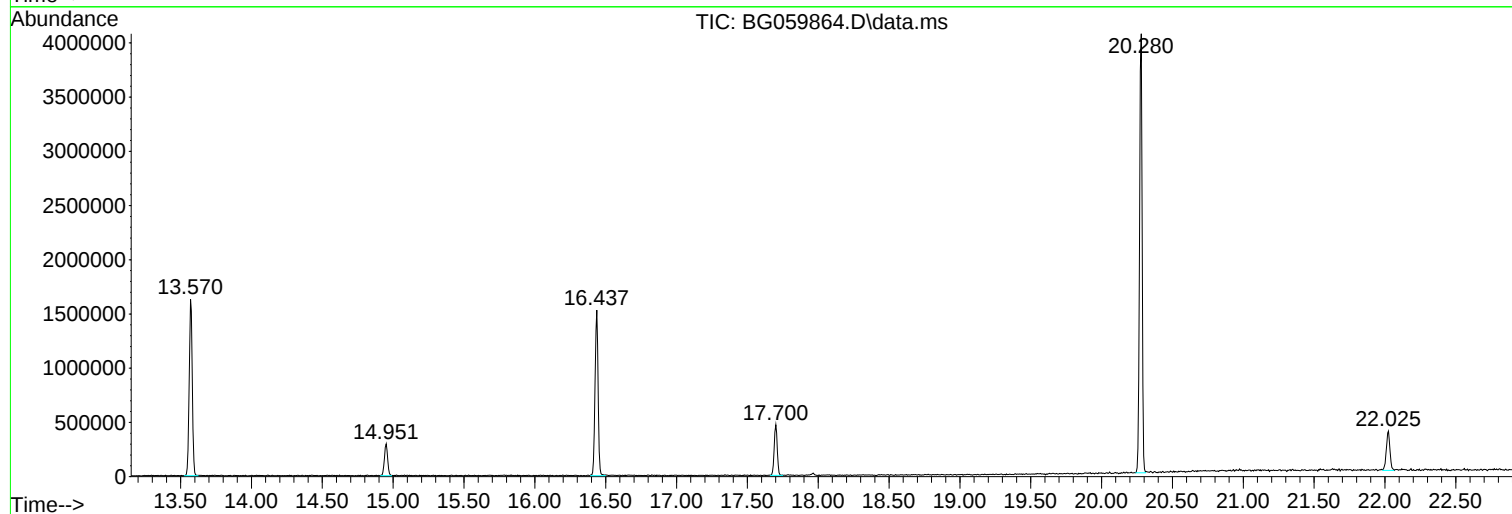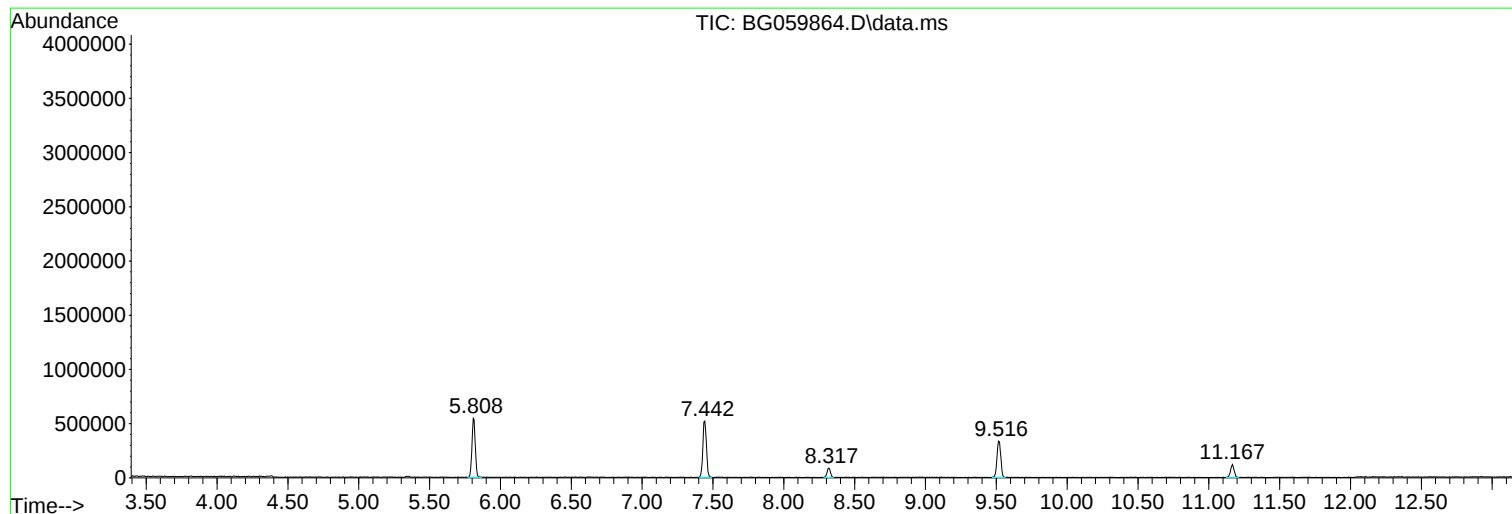

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059864.D
Acq On : 24 Nov 2023 19:02
Operator : MA/JU
Sample : PB157019BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157019BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059864.D
Acq On : 24 Nov 2023 19:02
Operator : MA/JU
Sample : PB157019BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157019BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------