
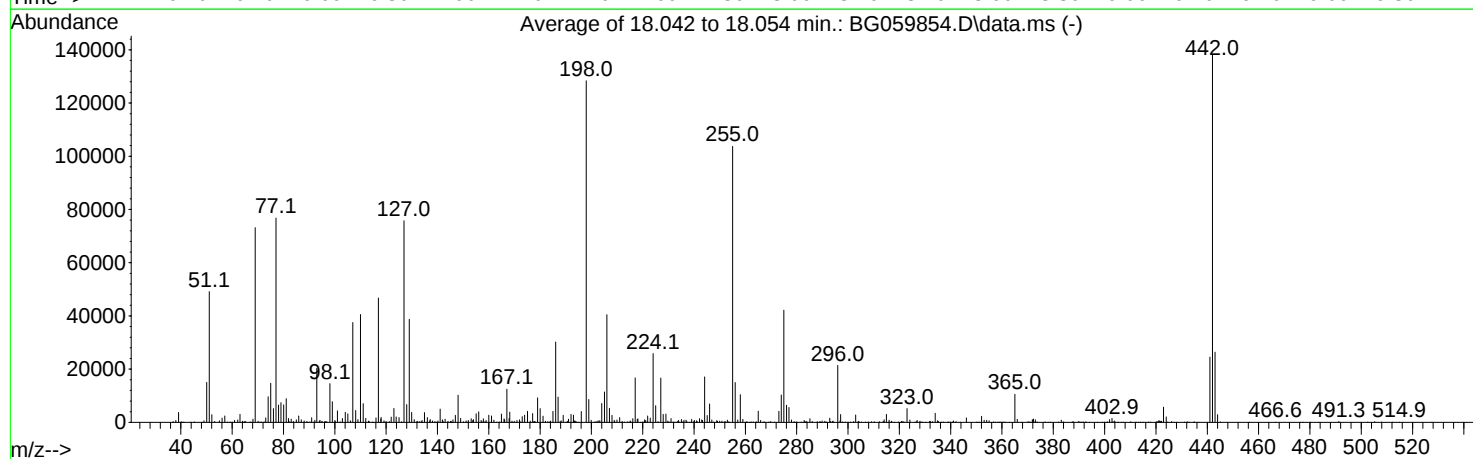


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
 Data File : BG059854.D
 Acq On : 24 Nov 2023 10:56
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 27 13:17:45 2023

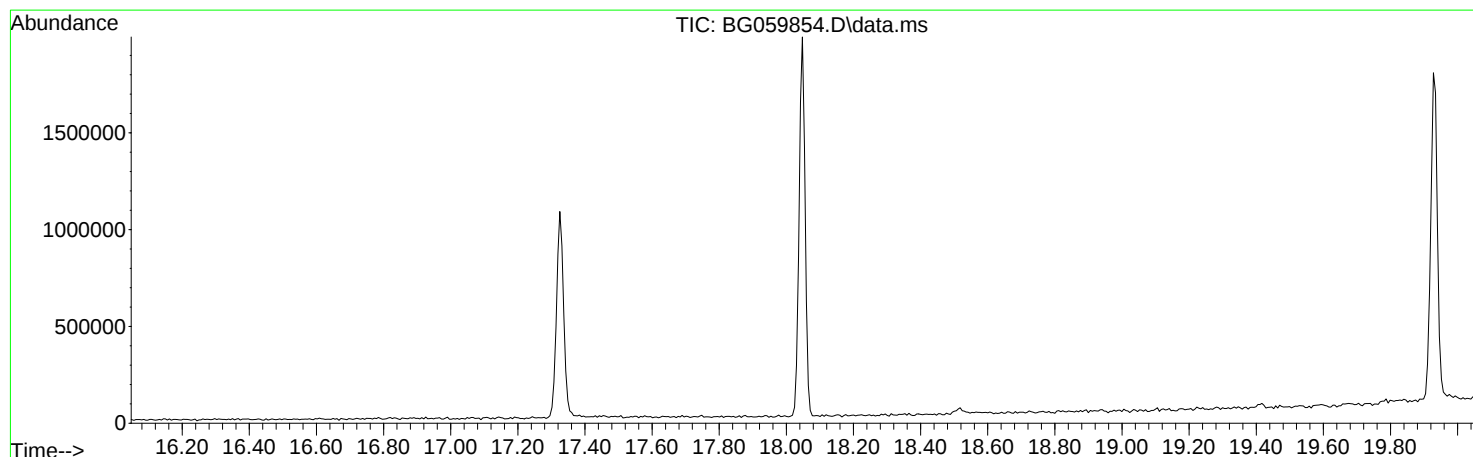




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	49147	PASS
68	69	0.00	2	1.7	1236	PASS
69	198	0.00	100	57.0	73192	PASS
70	69	0.00	2	0.6	434	PASS
127	198	10	80	59.0	75785	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128373	PASS
199	198	5	9	6.7	8603	PASS
275	198	10	60	32.8	42163	PASS
365	198	1	100	8.3	10597	PASS
441	198	0.01	100	19.1	24565	PASS
442	442	50	100	100.0	138232	PASS
443	442	15	24	19.1	26411	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059854.D
Acq On : 24 Nov 2023 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 24 13:30:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

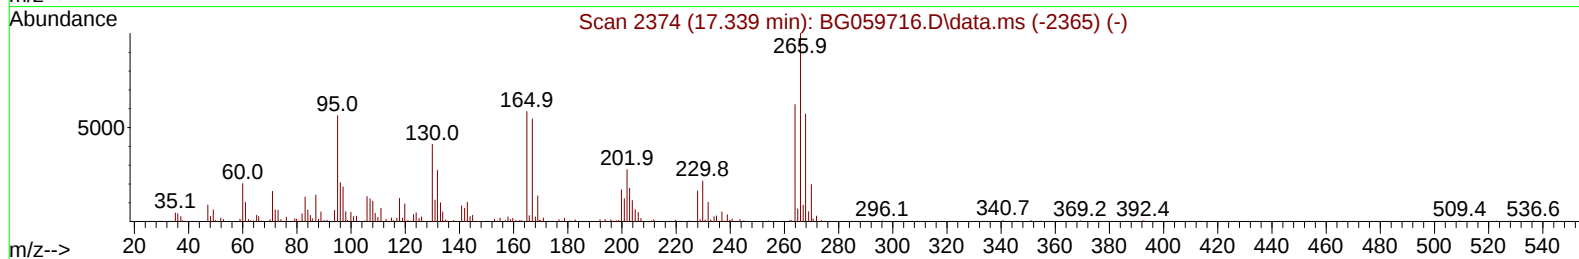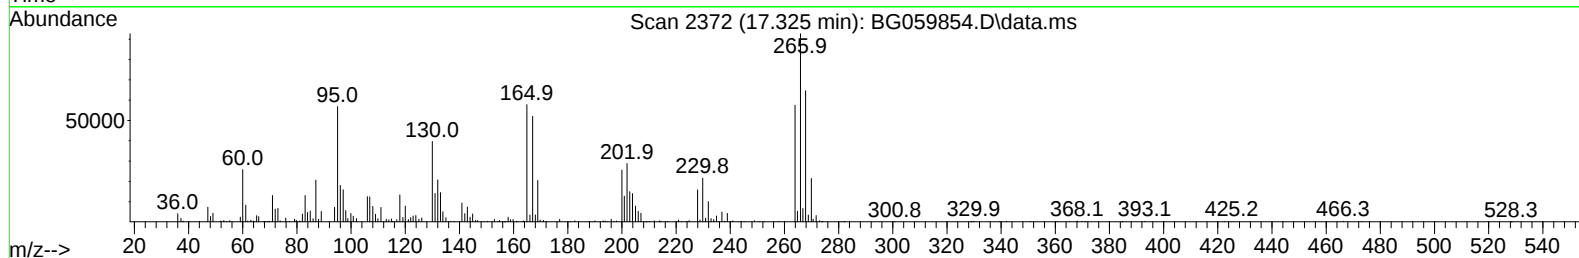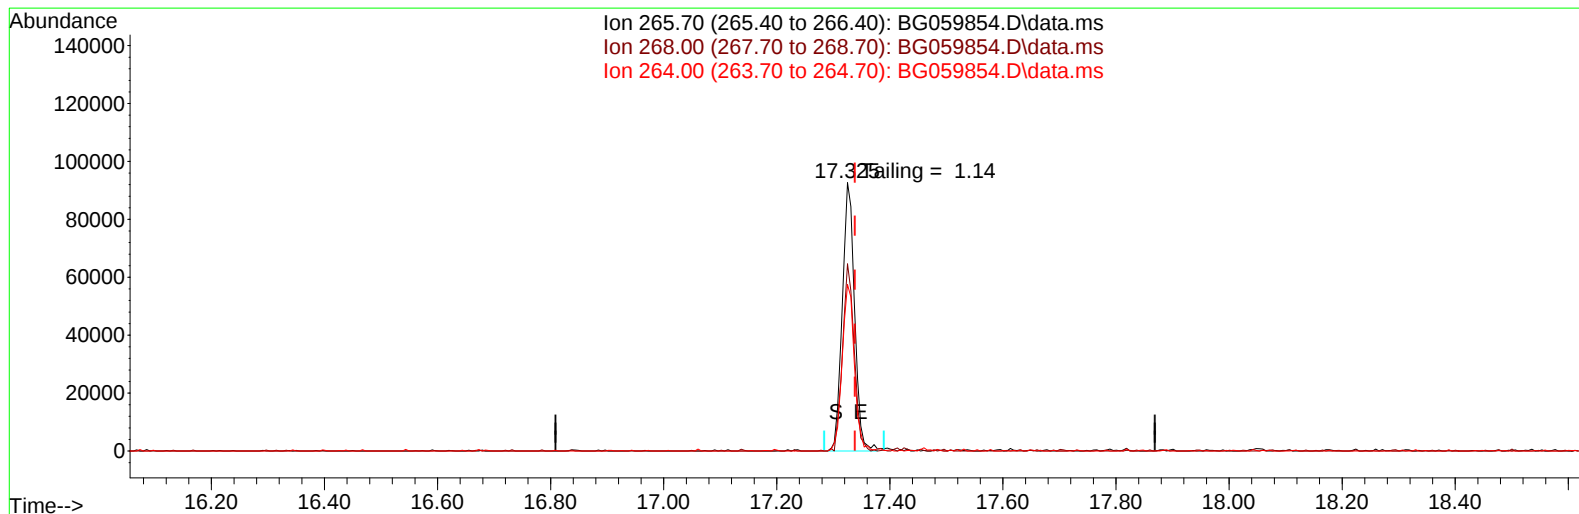

TIC: BG059854.D\data.ms

(70) Pentachlorophenol (C)

17.325min (-0.014) 24563.53 ng




response 140363

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	69.78#
264.00	62.30	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059854.D
Acq On : 24 Nov 2023 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 24 13:30:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

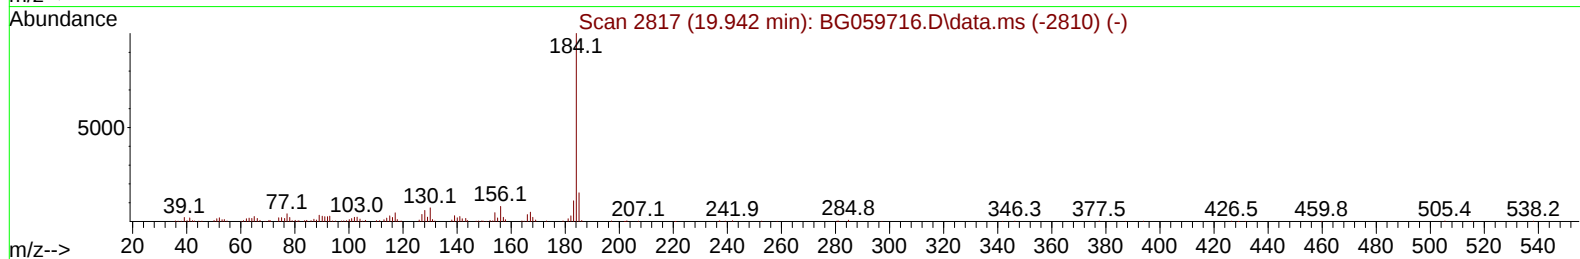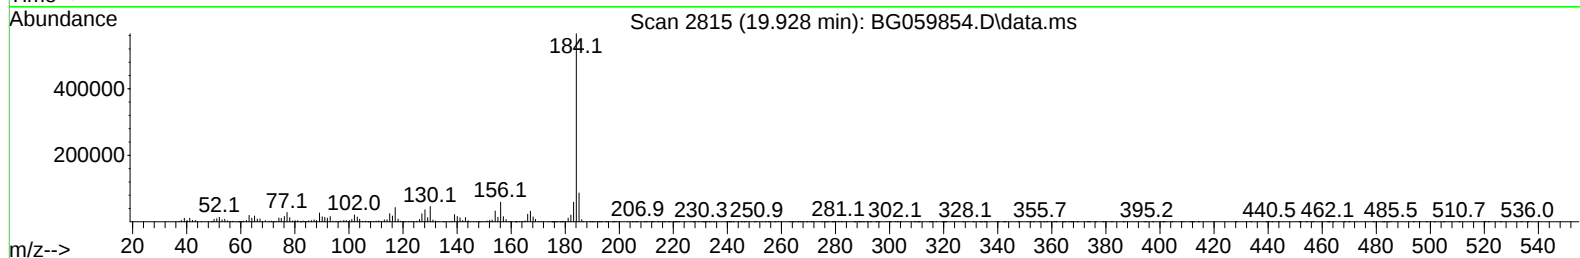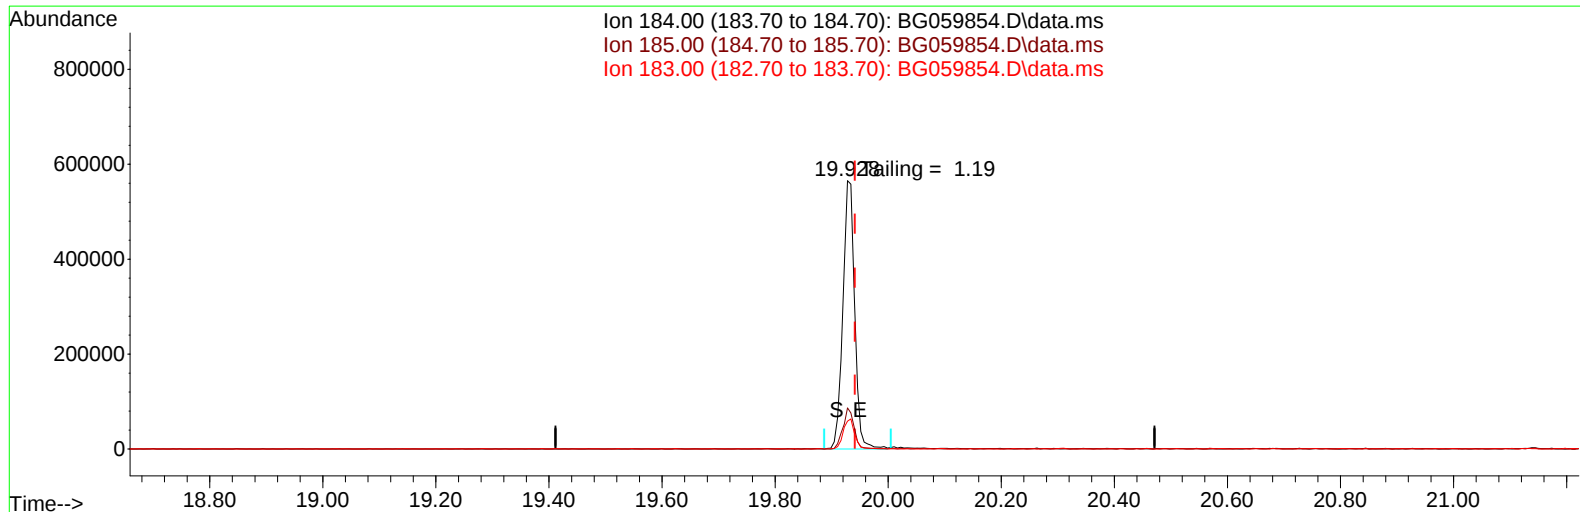

TIC: BG059854.D\data.ms

(77) Benzidine

19.928min (-0.014) 29495.18 ng

response 820649

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.37
183.00	11.00	10.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/24/2023	BNA_G	<u>BG059854.D</u>
Compound Name	Response	Retention Time
DDT	243738	21.138
DDD	55160	20.68
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
55160	298898	18.45

Instrument :
BNA_G
ClientSampleId :
DFTPP