
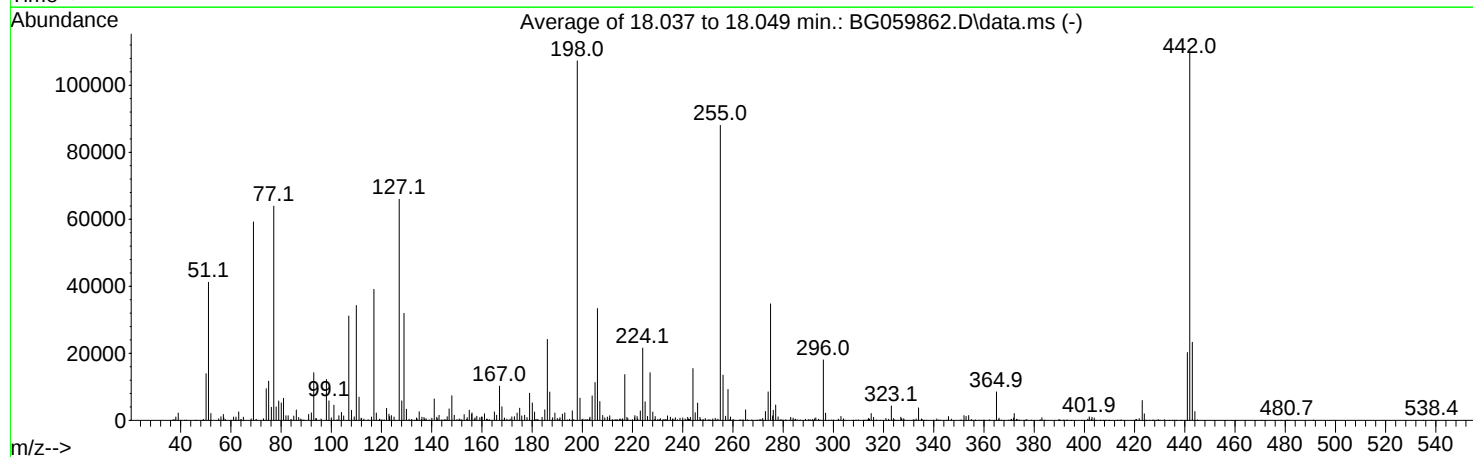


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059862.D
Acq On : 24 Nov 2023 17:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 27 13:17:45 2023

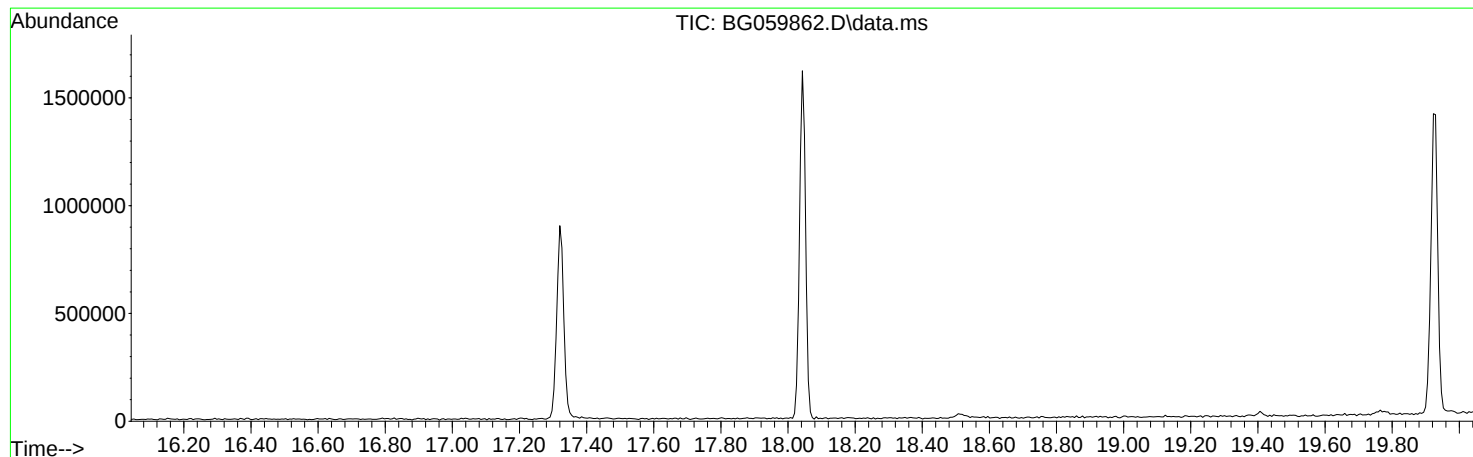




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	41211	PASS
68	69	0.00	2	0.8	461	PASS
69	198	0.00	100	55.2	59192	PASS
70	69	0.00	2	0.5	316	PASS
127	198	10	80	61.5	65997	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	107275	PASS
199	198	5	9	6.2	6632	PASS
275	198	10	60	32.4	34755	PASS
365	198	1	100	7.9	8489	PASS
441	198	0.01	100	18.9	20267	PASS
442	442	50	100	100.0	109776	PASS
443	442	15	24	21.2	23296	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059862.D
Acq On : 24 Nov 2023 17:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 25 00:25:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:11:07 2023
Response via : Initial Calibration

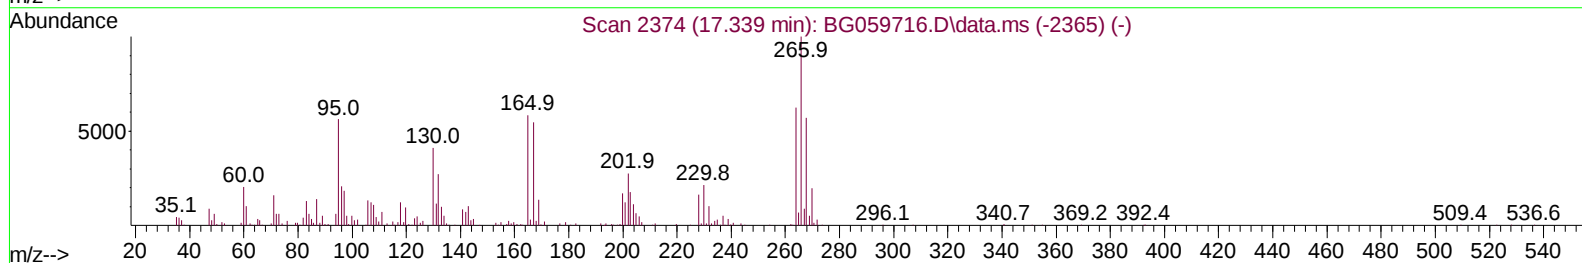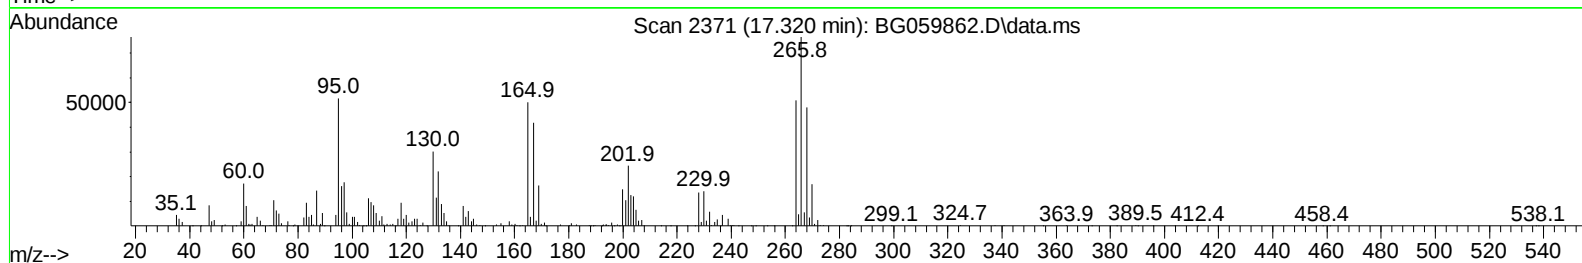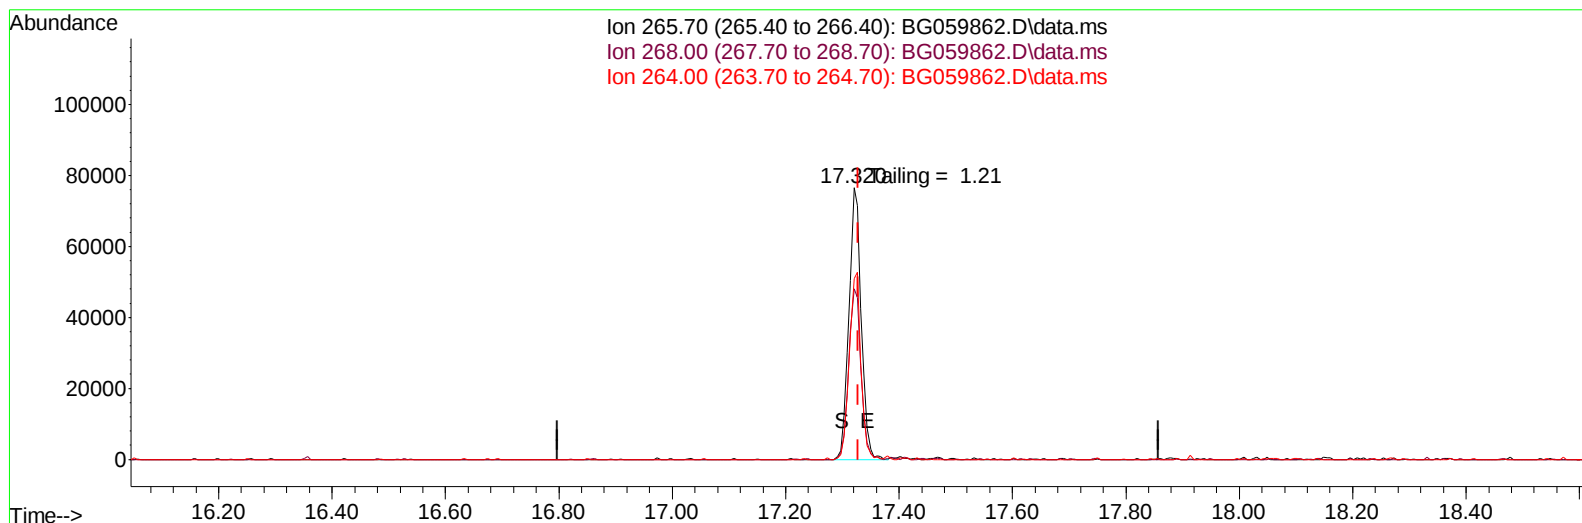

TIC: BG059862.D\data.ms

(70) Pentachlorophenol (C)

17.320min (-0.007) 54473.83 ng




response 114594

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	62.80
264.00	62.30	66.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059862.D
Acq On : 24 Nov 2023 17:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 25 00:25:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:11:07 2023
Response via : Initial Calibration

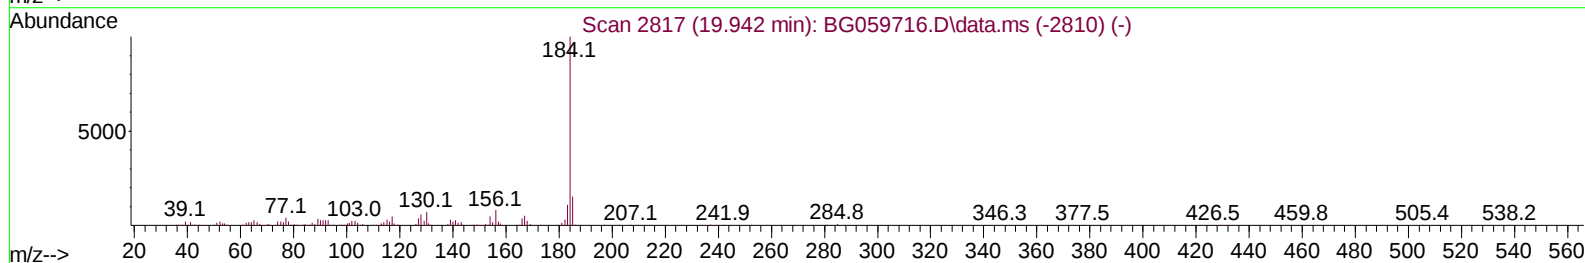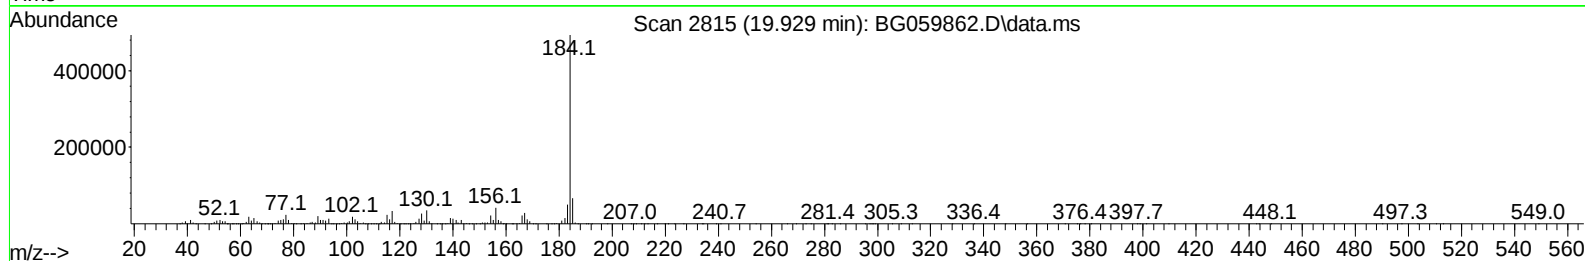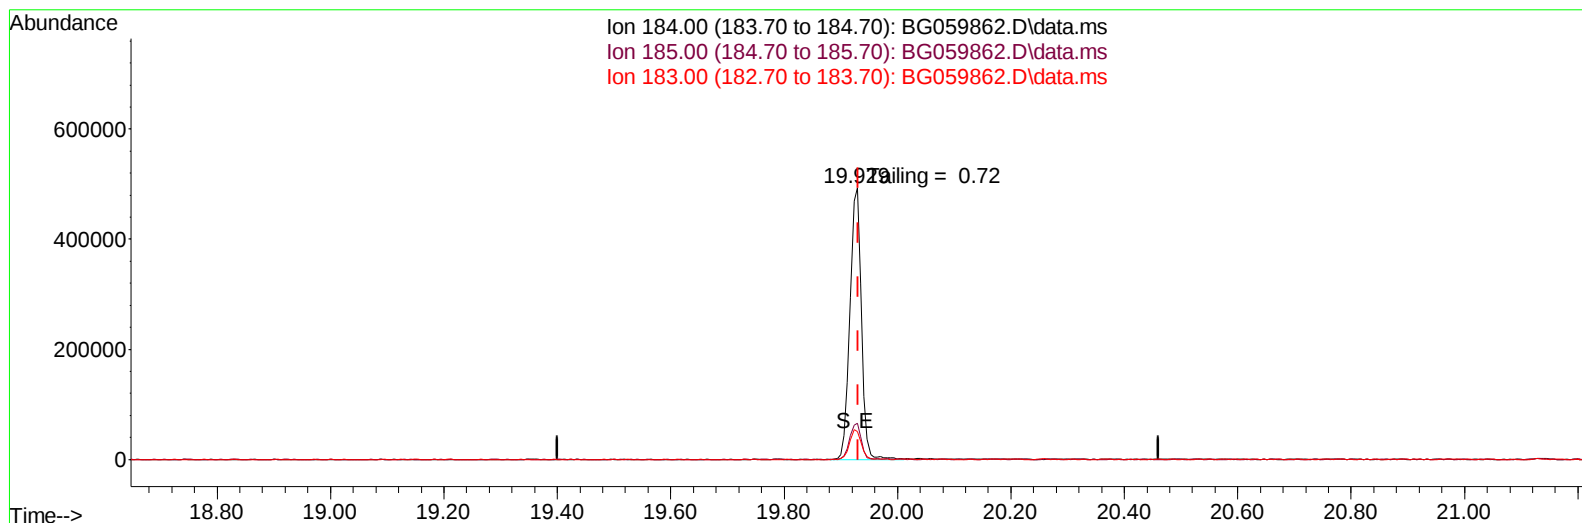

TIC: BG059862.D\data.ms

(77) Benzidine

19.929min (-0.001) 267351.38 ng

response 691113

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.45
183.00	11.00	10.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/24/2023	BNA_G	<u>BG059862.D</u>
Compound Name	Response	Retention Time
DDT	290679	21.133
DDD	5741	20.728
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5741	296420	1.94

Instrument :
BNA_G
ClientSampleId :
DFTPP