


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
Data File : BG059879.D
Acq On : 25 Nov 2023 5:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 27 13:17:45 2023

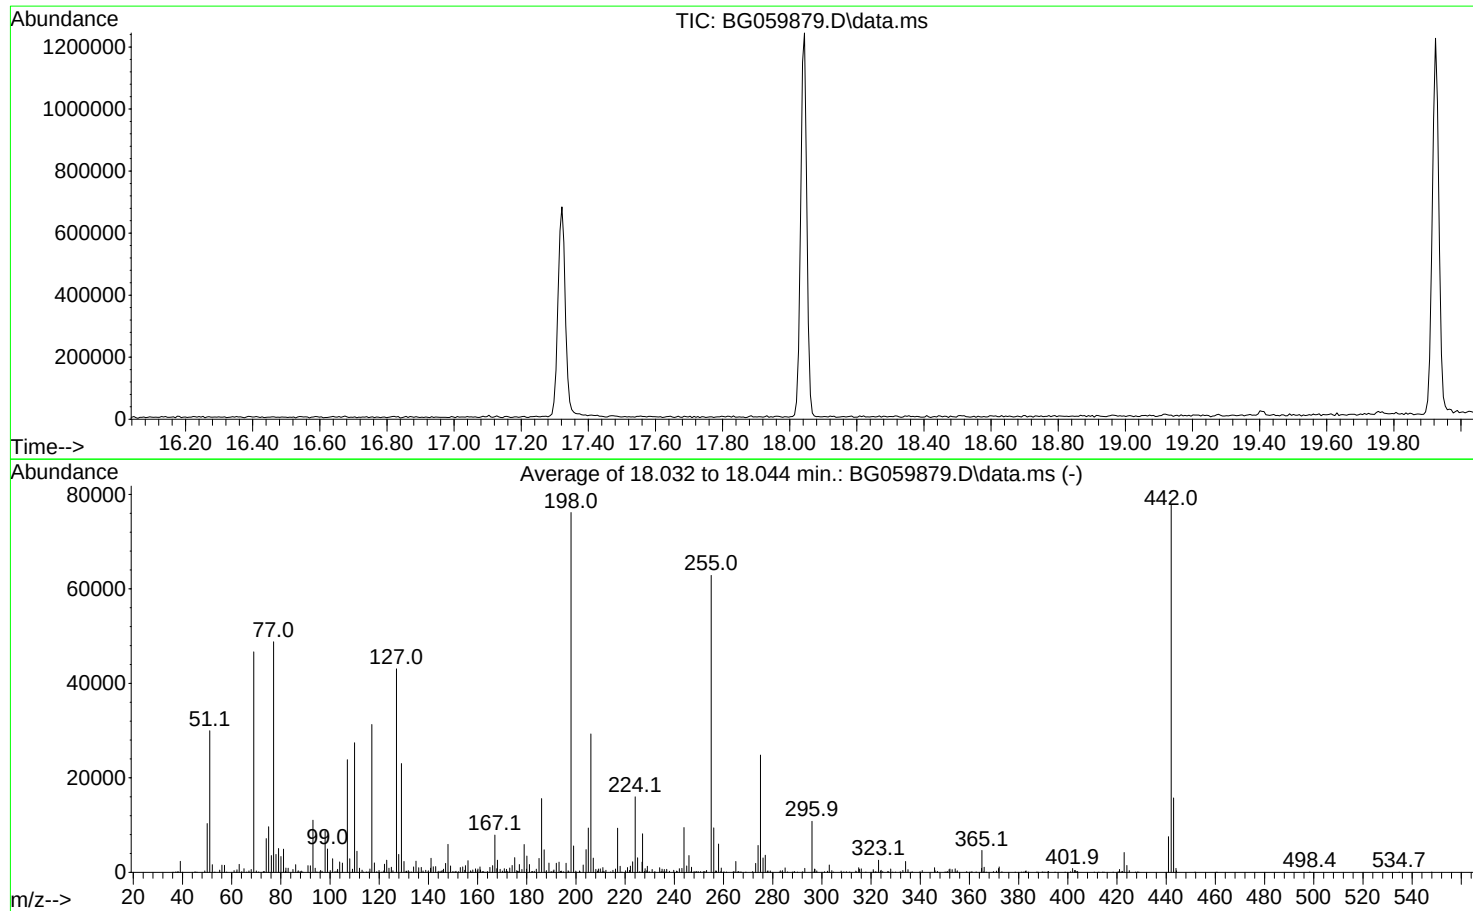




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	29981	PASS
68	69	0.00	2	1.3	612	PASS
69	198	0.00	100	61.3	46675	PASS
70	69	0.00	2	0.7	318	PASS
127	198	10	80	56.6	43080	PASS
197	198	0.00	2	0.5	351	PASS
198	198	100	100	100.0	76157	PASS
199	198	5	9	7.4	5601	PASS
275	198	10	60	32.6	24809	PASS
365	198	1	100	6.1	4639	PASS
441	198	0.01	100	9.9	7563	PASS
442	442	50	100	100.0	77856	PASS
443	442	15	24	20.2	15754	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
 Data File : BG059879.D
 Acq On : 25 Nov 2023 5:50
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 25 06:29:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 15:11:07 2023
 Response via : Initial Calibration

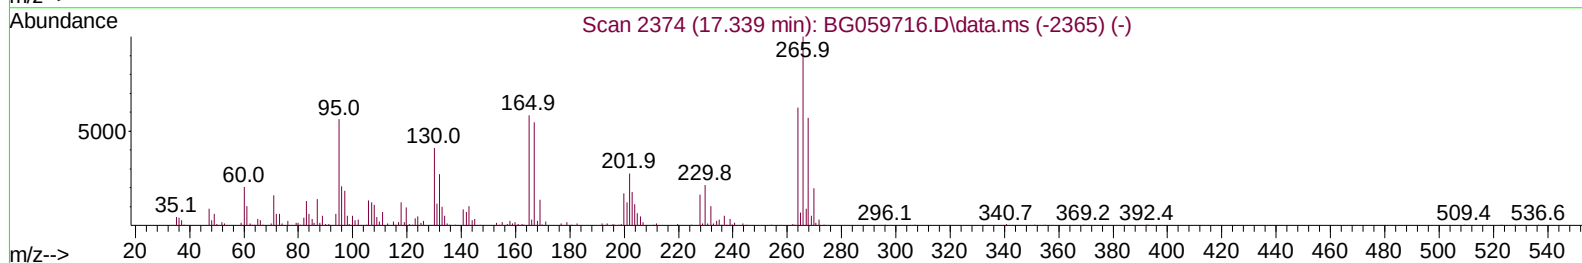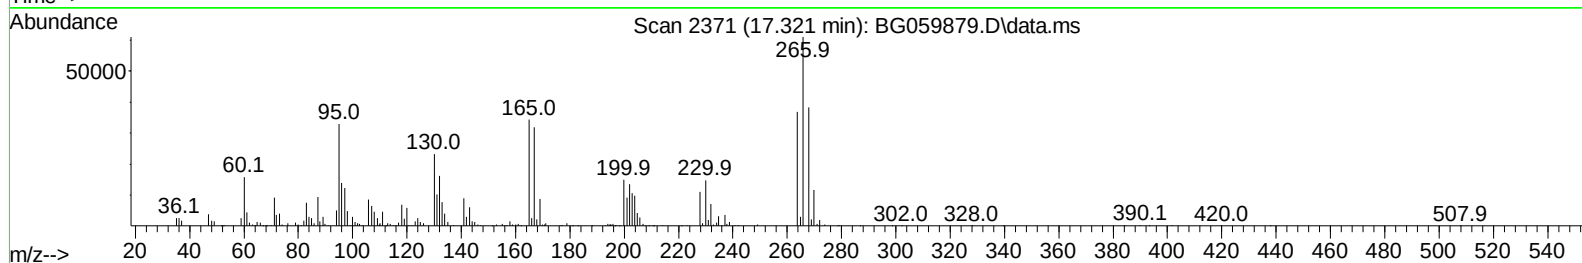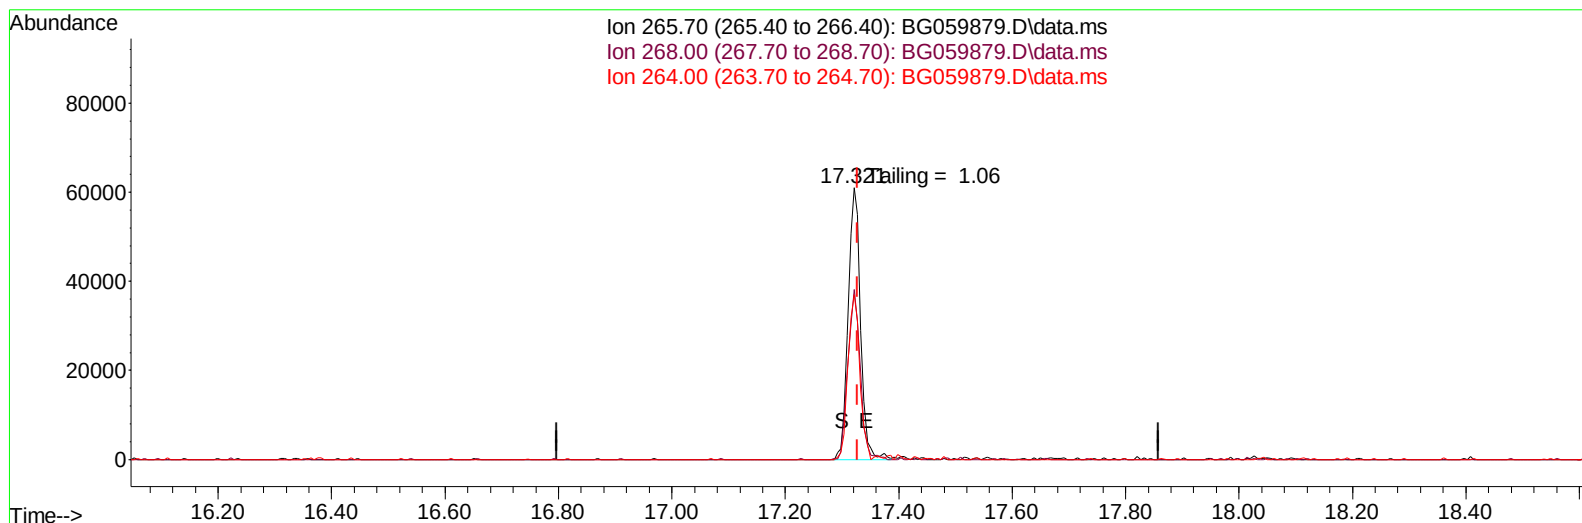

TIC: BG059879.D\data.ms

(70) Pentachlorophenol (C)

17.321min (-0.006) 109416.85 ng




response 91233

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	62.72
264.00	62.30	60.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112423\
 Data File : BG059879.D
 Acq On : 25 Nov 2023 5:50
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 25 06:29:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 15:11:07 2023
 Response via : Initial Calibration

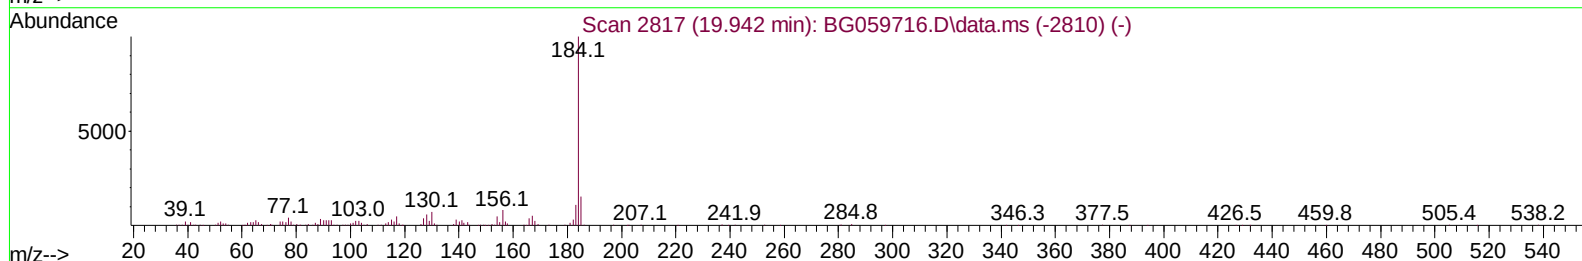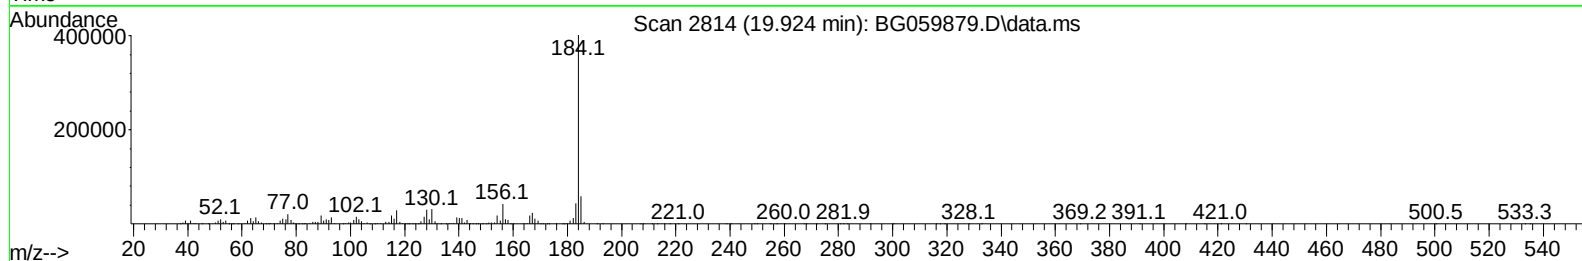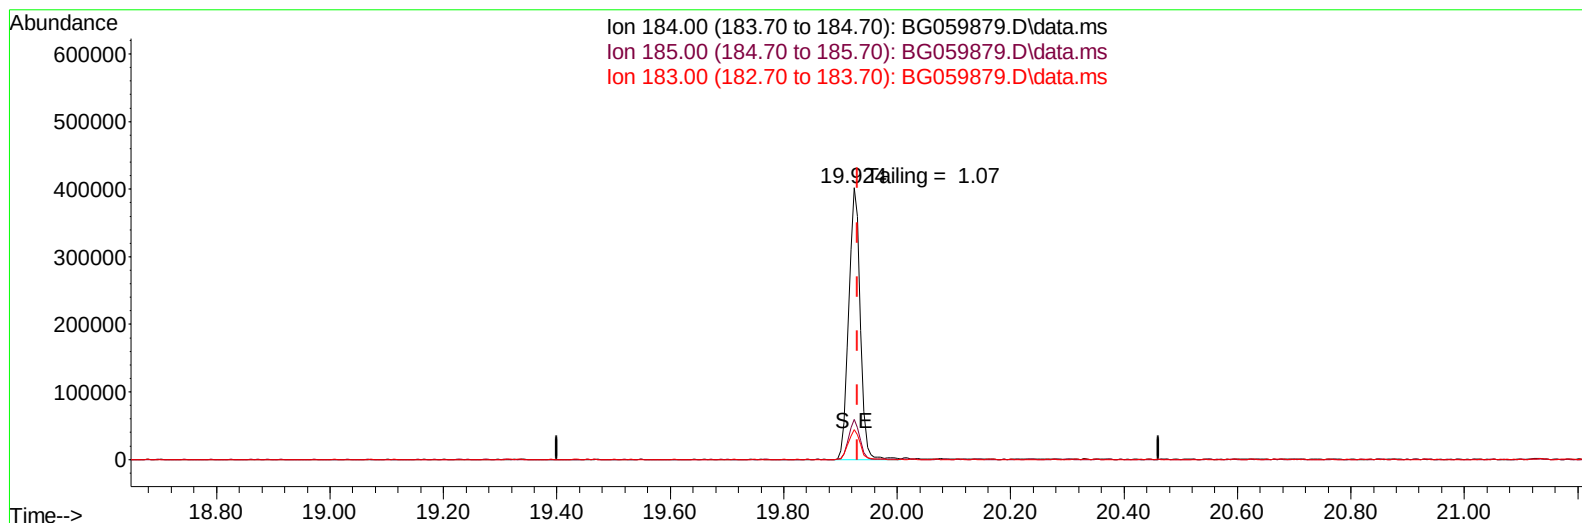

TIC: BG059879.D\data.ms

(77) Benzidine**19.924min (-0.006) 71201.58 ng****response 569936**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.64
183.00	11.00	11.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/24/2023	BNA_G	<u>BG059879.D</u>
Compound Name	Response	Retention Time
DDT	192745	21.128
DDD	43977	20.676
DDE	169	19.901
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44146	236891	18.64

Instrument :
BNA_G
ClientSampleId :
DFTPP