
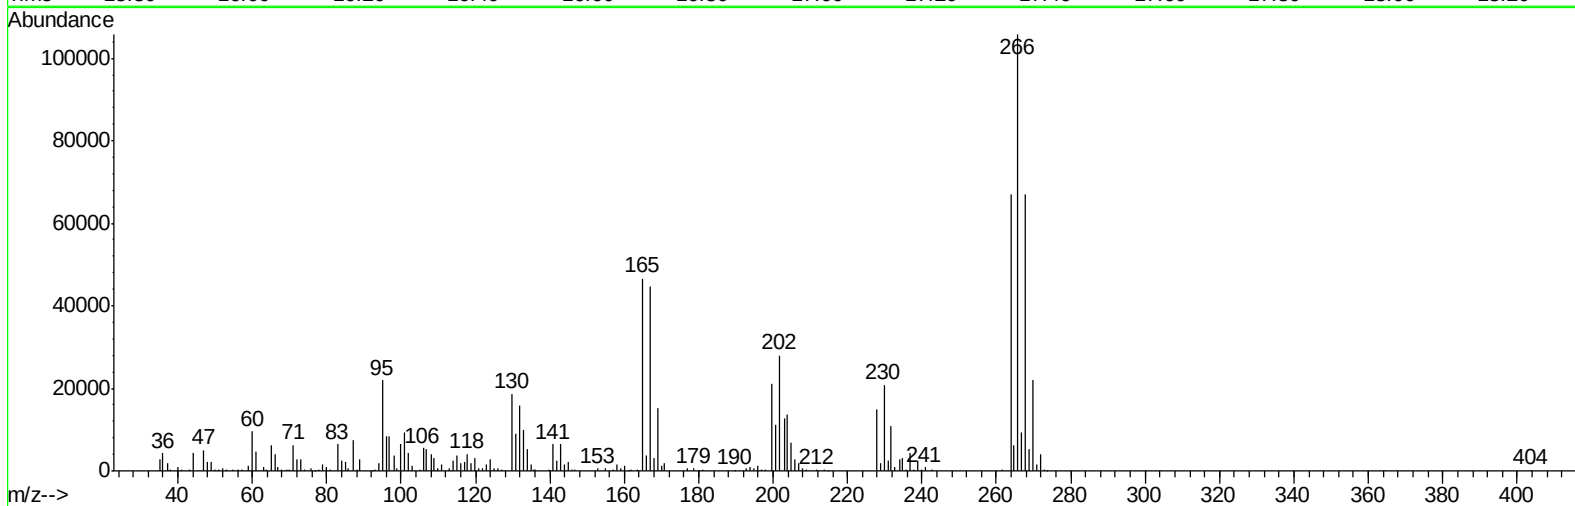


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112519\
Data File : BG043768.D
Acq On : 25 Nov 2019 13:31
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 02:27:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG112219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 23 00:54:00 2019
Response via : Initial Calibration

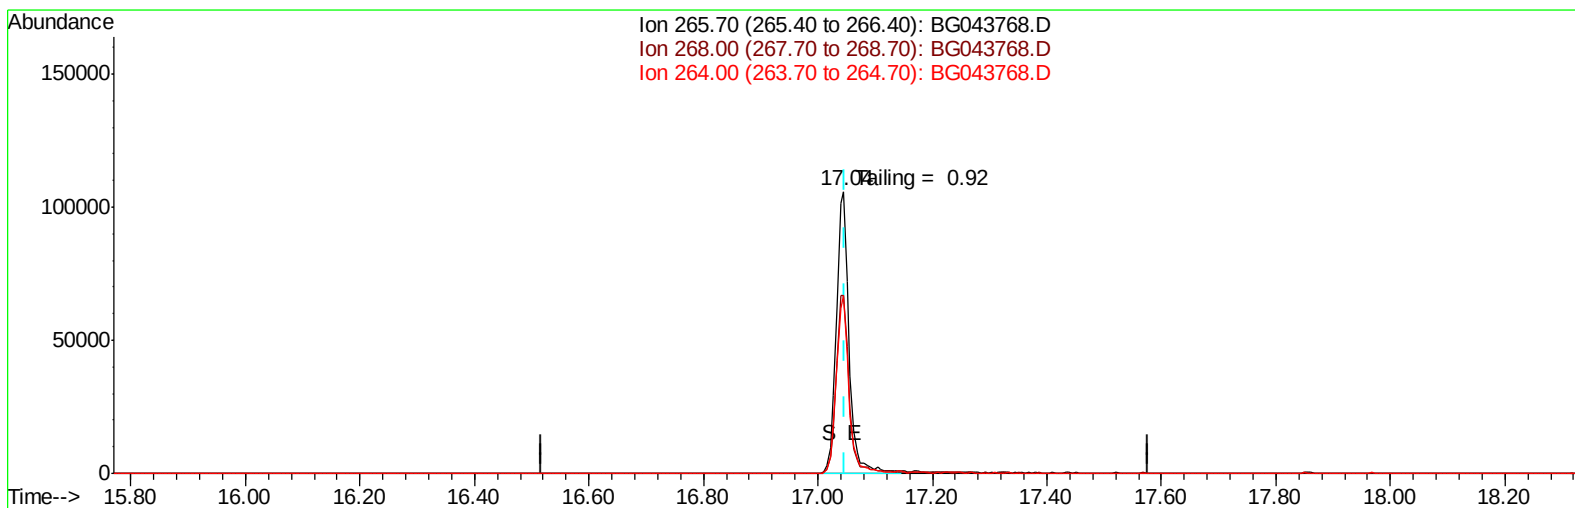

TIC: BG043768.D

(70) Pentachlorophenol (C)



17.045min (-0.002) 436568.56ng

response 165843

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	63.33
264.00	64.50	63.24
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112519\
Data File : BG043768.D
Acq On : 25 Nov 2019 13:31
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 02:27:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG112219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 23 00:54:00 2019
Response via : Initial Calibration

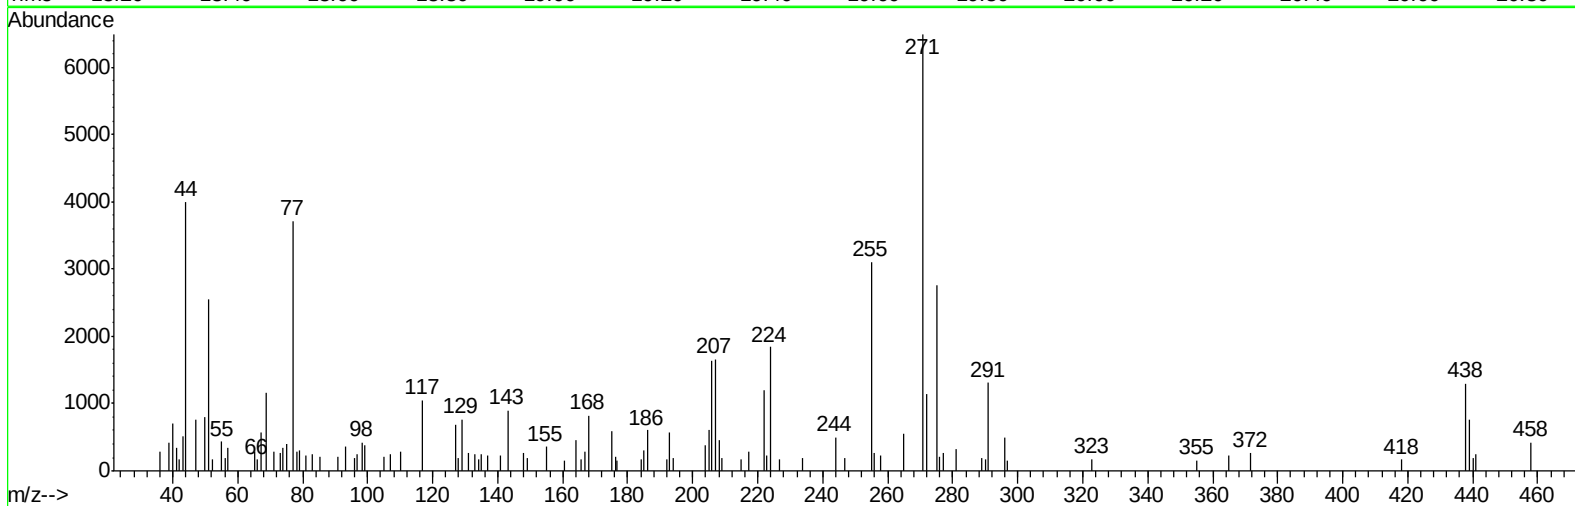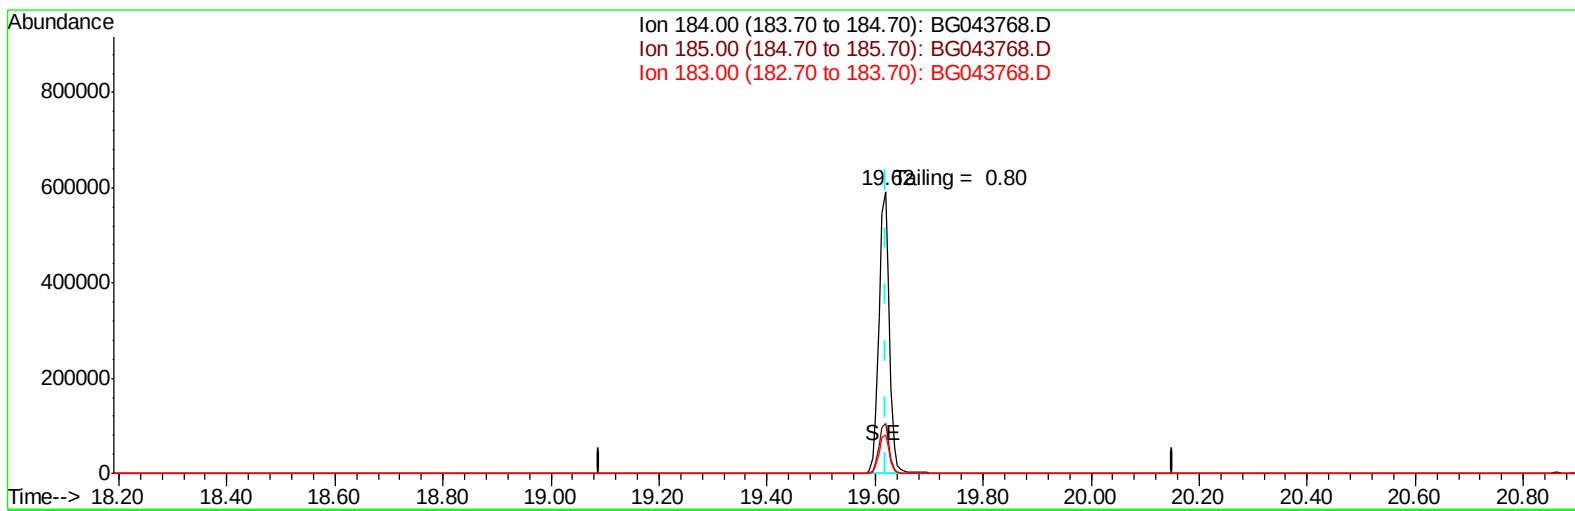

TIC: BG043768.D

(77) Benzidine

19.201min (-0.420) 0.32ng


response 59

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	180.24#
183.00	14.10	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112519\
Data File : BG043768.D
Acq On : 25 Nov 2019 13:31
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG112219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Nov 23 00:54:00 2019

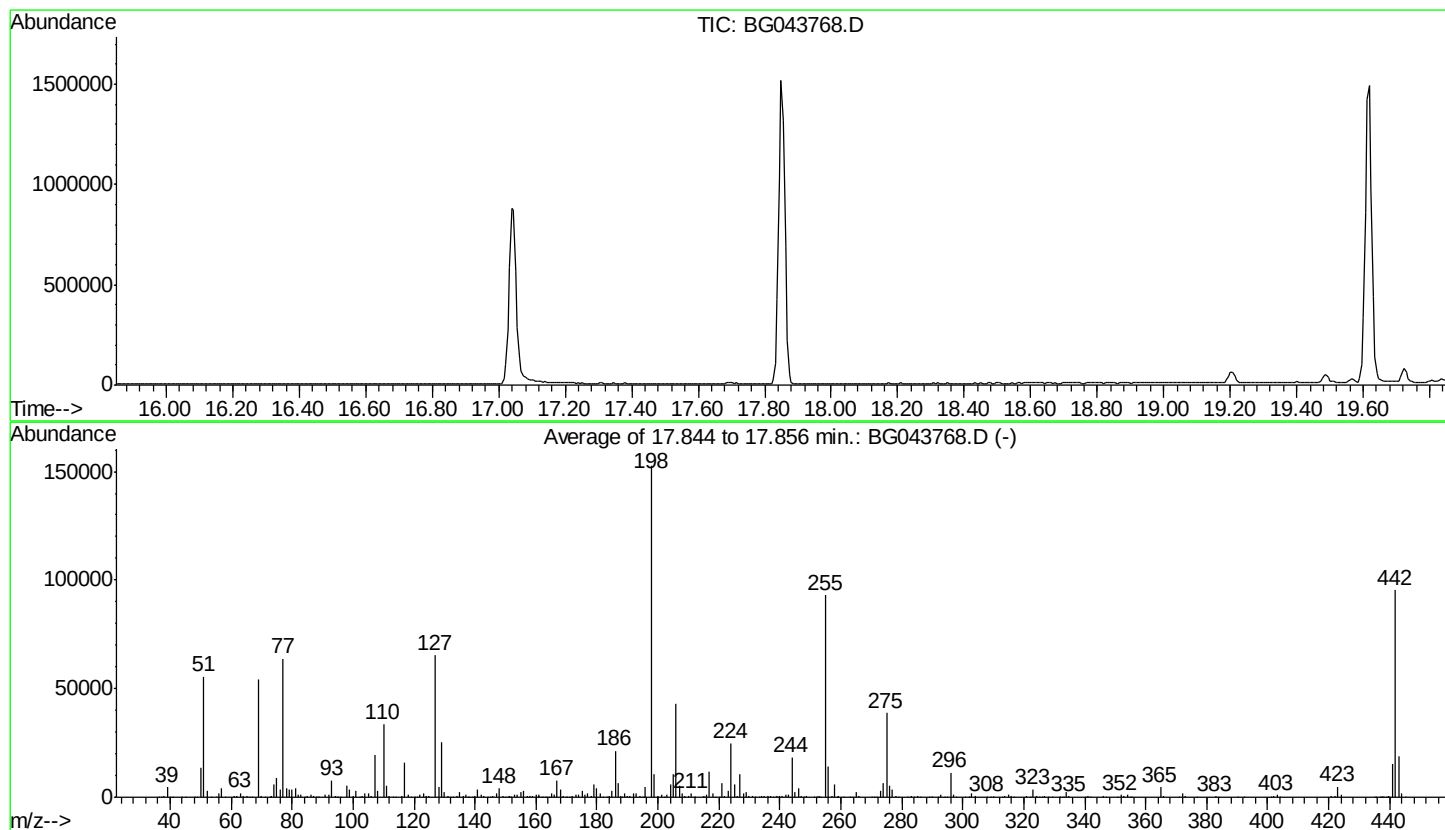

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	55468	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	54381	PASS
70	69	0.00	2	0.7	361	PASS
127	198	10	80	42.8	65392	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	152696	PASS
199	198	5	9	6.8	10392	PASS
275	198	10	60	25.4	38808	PASS
365	198	1	100	3.1	4712	PASS
441	198	0.01	100	10.2	15509	PASS
442	198	50	100	62.5	95424	PASS
443	442	15	24	20.1	19157	PASS