


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112519\
 Data File : BG043768.D
 Acq On : 25 Nov 2019 13:31
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG112219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 23 00:54:00 2019

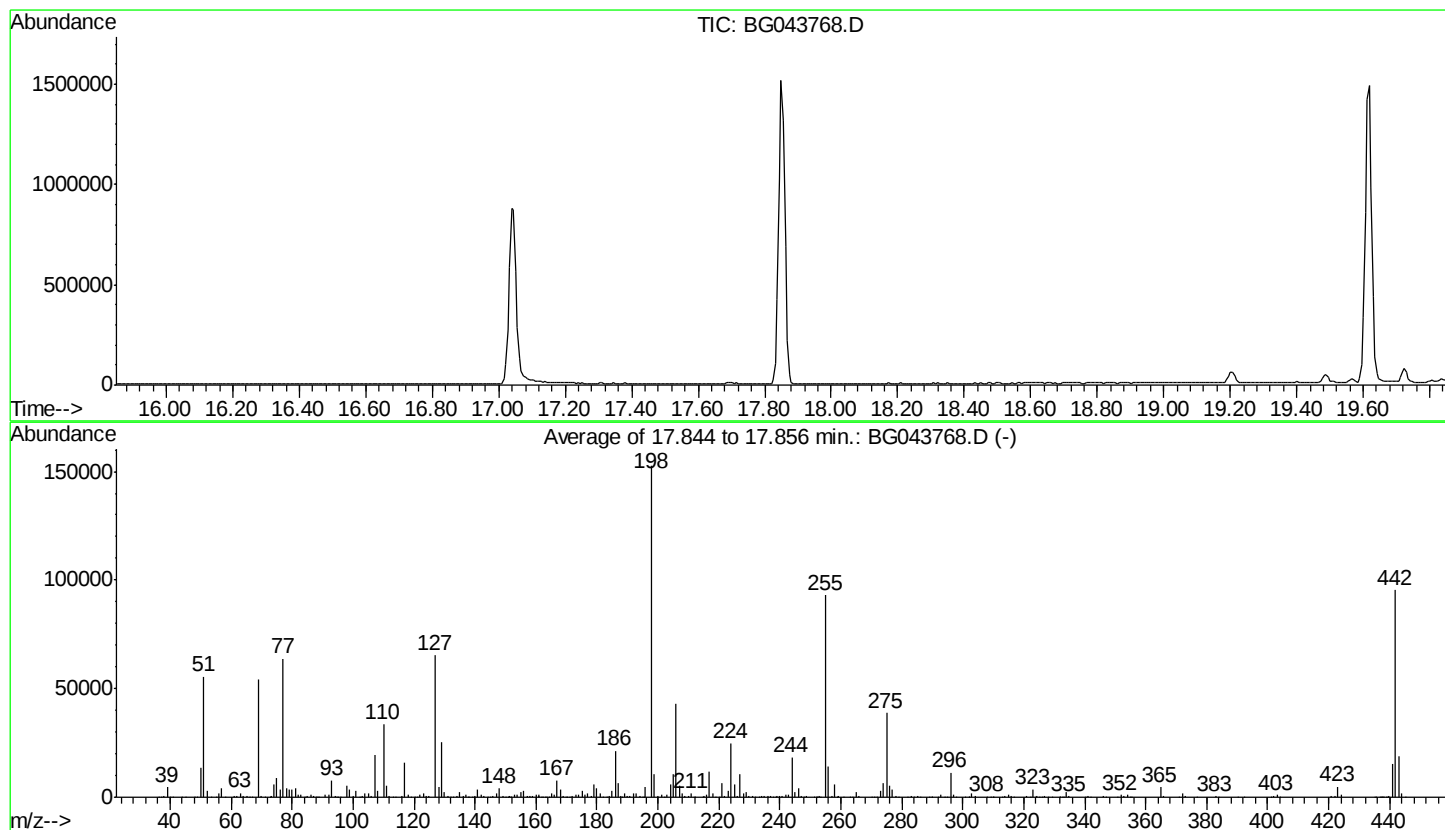

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	55468	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	54381	PASS
70	69	0.00	2	0.7	361	PASS
127	198	10	80	42.8	65392	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	152696	PASS
199	198	5	9	6.8	10392	PASS
275	198	10	60	25.4	38808	PASS
365	198	1	100	3.1	4712	PASS
441	198	0.01	100	10.2	15509	PASS
442	198	50	100	62.5	95424	PASS
443	442	15	24	20.1	19157	PASS