

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
 Data File : BG064859.D
 Acq On : 25 Nov 2025 13:52
 Operator : RC/JU
 Sample : Q3688-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 M-31S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG064859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.126	3	6	15	rVB	64629	114488	6.77%	0.873%
2	3.208	15	20	38	rVB	297625	493421	29.18%	3.761%
3	3.385	47	50	53	rVB3	1764	2364	0.14%	0.018%
4	3.479	63	66	73	rVB3	5765	7829	0.46%	0.060%
5	3.913	134	140	149	rBV	37529	65759	3.89%	0.501%
6	4.266	197	200	206	rBV4	1375	2661	0.16%	0.020%
7	4.765	280	285	291	rVB3	681	1713	0.10%	0.013%
8	5.400	386	393	401	rVB	14754	26268	1.55%	0.200%
9	7.298	710	716	727	rBV2	29870	60632	3.59%	0.462%
10	7.468	738	745	753	rBV	80438	138903	8.22%	1.059%
11	7.686	775	782	792	rBV	84770	160142	9.47%	1.221%
12	8.109	848	854	855	rBV2	1664	2607	0.15%	0.020%
13	8.156	855	862	870	rVV	122241	212899	12.59%	1.623%
14	8.855	972	981	987	rBV2	23941	46415	2.75%	0.354%
15	9.313	1053	1059	1071	rBV	95437	187325	11.08%	1.428%
16	10.042	1176	1183	1192	rBV	79247	156946	9.28%	1.196%
17	10.106	1192	1194	1201	rVB4	2021	2429	0.14%	0.019%
18	10.582	1268	1275	1288	rBV	112012	240158	14.20%	1.830%
19	10.676	1288	1291	1298	rVB5	4090	8290	0.49%	0.063%
20	10.847	1315	1320	1329	rVB3	1714	4821	0.29%	0.037%
21	10.970	1334	1341	1349	rBV	173753	320302	18.95%	2.441%
22	11.099	1355	1363	1384	rVB	61668	139735	8.27%	1.065%
23	11.781	1473	1479	1485	rBV3	16539	32872	1.94%	0.251%
24	11.851	1485	1491	1505	rVV2	32151	83708	4.95%	0.638%
25	12.550	1605	1610	1614	rVB2	1678	2522	0.15%	0.019%
26	14.160	1878	1884	1904	rBV	354995	570331	33.73%	4.347%
27	14.466	1928	1936	1947	rBV	328904	546227	32.31%	4.163%
28	14.765	1980	1987	1997	rBV	340729	541776	32.04%	4.129%
29	14.942	2012	2017	2028	rBV3	23070	58926	3.49%	0.449%
30	15.559	2117	2122	2127	rBV3	4126	6175	0.37%	0.047%
31	15.753	2148	2155	2166	rBV	526175	873537	51.67%	6.658%
32	15.852	2166	2172	2180	rBV	165502	270169	15.98%	2.059%
33	16.105	2208	2215	2220	rBV	21697	34305	2.03%	0.261%
34	16.140	2220	2221	2226	rVB	2125	1758	0.10%	0.013%
35	16.669	2303	2311	2316	rBV4	6218	10367	0.61%	0.079%
36	17.028	2368	2372	2373	rBV2	1693	1857	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
 Data File : BG064859.D
 Acq On : 25 Nov 2025 13:52
 Operator : RC/JU
 Sample : Q3688-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 M-31S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
 Title : SVOA CALIBRATION

37	17.368	2425	2430	2433	rBV3	4852	7852	0.46%	0.060%
38	17.498	2444	2452	2462	rBV2	465813	763962	45.19%	5.823%
39	17.592	2462	2468	2487	rVB	694941	1142970	67.60%	8.712%
40	18.079	2547	2551	2554	rBV2	1260	1710	0.10%	0.013%
41	18.150	2556	2563	2571	rVV5	5433	9484	0.56%	0.072%
42	18.367	2596	2600	2607	rBV3	11513	18462	1.09%	0.141%
43	18.443	2611	2613	2618	rVB2	2435	3140	0.19%	0.024%
44	18.720	2655	2660	2662	rBV6	2676	4416	0.26%	0.034%
45	18.755	2665	2666	2671	rBV4	2439	3035	0.18%	0.023%
46	18.867	2683	2685	2689	rVB3	3223	3864	0.23%	0.029%
47	19.213	2740	2744	2749	rBV3	4133	6712	0.40%	0.051%
48	19.272	2752	2754	2756	rBV3	2107	1964	0.12%	0.015%
49	19.436	2776	2782	2787	rVB3	11933	18069	1.07%	0.138%
50	19.501	2788	2793	2798	rBV2	11348	18700	1.11%	0.143%
51	19.595	2806	2809	2812	rBV5	2317	3196	0.19%	0.024%
52	19.624	2812	2814	2820	rVB6	3550	6261	0.37%	0.048%
53	19.777	2838	2840	2843	rBV3	2355	2138	0.13%	0.016%
54	19.865	2848	2855	2869	rBV	1130039	1690683	100.00%	12.886%
55	20.036	2883	2884	2890	rVB6	2770	3844	0.23%	0.029%
56	20.089	2890	2893	2895	rBV4	2168	2872	0.17%	0.022%
57	20.377	2938	2942	2945	rBV5	3019	3905	0.23%	0.030%
58	20.488	2959	2961	2963	rBV3	2501	1820	0.11%	0.014%
59	20.606	2979	2981	2983	rBV3	2863	1827	0.11%	0.014%
60	20.694	2994	2996	2998	rBV2	3078	2982	0.18%	0.023%
61	21.381	3108	3113	3118	rBV7	10699	22307	1.32%	0.170%
62	21.740	3167	3174	3188	rBV2	549040	1034604	61.19%	7.886%
63	21.934	3203	3207	3213	rVB9	6083	12118	0.72%	0.092%
64	22.539	3307	3310	3317	rVB9	12656	22393	1.32%	0.171%
65	23.438	3458	3463	3471	rVB9	16447	38220	2.26%	0.291%
66	24.066	3565	3570	3576	rVB6	15095	29274	1.73%	0.223%
67	24.366	3619	3621	3623	rBV3	4119	3758	0.22%	0.029%
68	24.771	3678	3690	3708	rBV	534011	1557067	92.10%	11.868%
69	24.995	3717	3728	3750	rVB	373663	1160064	68.62%	8.842%
70	25.758	3856	3858	3859	rBV2	3426	2845	0.17%	0.022%
71	25.829	3867	3870	3871	rBV2	8865	8221	0.49%	0.063%
72	25.935	3886	3888	3890	rBV3	3647	3165	0.19%	0.024%
73	27.521	4148	4158	4159	rBV8	12860	35751	2.11%	0.272%
74	28.649	4348	4350	4352	rBV3	3743	3679	0.22%	0.028%
75	28.726	4361	4363	4367	rBV5	4388	6618	0.39%	0.050%
76	29.207	4443	4445	4446	rBV2	6899	6270	0.37%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064859.D
Acq On : 25 Nov 2025 13:52
Operator : RC/JU
Sample : Q3688-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
M-31S

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Title : SVOA CALIBRATION

77	30.106	4596	4598	4600	rBV3	3997	3589	0.21%	0.027%
78	31.223	4784	4788	4792	rBV6	6397	12790	0.76%	0.097%
79	31.757	4877	4879	4881	rVB3	3671	2635	0.16%	0.020%




Sum of corrected areas: 13119873

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064859.D
Acq On : 25 Nov 2025 13:52
Operator : RC/JU
Sample : Q3688-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
M-31S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

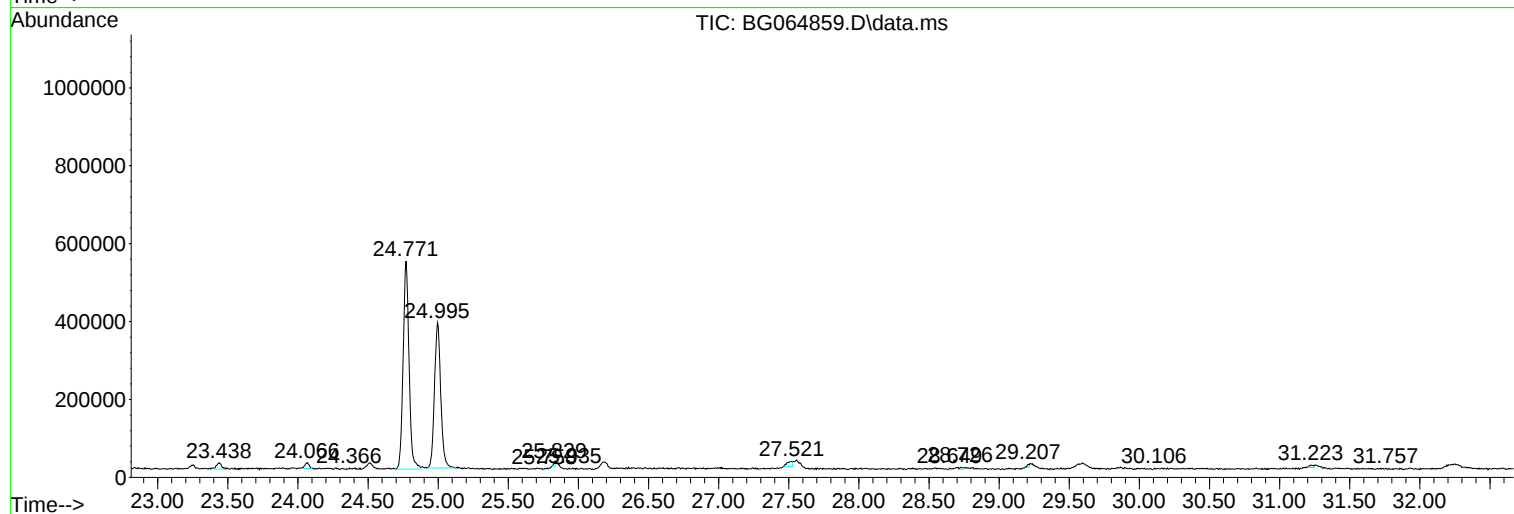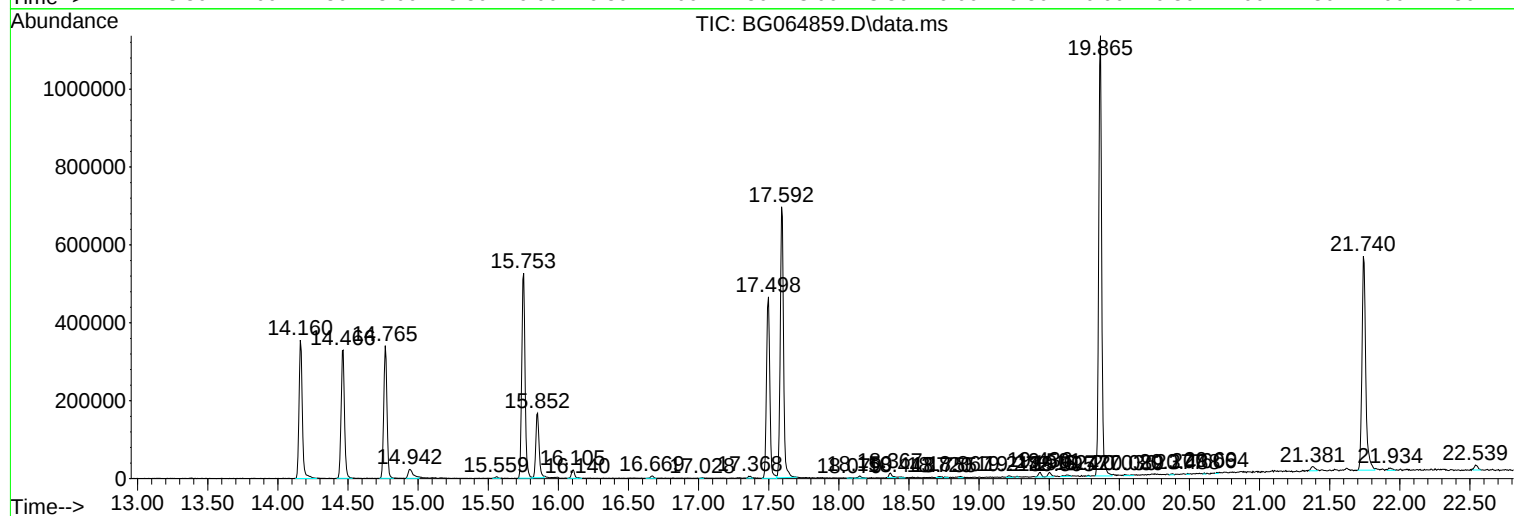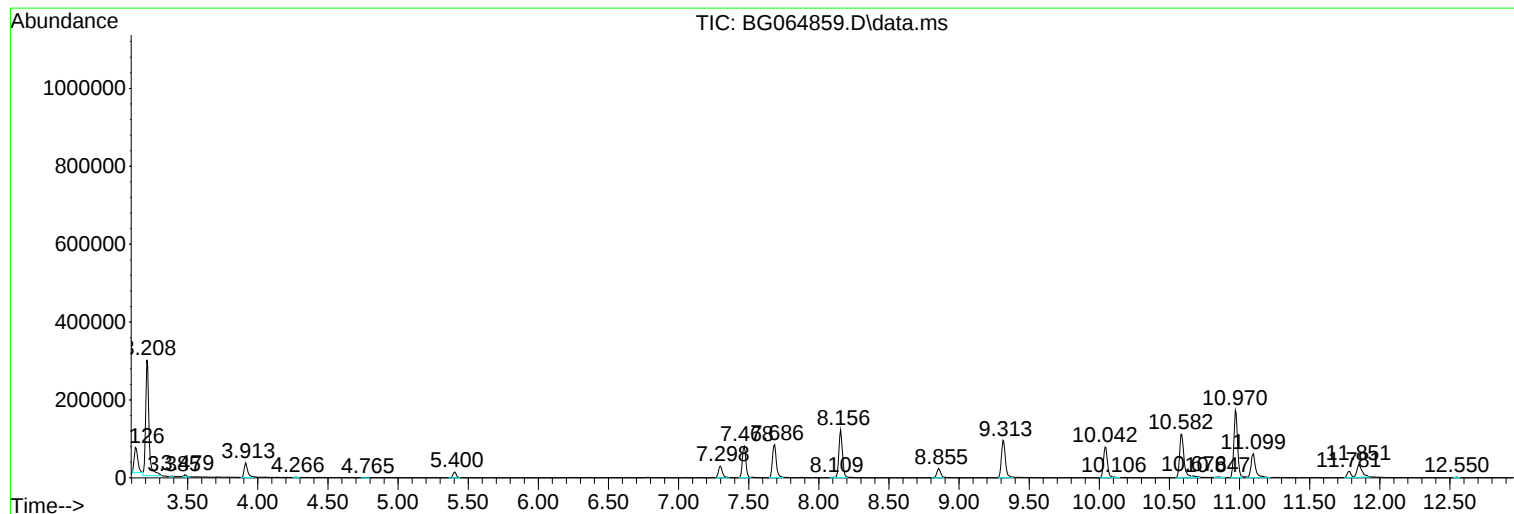

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064859.D
Acq On : 25 Nov 2025 13:52
Operator : RC/JU
Sample : Q3688-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
M-31S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064859.D
Acq On : 25 Nov 2025 13:52
Operator : RC/JU
Sample : Q3688-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
M-31S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc