

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
 Data File : BG064883.D
 Acq On : 26 Nov 2025 10:54
 Operator : RC/JU
 Sample : PB170721BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG064883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	13	rVB3	5275	9667	0.79%	0.100%
2	3.206	15	20	27	rVB	19624	30004	2.46%	0.310%
3	3.476	61	66	73	rVV	11645	17572	1.44%	0.182%
4	3.905	133	139	155	rBV	86559	145710	11.93%	1.507%
5	4.257	196	199	205	rVB	1600	1734	0.14%	0.018%
6	7.295	709	716	734	rBV	92332	175910	14.40%	1.819%
7	7.459	738	744	756	rVV	57764	103209	8.45%	1.067%
8	7.677	775	781	792	rBV2	94310	173521	14.21%	1.794%
9	8.147	855	861	872	rBV	78293	137587	11.27%	1.423%
10	8.846	973	980	991	rBV	115926	217092	17.78%	2.245%
11	9.310	1052	1059	1069	rBV2	87890	160260	13.12%	1.657%
12	10.039	1176	1183	1195	rVB	81273	145517	11.92%	1.505%
13	10.585	1268	1276	1287	rBV	118723	231606	18.97%	2.395%
14	10.967	1333	1341	1349	rBV	107102	195915	16.04%	2.026%
15	11.090	1354	1362	1372	rBV	104007	206324	16.90%	2.133%
16	12.542	1606	1609	1611	rBV	1319	1497	0.12%	0.015%
17	14.163	1878	1885	1901	rBV	255627	417984	34.23%	4.322%
18	14.463	1930	1936	1945	rBV2	294528	474567	38.86%	4.907%
19	14.768	1981	1988	1996	rBV	208754	342918	28.08%	3.546%
20	14.939	2010	2017	2032	rBV	73131	160741	13.16%	1.662%
21	15.750	2148	2155	2167	rBV	416976	655568	53.68%	6.778%
22	15.850	2167	2172	2185	rVV	99297	167482	13.71%	1.732%
23	15.985	2192	2195	2201	rVV3	1971	2847	0.23%	0.029%
24	17.283	2414	2416	2420	rVB2	1133	1293	0.11%	0.013%
25	17.495	2446	2452	2462	rBV	321828	490060	40.13%	5.067%
26	17.595	2462	2469	2483	rVV	517641	811615	66.46%	8.392%
27	17.683	2483	2484	2488	rVB3	1329	1290	0.11%	0.013%
28	17.888	2516	2519	2522	rBV2	1316	1826	0.15%	0.019%
29	18.441	2610	2613	2620	rBV2	595	1409	0.12%	0.015%
30	19.434	2777	2782	2786	rBV4	7497	11978	0.98%	0.124%
31	19.504	2790	2794	2797	rVV	5822	8319	0.68%	0.086%
32	19.533	2797	2799	2804	rVB5	2697	4049	0.33%	0.042%
33	19.569	2804	2805	2811	rBV4	1218	2019	0.17%	0.021%
34	19.774	2836	2840	2847	rVB4	2290	3949	0.32%	0.041%
35	19.863	2849	2855	2871	rVV	750812	1093277	89.52%	11.304%
36	20.133	2898	2901	2902	rBV	1782	1786	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
 Data File : BG064883.D
 Acq On : 26 Nov 2025 10:54
 Operator : RC/JU
 Sample : PB170721BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
 Title : SVOA CALIBRATION

37	20.215	2912	2915	2916	rBV4	2030	1872	0.15%	0.019%
38	20.350	2936	2938	2939	rBV	1530	1325	0.11%	0.014%
39	20.756	3004	3007	3009	rBV4	1682	1930	0.16%	0.020%
40	20.803	3013	3015	3021	rVB6	2471	3456	0.28%	0.036%

41	21.061	3057	3059	3062	rBV4	1977	2476	0.20%	0.026%
42	21.096	3064	3065	3068	rBV3	2199	1780	0.15%	0.018%
43	21.267	3092	3094	3095	rVB2	2255	1558	0.13%	0.016%
44	21.314	3098	3102	3106	rVV6	2871	4195	0.34%	0.043%
45	21.496	3131	3133	3137	rBV4	1894	1758	0.14%	0.018%

46	21.749	3169	3176	3191	rBV	381551	713436	58.42%	7.377%
47	21.931	3202	3207	3210	rBV4	4925	6389	0.52%	0.066%
48	22.548	3304	3312	3317	rBV4	9010	19133	1.57%	0.198%
49	22.747	3344	3346	3349	rBV3	1644	2069	0.17%	0.021%
50	23.253	3424	3432	3438	rBV4	16743	36524	2.99%	0.378%

51	23.347	3446	3448	3452	rVB5	2917	2290	0.19%	0.024%
52	23.846	3531	3533	3534	rBV2	1802	1643	0.13%	0.017%
53	24.069	3564	3571	3578	rVB4	19560	46271	3.79%	0.478%
54	24.304	3609	3611	3613	rBV3	1871	2015	0.17%	0.021%
55	24.686	3674	3676	3677	rBV2	2718	2174	0.18%	0.022%

56	24.780	3680	3692	3709	rVV	419657	1221198	100.00%	12.627%
57	24.998	3718	3729	3745	rVB2	250405	797386	65.30%	8.245%
58	25.415	3798	3800	3801	rBV	2102	1300	0.11%	0.013%
59	25.709	3849	3850	3853	rBV3	3053	3152	0.26%	0.033%
60	25.803	3864	3866	3867	rBV2	1995	1682	0.14%	0.017%

61	25.826	3868	3870	3874	rVV3	3158	4483	0.37%	0.046%
62	26.190	3923	3932	3939	rVB5	19903	59065	4.84%	0.611%
63	26.302	3949	3951	3955	rVB5	2186	2915	0.24%	0.030%
64	26.337	3955	3957	3959	rBV3	2286	1949	0.16%	0.020%
65	26.707	4016	4020	4022	rBV5	2394	4024	0.33%	0.042%

66	26.749	4026	4027	4029	rBV2	1922	1866	0.15%	0.019%
67	27.177	4098	4100	4102	rBV3	2387	2327	0.19%	0.024%
68	27.289	4117	4119	4120	rBV2	2689	2111	0.17%	0.022%
69	27.365	4130	4132	4133	rBV2	2220	1811	0.15%	0.019%
70	27.448	4144	4146	4147	rBV2	2240	1926	0.16%	0.020%

71	27.495	4152	4154	4155	rBV	4029	1995	0.16%	0.021%
72	27.559	4158	4165	4166	rBV5	17776	30086	2.46%	0.311%
73	27.712	4189	4191	4195	rBV4	1716	1700	0.14%	0.018%
74	27.947	4229	4231	4233	rBV3	2015	1308	0.11%	0.014%
75	28.082	4252	4254	4256	rBV3	1872	1643	0.13%	0.017%

76	28.370	4299	4303	4304	rBV4	2549	3504	0.29%	0.036%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
 Data File : BG064883.D
 Acq On : 26 Nov 2025 10:54
 Operator : RC/JU
 Sample : PB170721BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
 Title : SVOA CALIBRATION

77	28.476	4320	4321	4323	rBV2	2424	1775	0.15%	0.018%
78	29.022	4413	4414	4418	rVV4	2021	1768	0.14%	0.018%
79	29.181	4438	4441	4442	rBV3	4138	4520	0.37%	0.047%
80	29.210	4442	4446	4447	rBV4	9089	10634	0.87%	0.110%
81	29.387	4474	4476	4477	rBV	3354	1606	0.13%	0.017%
82	29.833	4551	4552	4553	rBV	2596	1497	0.12%	0.015%
83	29.957	4571	4573	4574	rBV2	1917	1279	0.10%	0.013%
84	30.051	4587	4589	4590	rBV2	2807	1660	0.14%	0.017%
85	30.139	4601	4604	4607	rBV5	2544	4222	0.35%	0.044%
86	30.309	4632	4633	4637	rVB4	2783	2193	0.18%	0.023%
87	30.338	4637	4638	4640	rBV2	2670	1772	0.15%	0.018%
88	30.938	4738	4740	4742	rVB2	2282	1770	0.14%	0.018%
89	30.961	4742	4744	4745	rBV2	2107	1349	0.11%	0.014%
90	30.997	4748	4750	4753	rVB5	2055	2060	0.17%	0.021%
91	31.185	4778	4782	4783	rBV3	5641	5962	0.49%	0.062%
92	31.232	4788	4790	4792	rVV2	3918	3921	0.32%	0.041%
93	31.343	4807	4809	4812	rBV4	2031	2616	0.21%	0.027%
94	31.414	4818	4821	4822	rBV2	2377	2605	0.21%	0.027%
95	31.508	4835	4837	4839	rVB2	2231	1415	0.12%	0.015%
96	31.737	4874	4876	4878	rBV3	2288	1790	0.15%	0.019%
97	31.760	4878	4880	4884	rVV5	2023	1550	0.13%	0.016%
98	31.989	4918	4919	4921	rVB2	2204	1455	0.12%	0.015%
99	32.595	5020	5022	5025	rVB5	2114	2103	0.17%	0.022%
100	32.624	5025	5027	5030	rBV4	1741	2123	0.17%	0.022%




Sum of corrected areas: 9671472

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064883.D
Acq On : 26 Nov 2025 10:54
Operator : RC/JU
Sample : PB170721BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

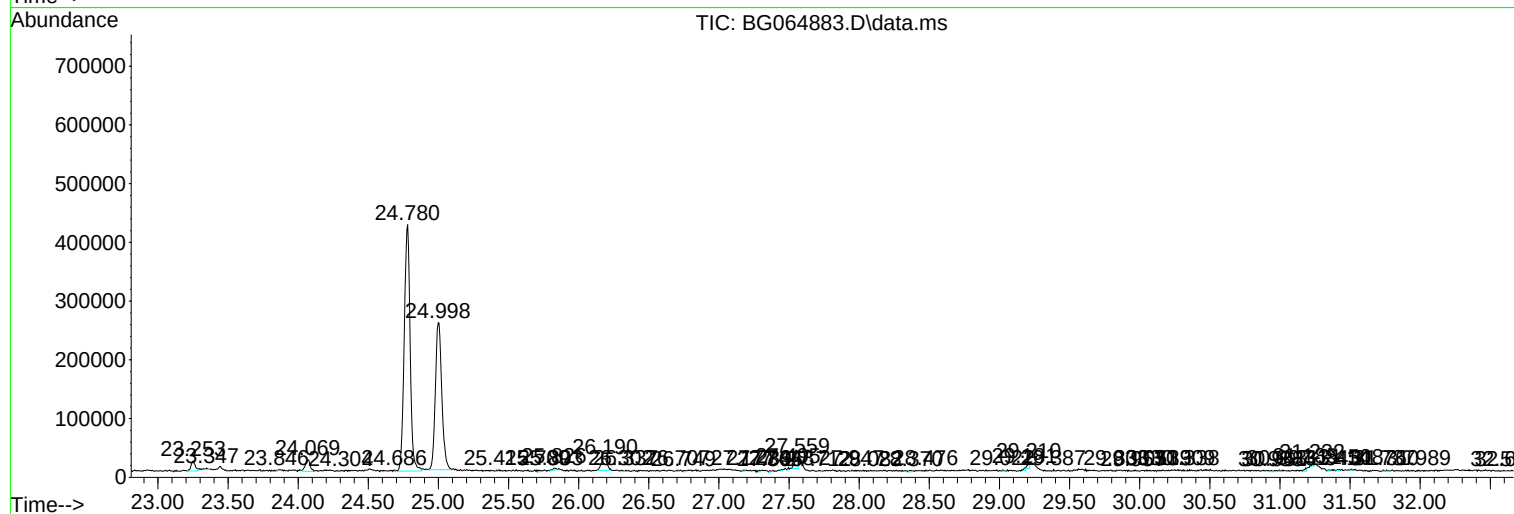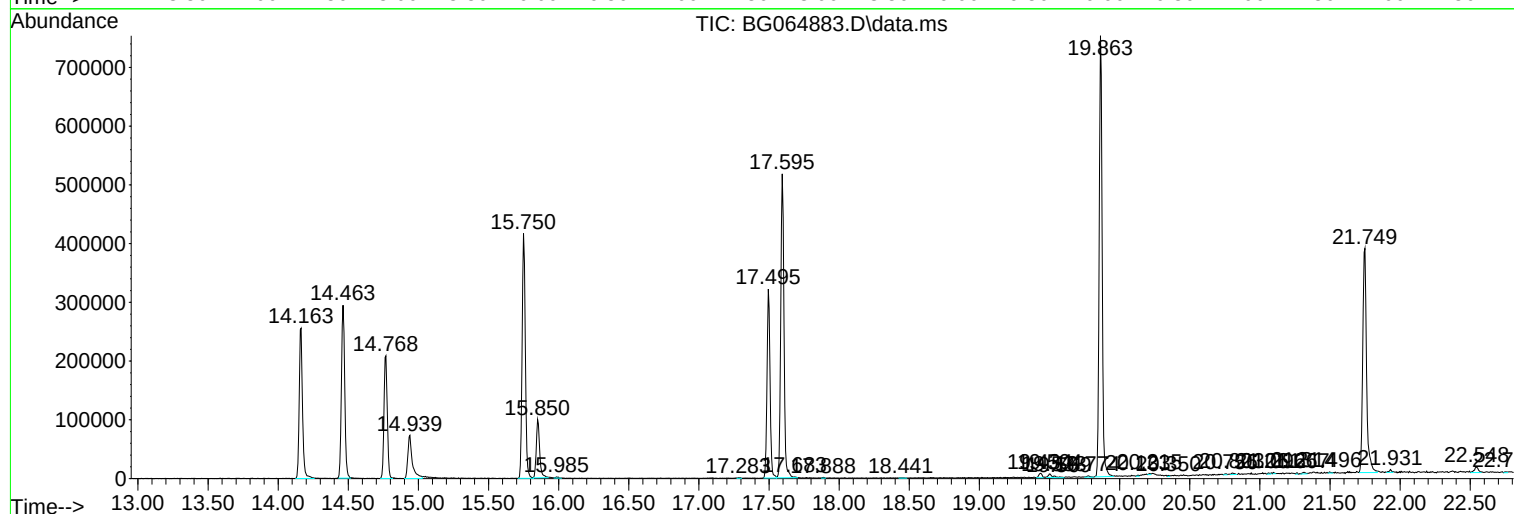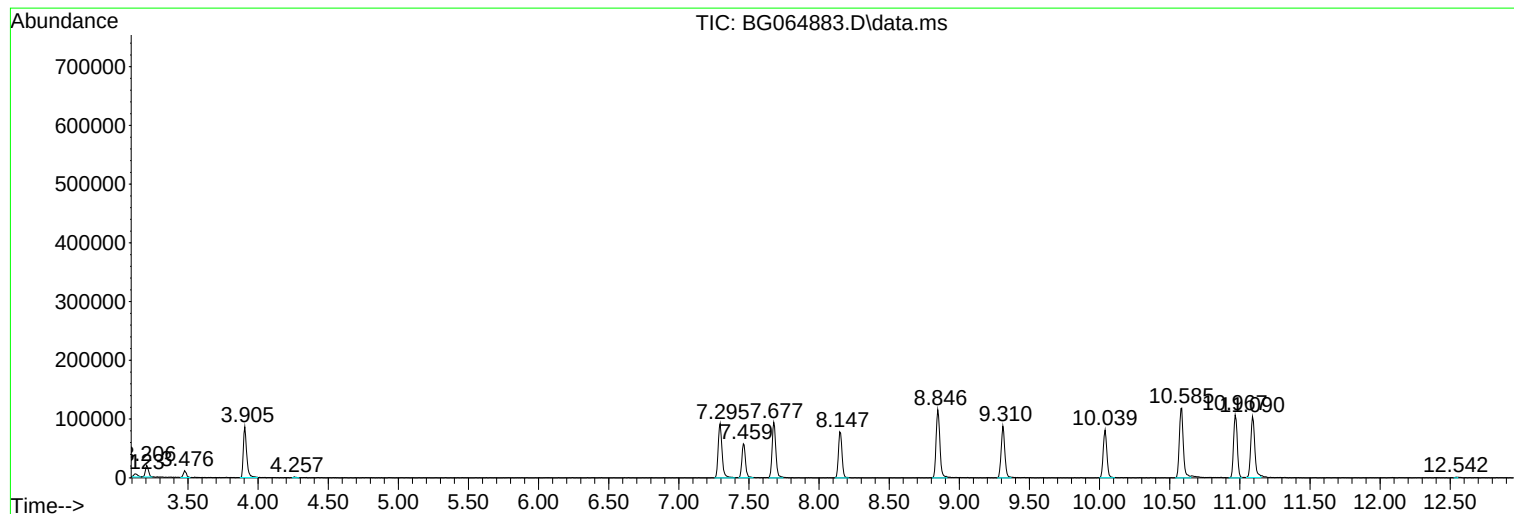

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064883.D
Acq On : 26 Nov 2025 10:54
Operator : RC/JU
Sample : PB170721BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064883.D
Acq On : 26 Nov 2025 10:54
Operator : RC/JU
Sample : PB170721BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc