
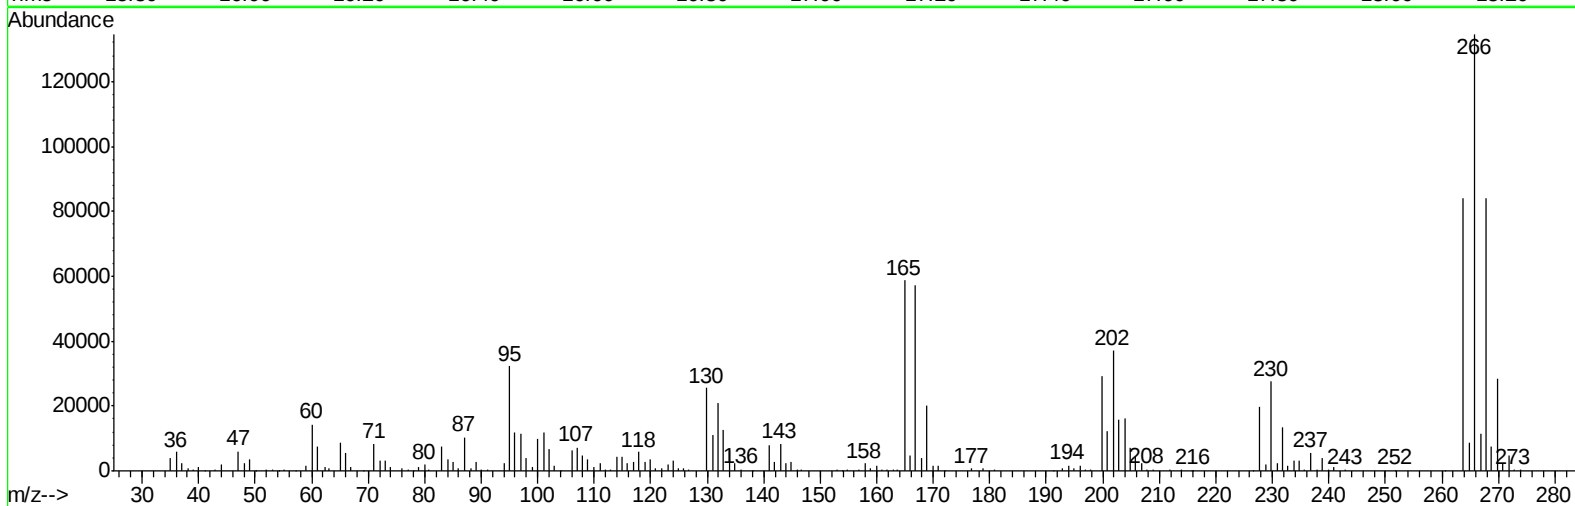


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112619\  
Data File : BG043777.D  
Acq On : 26 Nov 2019 14:35  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 07:34:05 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG112219.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Nov 23 00:54:00 2019  
Response via : Initial Calibration

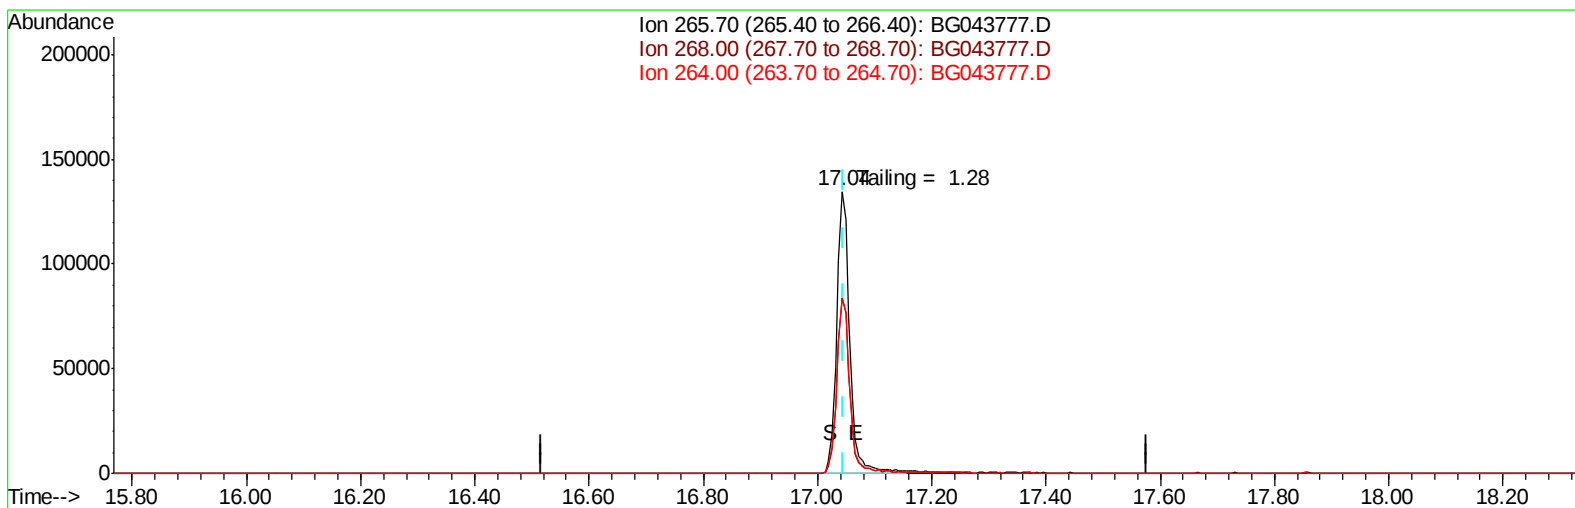

TIC: BG043777.D

(70) Pentachlorophenol (C)



17.043min (-0.005) 546355.01ng

response 211392

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.10 | 62.39 |
| 264.00 | 64.50 | 62.45 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112619\  
Data File : BG043777.D  
Acq On : 26 Nov 2019 14:35  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 07:34:05 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG112219.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Nov 23 00:54:00 2019  
Response via : Initial Calibration

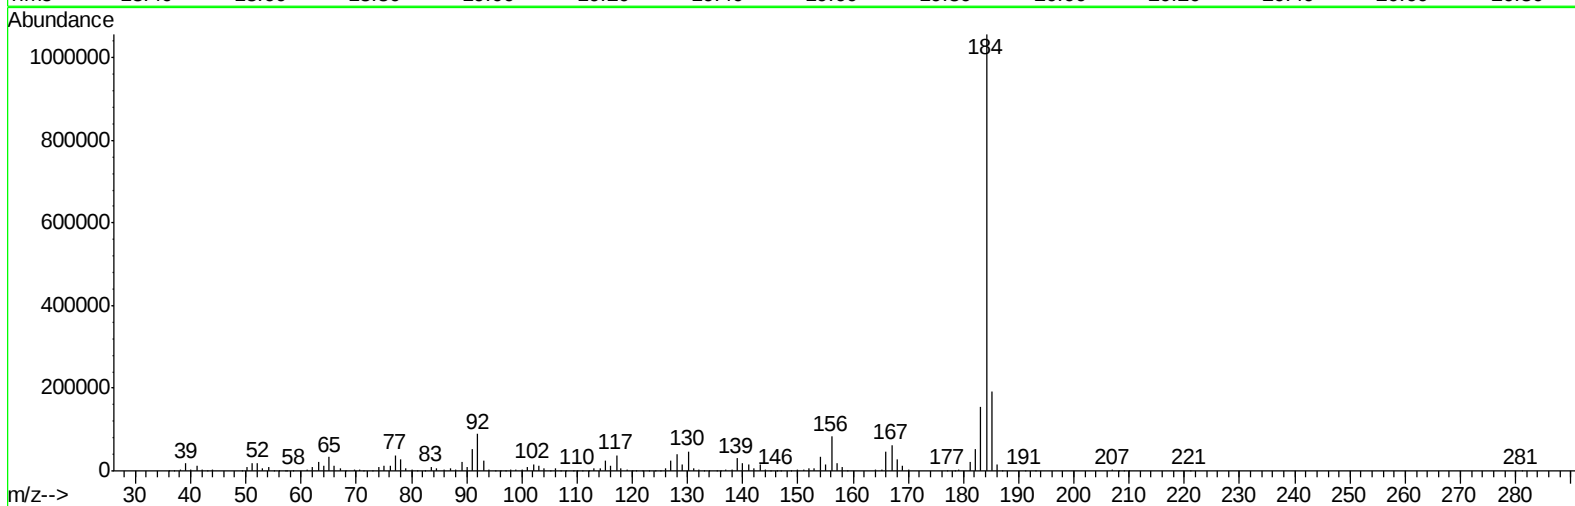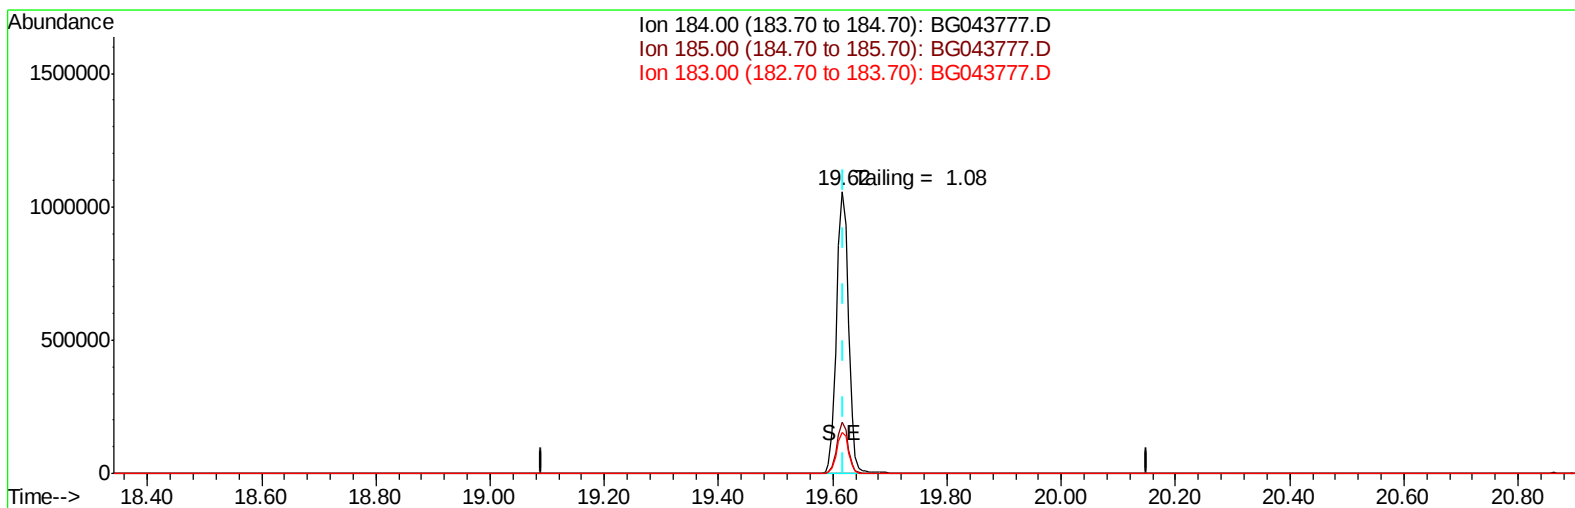

TIC: BG043777.D

(77) Benzidine

19.616min (-0.005) 176039.61ng

response 1552983

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.00 | 18.13 |
| 183.00 | 14.10 | 14.77 |
| 0.00   | 0.00  | 0.00  |