


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112619\
 Data File : BG043777.D
 Acq On : 26 Nov 2019 14:35
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG112219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 23 00:54:00 2019

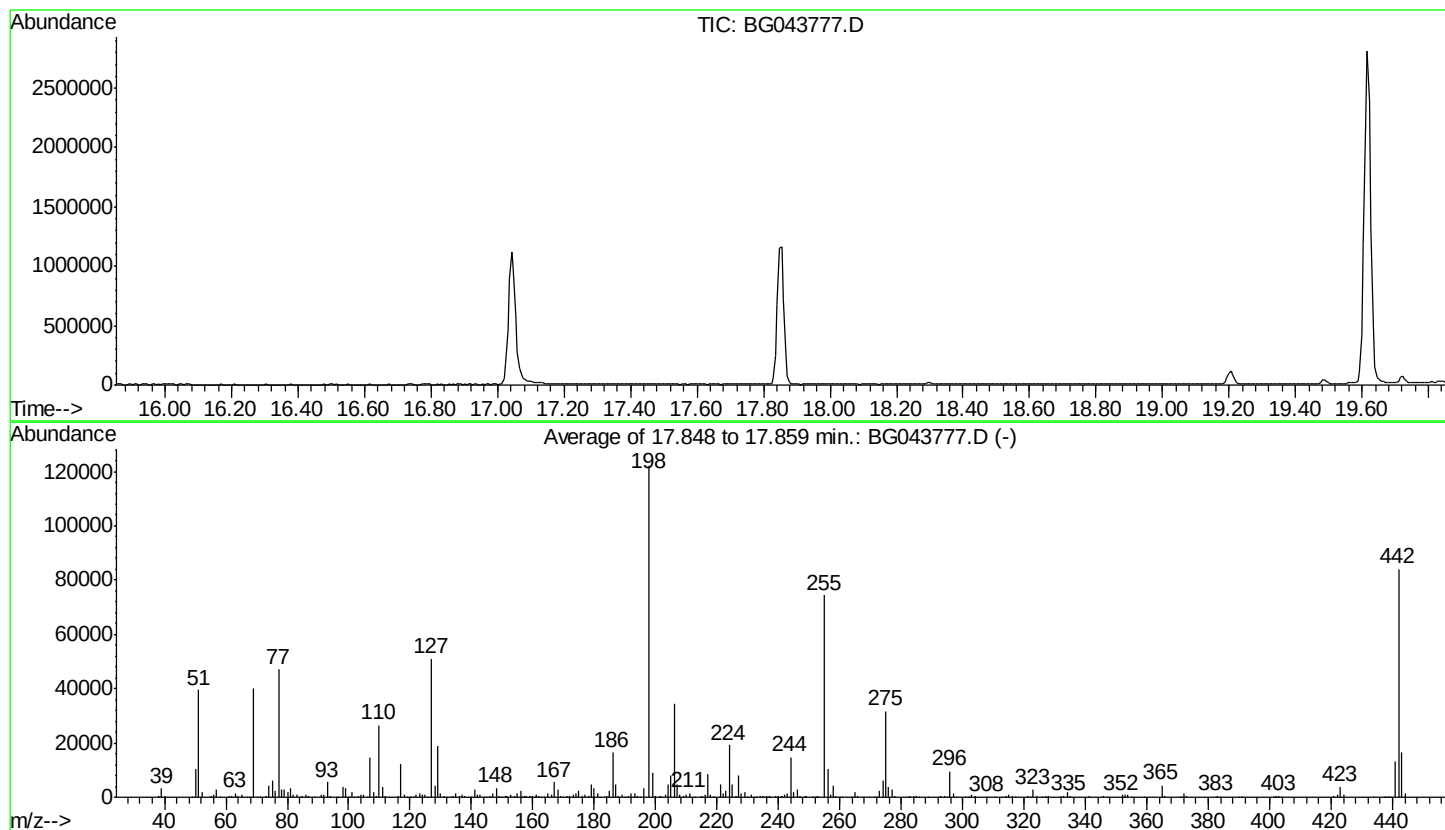

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	39594	PASS
68	69	0.00	2	0.4	173	PASS
69	198	0.00	100	32.8	40077	PASS
70	69	0.00	2	0.6	239	PASS
127	198	10	80	41.8	51117	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	122152	PASS
199	198	5	9	7.5	9109	PASS
275	198	10	60	25.9	31653	PASS
365	198	1	100	3.6	4338	PASS
441	198	0.01	100	10.9	13311	PASS
442	198	50	100	68.9	84125	PASS
443	442	15	24	19.4	16347	PASS