

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112718\
 Data File : BG038179.D
 Acq On : 27 Nov 2018 22:55
 Operator : JU/SJ
 Sample : J5774-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SU-02-112118

Quant Time: Nov 28 04:13:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	37653	20.00	ng	0.00
21) Naphthalene-d8	10.91	136	165163	20.00	ng	0.00
39) Acenaphthene-d10	14.72	164	101016	20.00	ng	0.00
64) Phenanthrene-d10	17.47	188	229134	20.00	ng	0.00
76) Chrysene-d12	21.76	240	213322	20.00	ng	0.00
87) Perylene-d12	25.09	264	183863	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	253770	116.37	ng	0.00
7) Phenol-d6	7.24	99	322877	103.72	ng	0.00
23) Nitrobenzene-d5	9.26	82	255686	82.87	ng	0.00
42) 2,4,6-Tribromophenol	16.21	330	98316	85.34	ng	0.00
45) 2-Fluorobiphenyl	13.34	172	523403	75.49	ng	0.00
79) Terphenyl-d14	20.07	244	846008	93.32	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.26	70	32901	14.607	ng	# 76
51) 2,6-Dinitrotoluene	14.72	165	12695	7.004	ng	# 23
57) 2,4-Dinitrotoluene	14.72	165	12695	5.148	ng	# 23
67) 4-Bromophenyl-phenylether	16.21	248	6939	2.759	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112718\
Data File : BG038179.D
Acq On : 27 Nov 2018 22:55
Operator : JU/SJ
Sample : J5774-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SU-02-112118

Quant Time: Nov 28 04:13:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

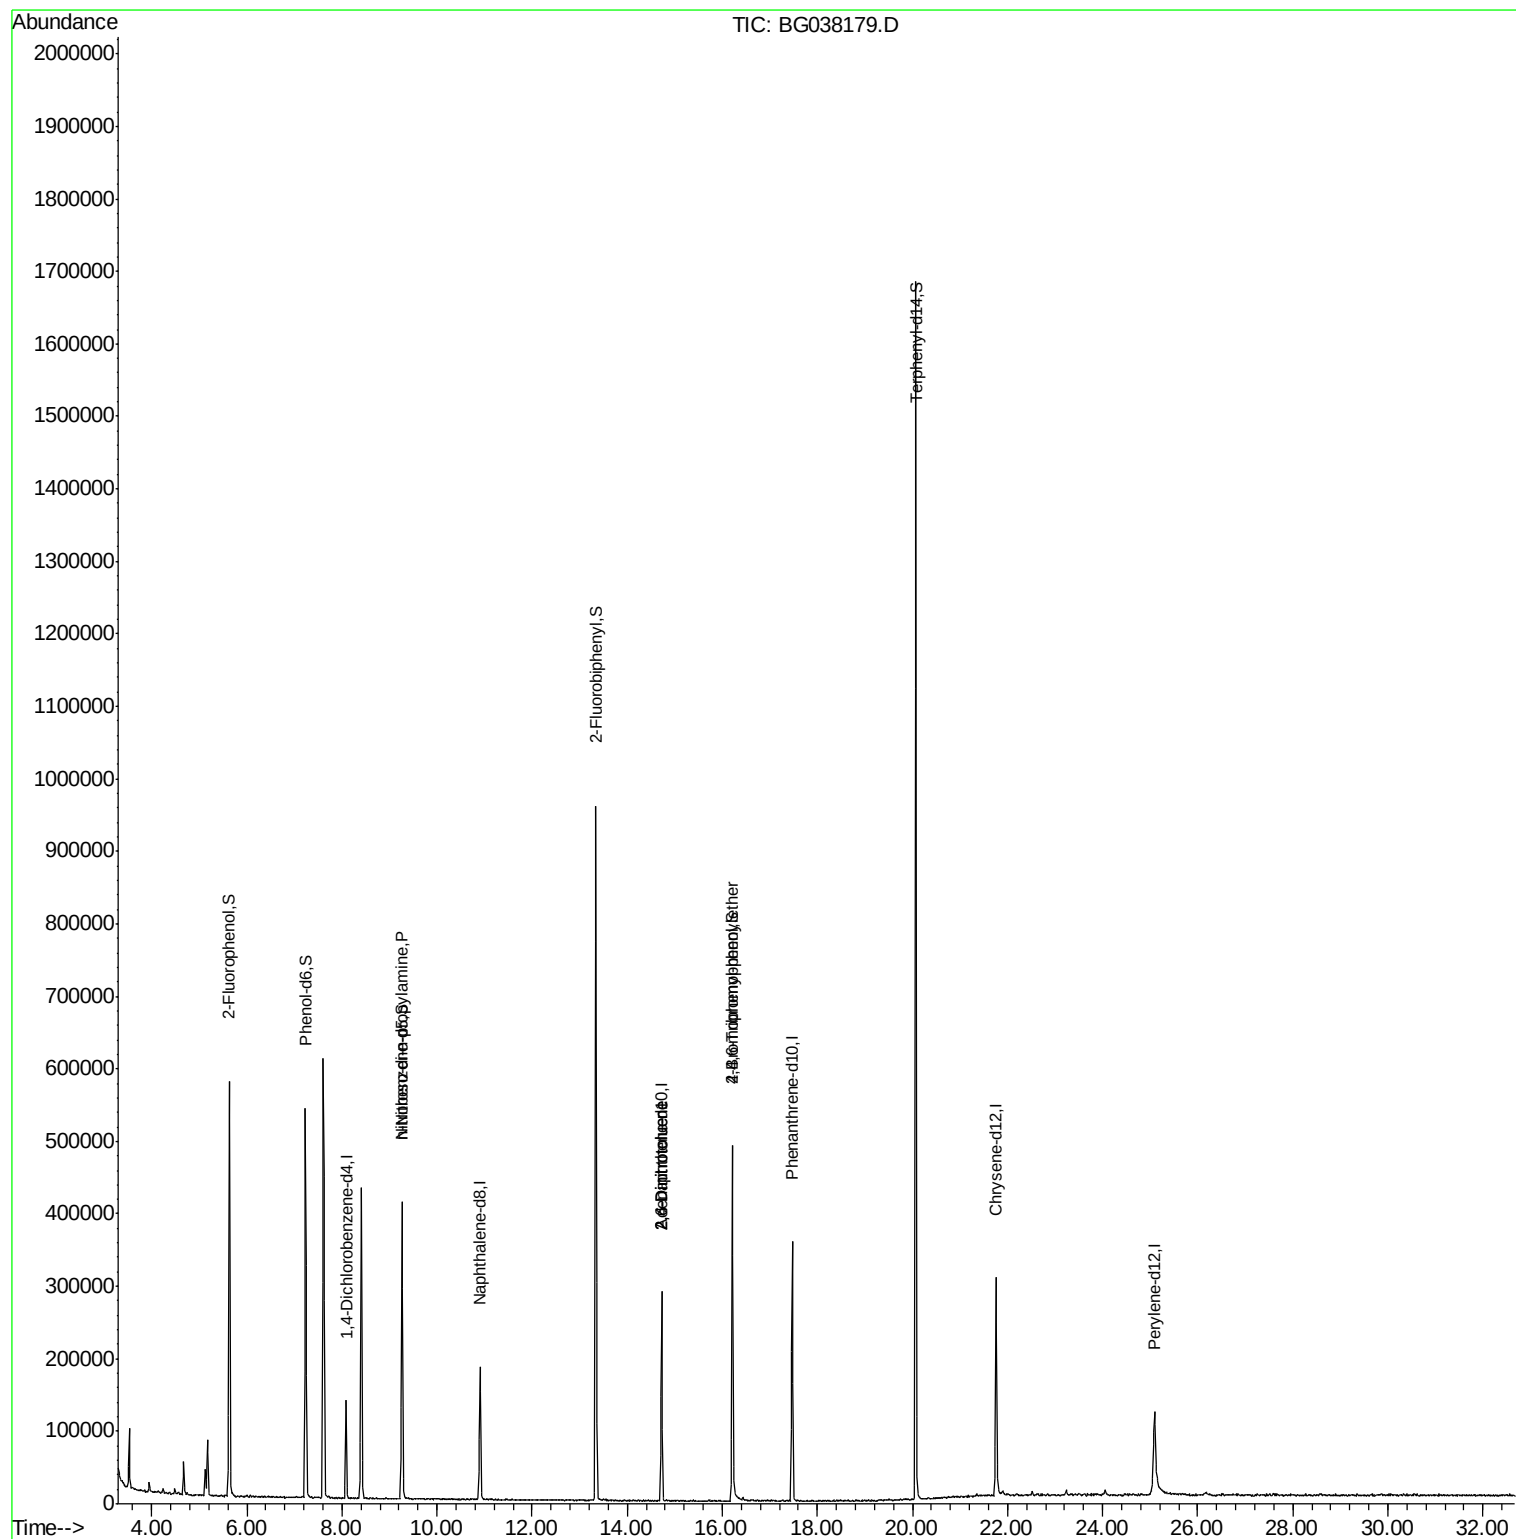

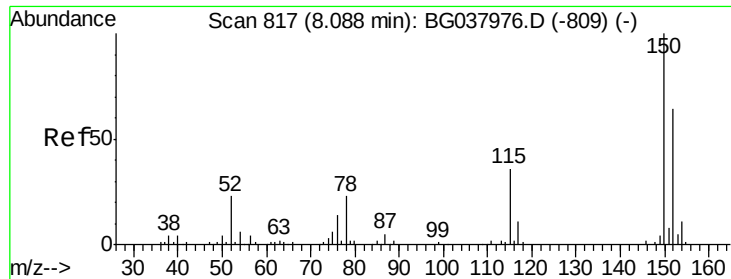


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.09 min Scan# 817
Delta R.T. -0.00 min
Lab File: BG038179.D
Acq: 27 Nov 2018 22:55

Instrument :
BNA_G
ClientSampleId :
SU-02-112118

Tgt Ion:152 Resp: 37653
Ion Ratio Lower Upper
152 100
150 157.1 126.0 189.0
115 55.1 45.5 68.3

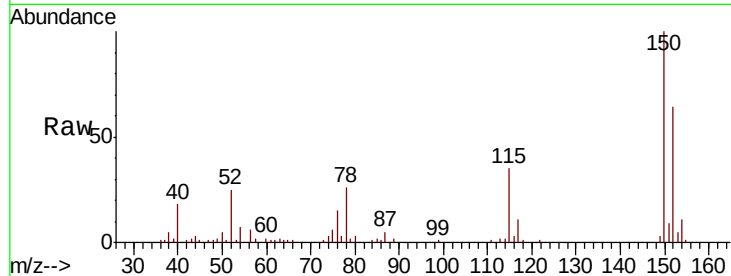


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

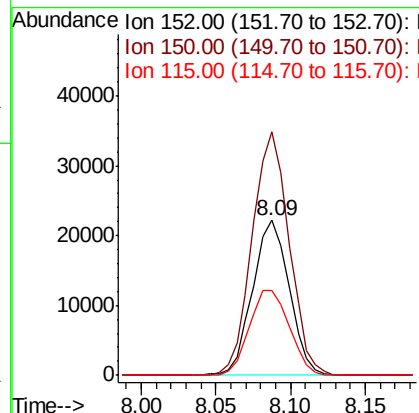



#5


2-Fluorophenol
Concen: 116.365 ng
RT: 5.63 min Scan# 399
Delta R.T. -0.00 min
Lab File: BG038179.D
Acq: 27 Nov 2018 22:55

Tgt Ion:112 Resp: 253770
Ion Ratio Lower Upper
112 100
64 70.8 53.1 79.7
63 36.6 27.3 40.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

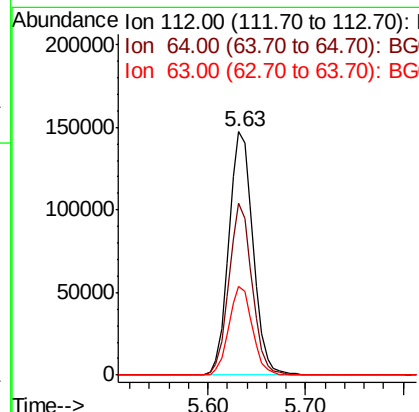

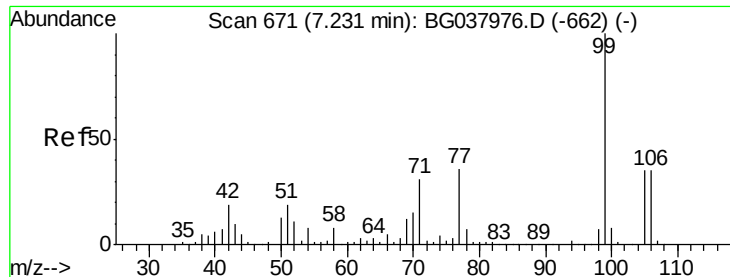

#7

Phenol-d6

Concen: 103.720 ng

RT: 7.24 min Scan# 672

Delta R.T. 0.00 min

Lab File: BG038179.D

Acq: 27 Nov 2018 22:55

Instrument :

BNA_G

ClientSampleId :

SU-02-112118


Tgt Ion: 99 Resp: 322877

Ion Ratio Lower Upper




99 100

42 20.2 15.0 22.4

71 33.4 25.5 38.3

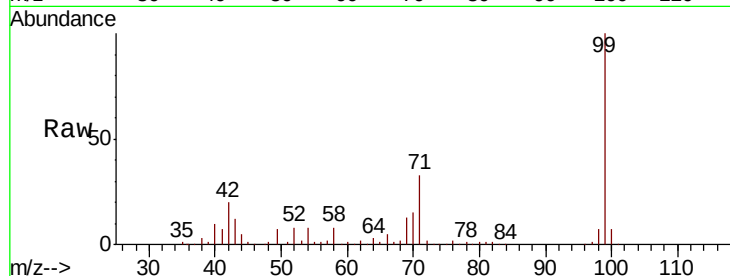

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

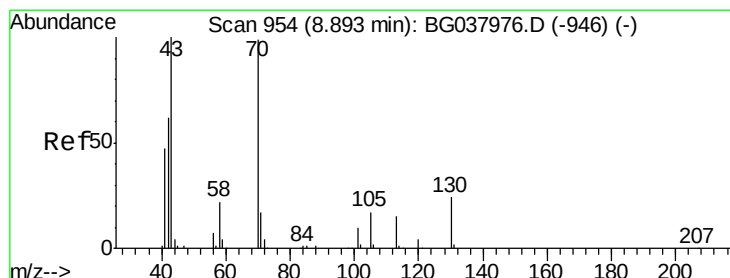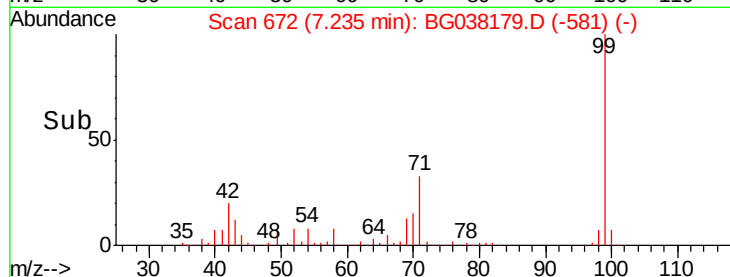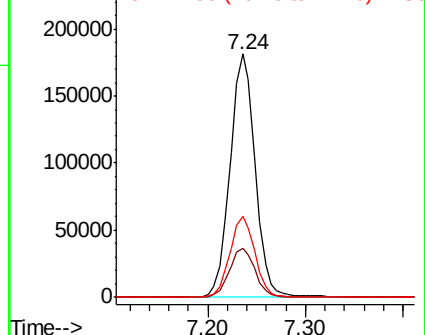

#19

n-Nitroso-di-n-propylamine

Concen: 14.607 ng

RT: 9.26 min Scan# 1017

Delta R.T. 0.37 min

Lab File: BG038179.D

Acq: 27 Nov 2018 22:55

Tgt Ion: 70 Resp: 32901


Ion Ratio Lower Upper

70 100



42 53.8 53.9 80.9#


101 0.0 8.2 12.2#

130 2.5 18.2 27.4#

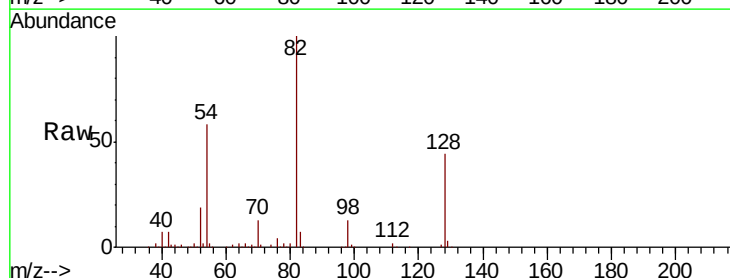

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

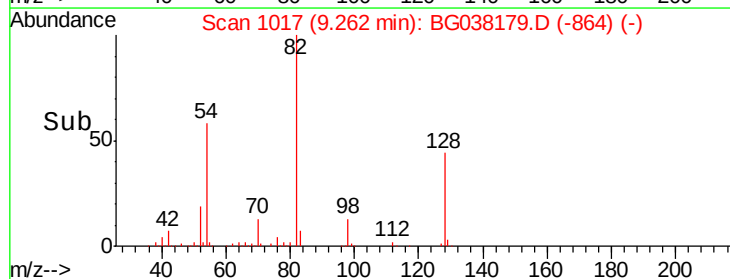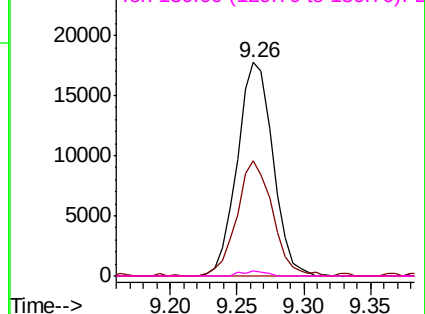







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.91 min Scan# 1297
Delta R.T. -0.00 min
Lab File: BG038179.D
Acq: 27 Nov 2018 22:55

Instrument :
BNA_G
ClientSampleId :
SU-02-112118

Tgt Ion:	136	Resp:	165163
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.6	14.4
54	9.8	7.9	11.9
68	5.9	4.8	7.2




Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


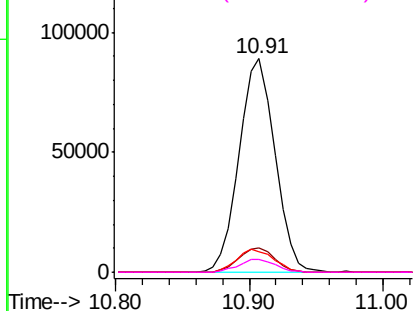



#23
Nitrobenzene-d5
Concen: 82.869 ng
RT: 9.26 min Scan# 1017
Delta R.T. -0.00 min
Lab File: BG038179.D
Acq: 27 Nov 2018 22:55

Tgt Ion:	82	Resp:	255686
Ion	Ratio	Lower	Upper
82	100		
128	43.9	34.6	51.8
54	58.1	45.3	67.9



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

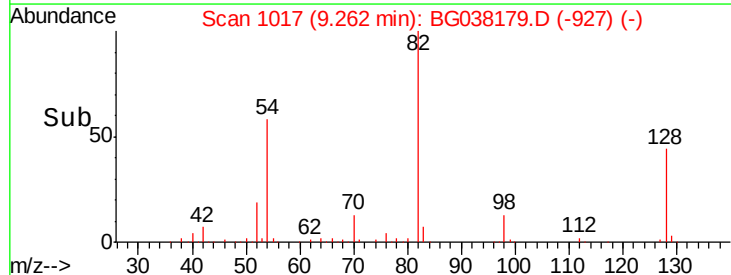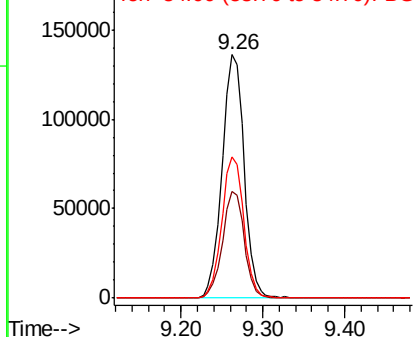

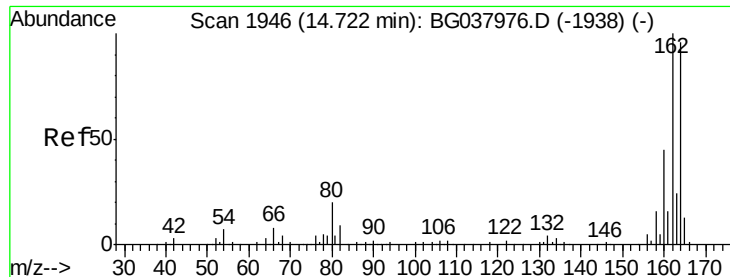

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.72 min Scan# 1946

Delta R.T. -0.00 min

Lab File: BG038179.D

Acq: 27 Nov 2018 22:55

Instrument :

BNA_G

ClientSampleId :

SU-02-112118


Tgt Ion:164 Resp: 101016

Ion Ratio Lower Upper

164 100

162 104.8 81.3 121.9




160 44.8 36.3 54.5

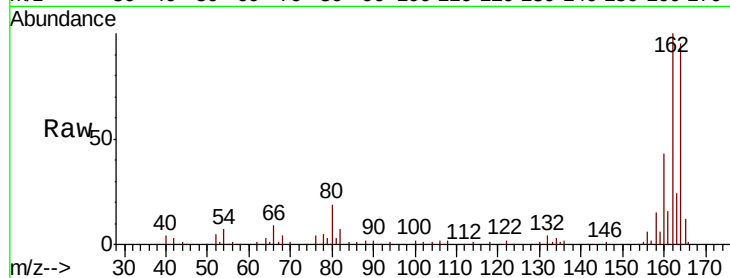

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

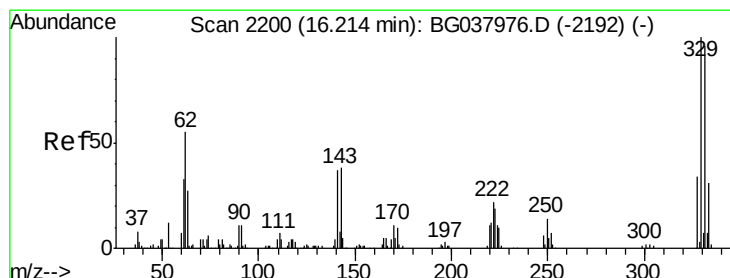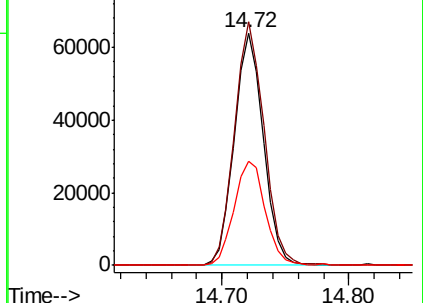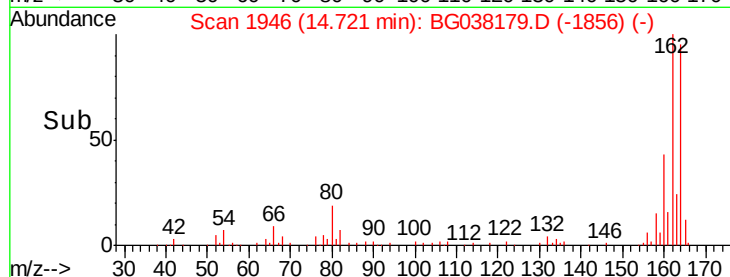

#42

2,4,6-Tribromophenol

Concen: 85.339 ng

RT: 16.21 min Scan# 2200

Delta R.T. -0.00 min

Lab File: BG038179.D

Acq: 27 Nov 2018 22:55


Tgt Ion:330 Resp: 98316

Ion Ratio Lower Upper

330 100

332 98.2 78.4 117.6



141 41.9 32.2 48.2

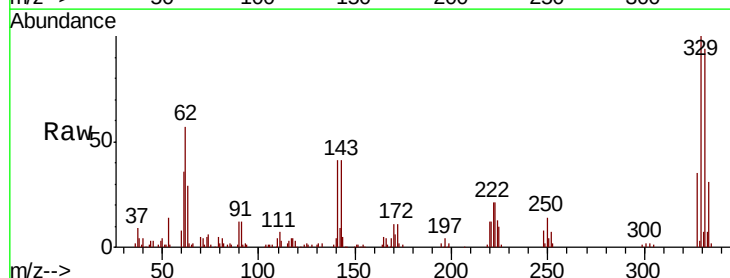


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

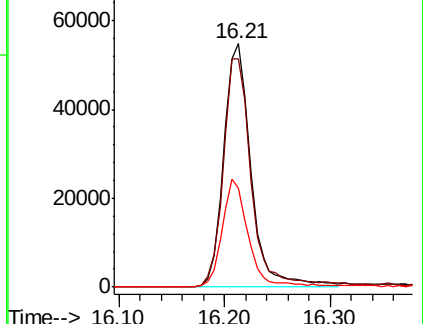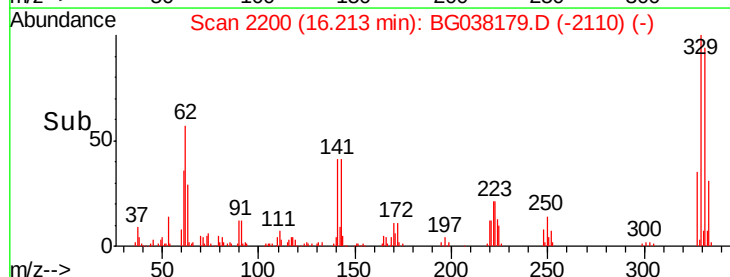







#45
 2-Fluorobiphenyl
 Concen: 75.485 ng
 RT: 13.34 min Scan# 1711
 Delta R.T. -0.01 min
 Lab File: BG038179.D
 Acq: 27 Nov 2018 22:55

Instrument :
 BNA_G
 ClientSampleId :
 SU-02-112118

Tgt Ion:172 Resp: 523403
 Ion Ratio Lower Upper
 172 100
 171 37.7 31.0 46.4
 170 25.1 20.2 30.2




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


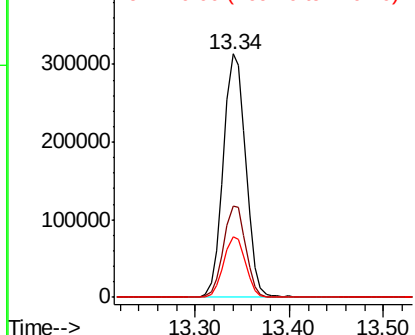



#51
 2,6-Dinitrotoluene
 Concen: 7.004 ng
 RT: 14.72 min Scan# 1946
 Delta R.T. 0.42 min
 Lab File: BG038179.D
 Acq: 27 Nov 2018 22:55

Tgt Ion:165 Resp: 12695
 Ion Ratio Lower Upper
 165 100
 63 0.0 43.4 65.2#
 89 0.0 45.8 68.6#



Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC

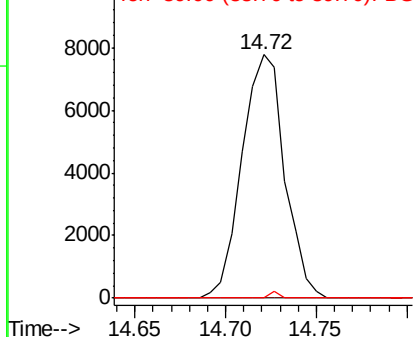


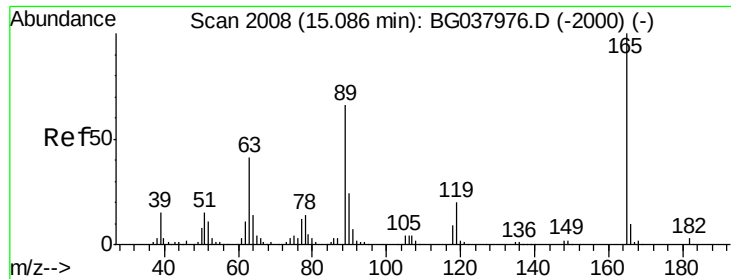




#57
 2,4-Dinitrotoluene
 Concen: 5.148 ng
 RT: 14.72 min Scan# 1946
 Delta R.T. -0.37 min
 Lab File: BG038179.D
 Acq: 27 Nov 2018 22:55

Instrument :
 BNA_G
 ClientSampleId :
 SU-02-112118

Tgt Ion:	165	Resp:	12695
Ion	Ratio	Lower	Upper
165	100		
63	0.0	33.4	50.0#
89	0.0	57.2	85.8#
182	0.0	2.6	4.0#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

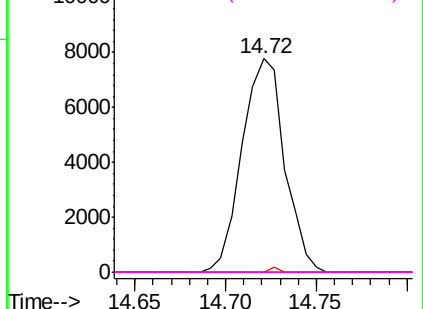




#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.47 min Scan# 2414
 Delta R.T. -0.00 min
 Lab File: BG038179.D
 Acq: 27 Nov 2018 22:55

Tgt Ion:	188	Resp:	229134
Ion	Ratio	Lower	Upper
188	100		
94	9.1	7.2	10.8
80	10.6	7.7	11.5



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

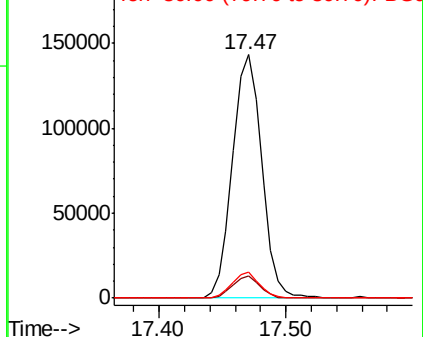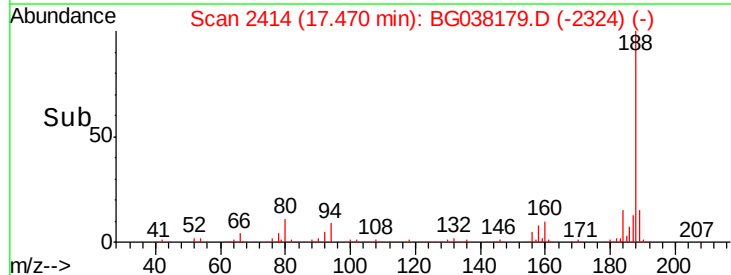


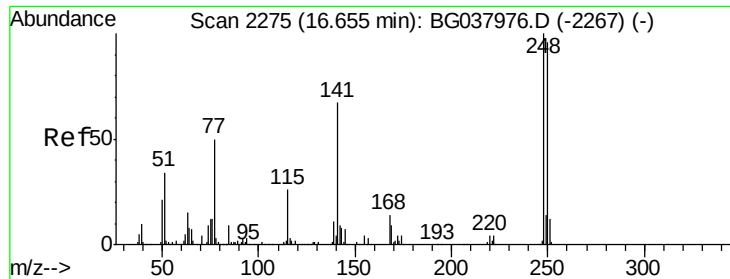




#67
 4-Bromophenyl-phenylether
 Concen: 2.759 ng
 RT: 16.21 min Scan# 2200
 Delta R.T. -0.44 min
 Lab File: BG038179.D
 Acq: 27 Nov 2018 22:55

Instrument :
 BNA_G
 ClientSampleId :
 SU-02-112118

Tgt Ion:248 Resp: 6939
 Ion Ratio Lower Upper
 248 100
 250 178.5 77.0 115.6#
 141 410.6 55.5 83.3#

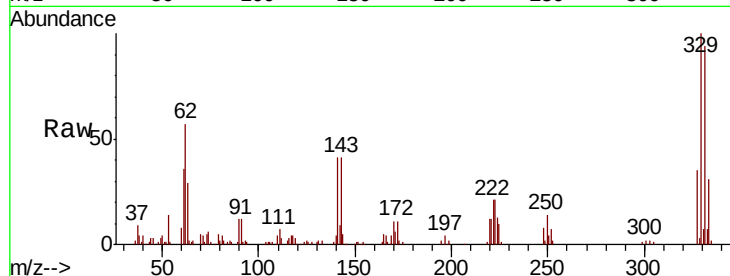


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

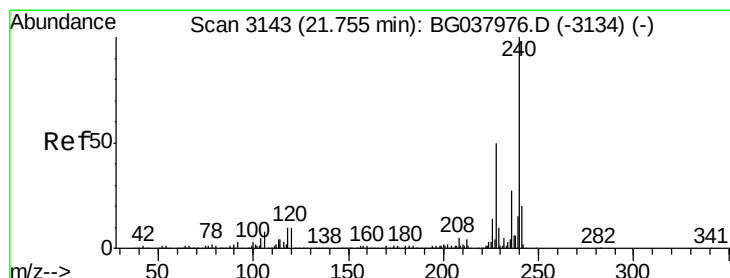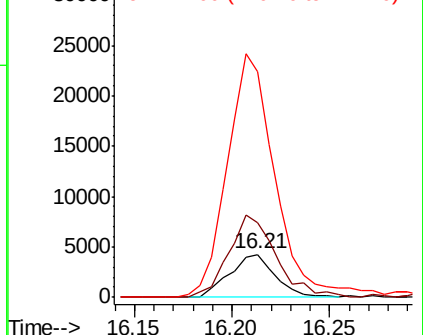
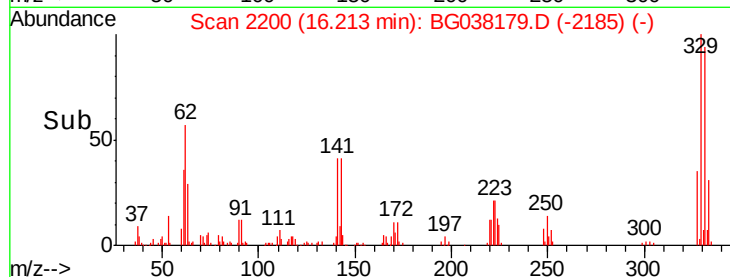



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.76 min Scan# 3144
 Delta R.T. 0.00 min
 Lab File: BG038179.D
 Acq: 27 Nov 2018 22:55

Tgt Ion:240 Resp: 213322
 Ion Ratio Lower Upper
 240 100
 120 9.6 8.1 12.1
 236 26.9 21.4 32.0

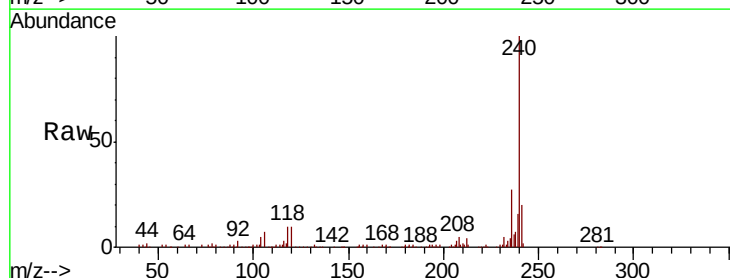

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

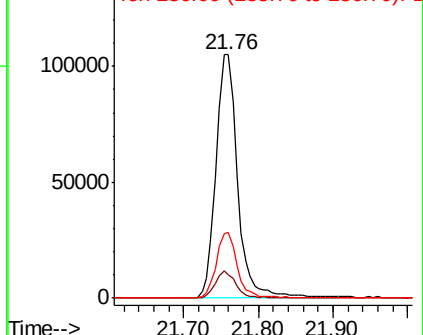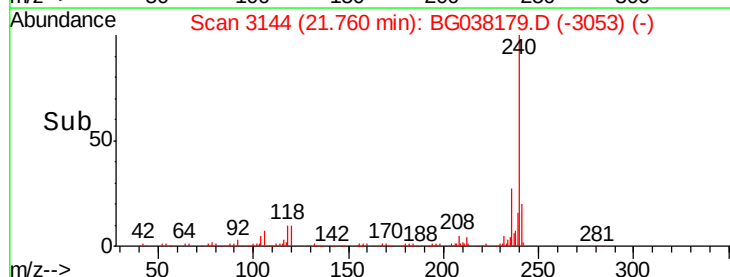



#79

Terphenyl-d14

Concen: 93.317 ng

RT: 20.07 min Scan# 2857

Delta R.T. 0.01 min

Lab File: BG038179.D

Acq: 27 Nov 2018 22:55

Instrument :

BNA_G

ClientSampleId :

SU-02-112118


Tgt Ion:244 Resp: 846008

Ion Ratio Lower Upper

244 100

212 8.0 6.5 9.7




122 9.8 9.0 13.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

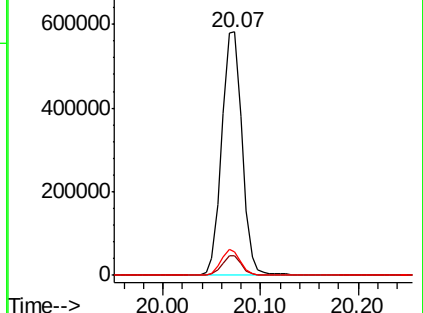

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.09 min Scan# 3710

Delta R.T. 0.00 min

Lab File: BG038179.D

Acq: 27 Nov 2018 22:55


Tgt Ion:264 Resp: 183863

Ion Ratio Lower Upper

264 100

260 21.4 18.2 27.4

265 19.3 17.9 26.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

