
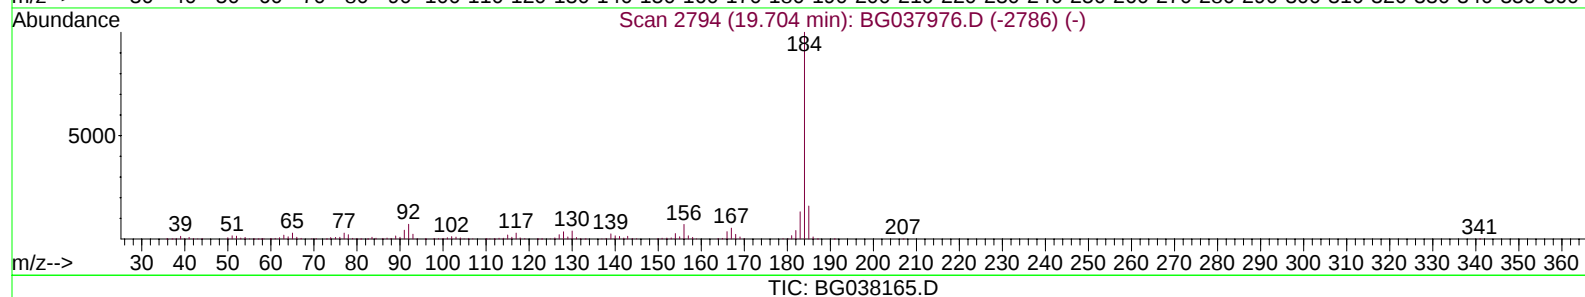
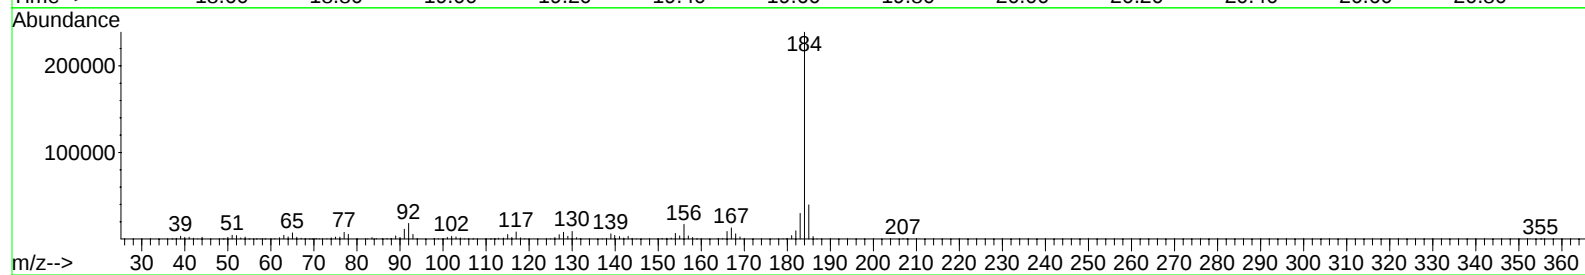


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112718\
Data File : BG038165.D
Acq On : 27 Nov 2018 13:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 17:20:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

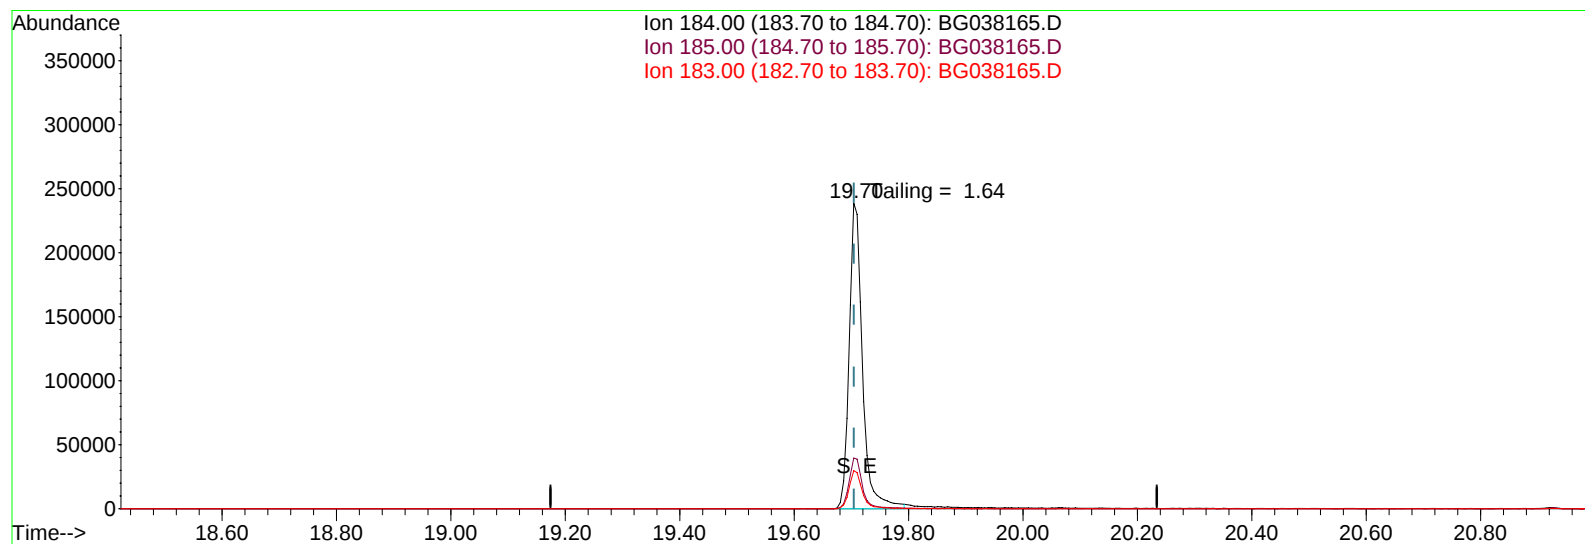

(77) Benzidine




19.704min (-0.000) 35204.77ng

response 397769

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.58
183.00	12.70	12.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112718\
Data File : BG038165.D
Acq On : 27 Nov 2018 13:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 17:20:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

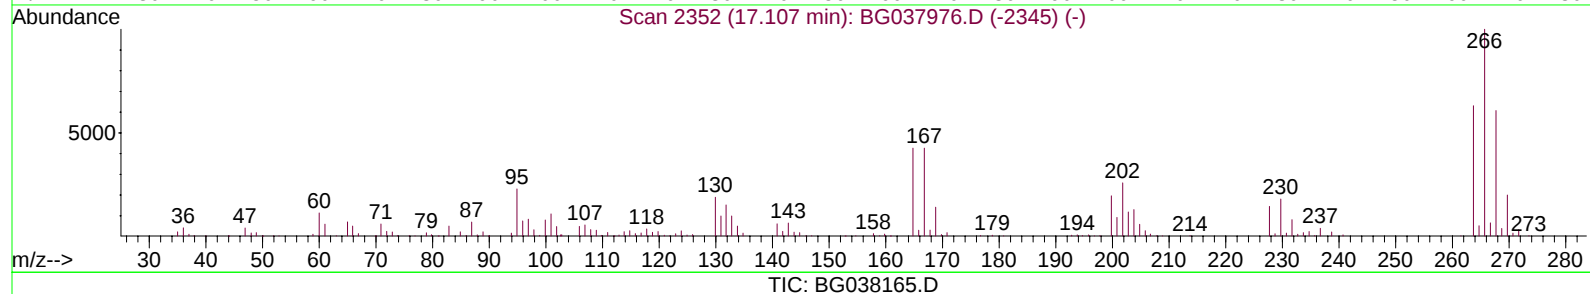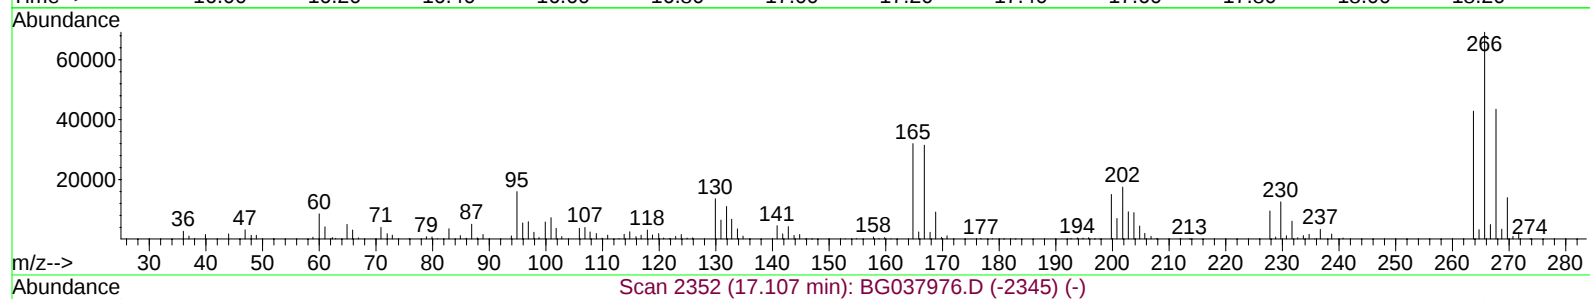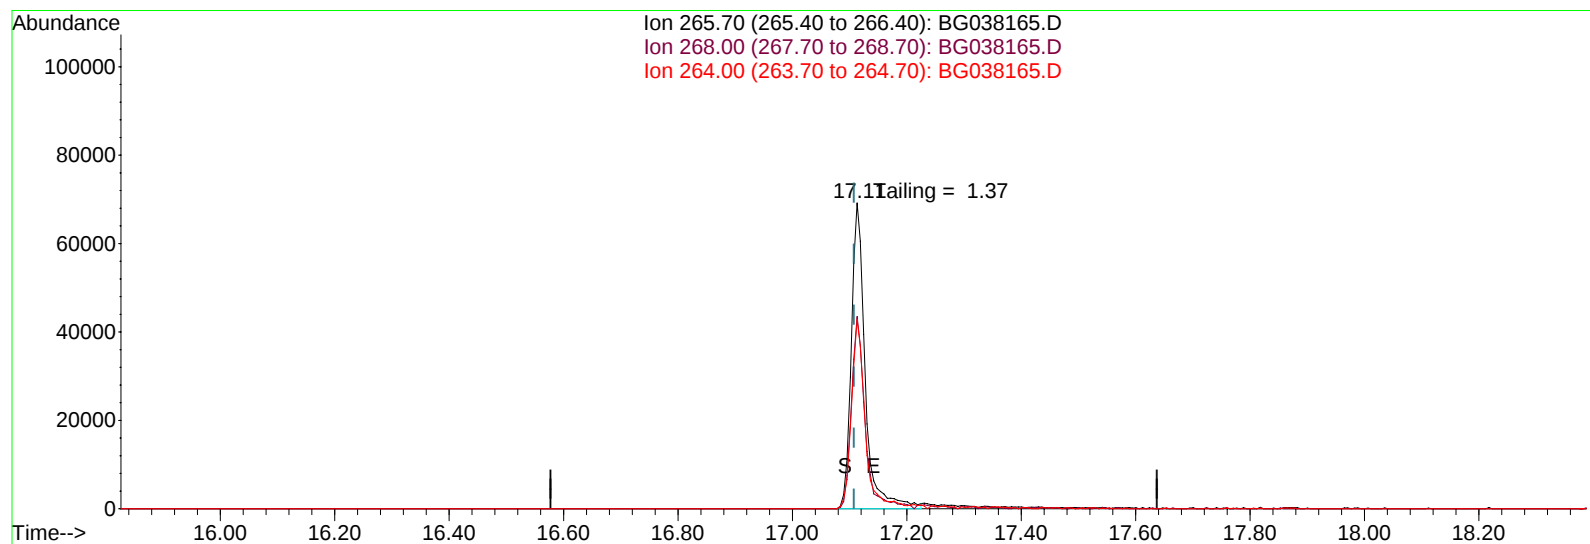

(70) Pentachlorophenol (C)

17.113min (+0.006) 64351.22ng

response 117845

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.78
264.00	73.60	66.58
0.00	0.00	0.00