
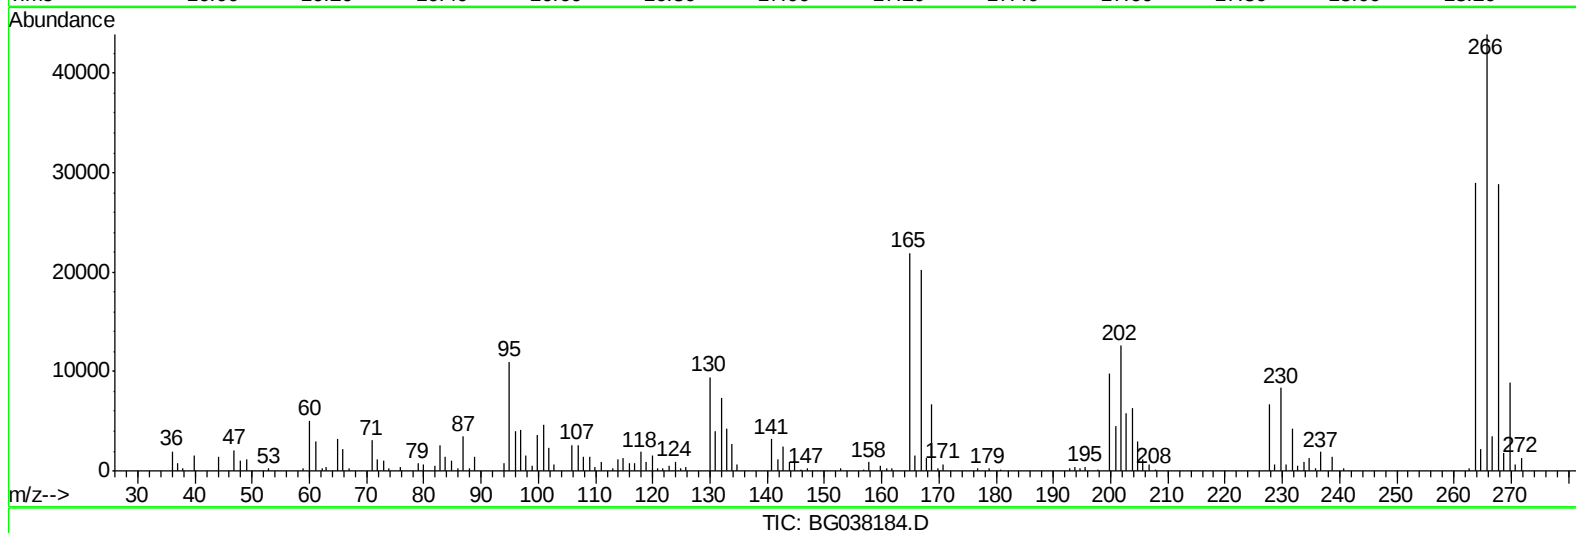


Data File : BG038184.D
Acq On : 28 Nov 2018 3:31
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 08:05:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

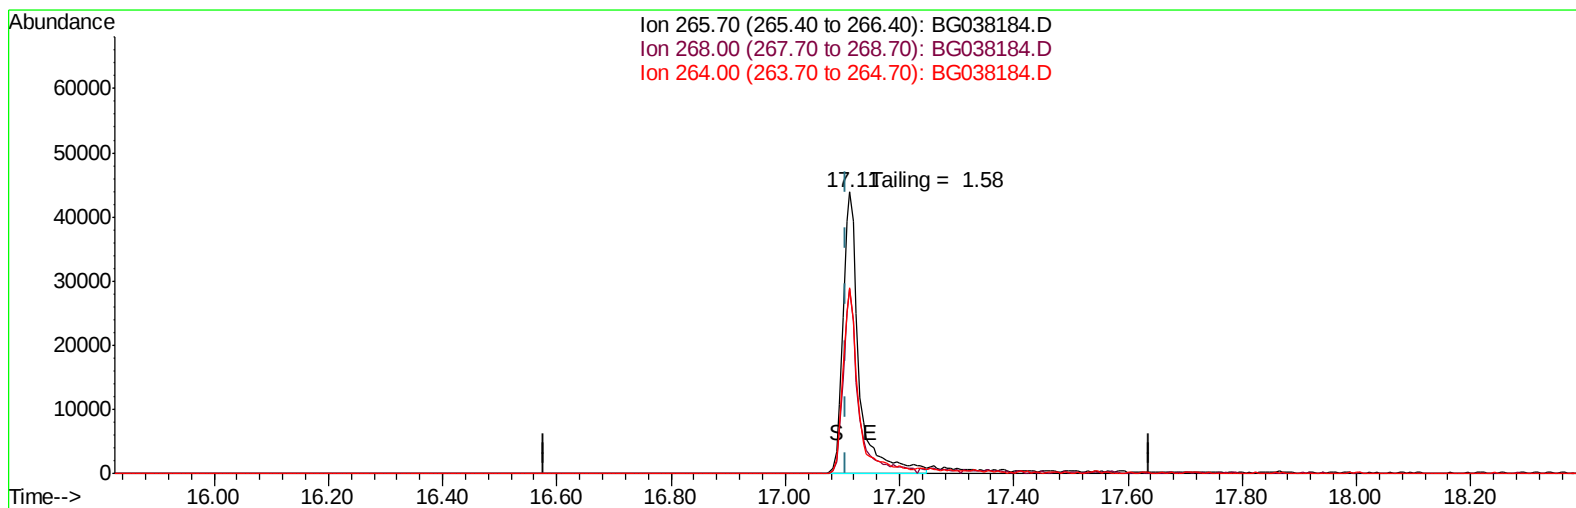

(70) Pentachlorophenol (C)



17.113min (+0.006) 157256.25ng

response 87120

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	69.75
264.00	73.60	71.11
0.00	0.00	0.00

Data File : BG038184.D
Acq On : 28 Nov 2018 3:31
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 08:05:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

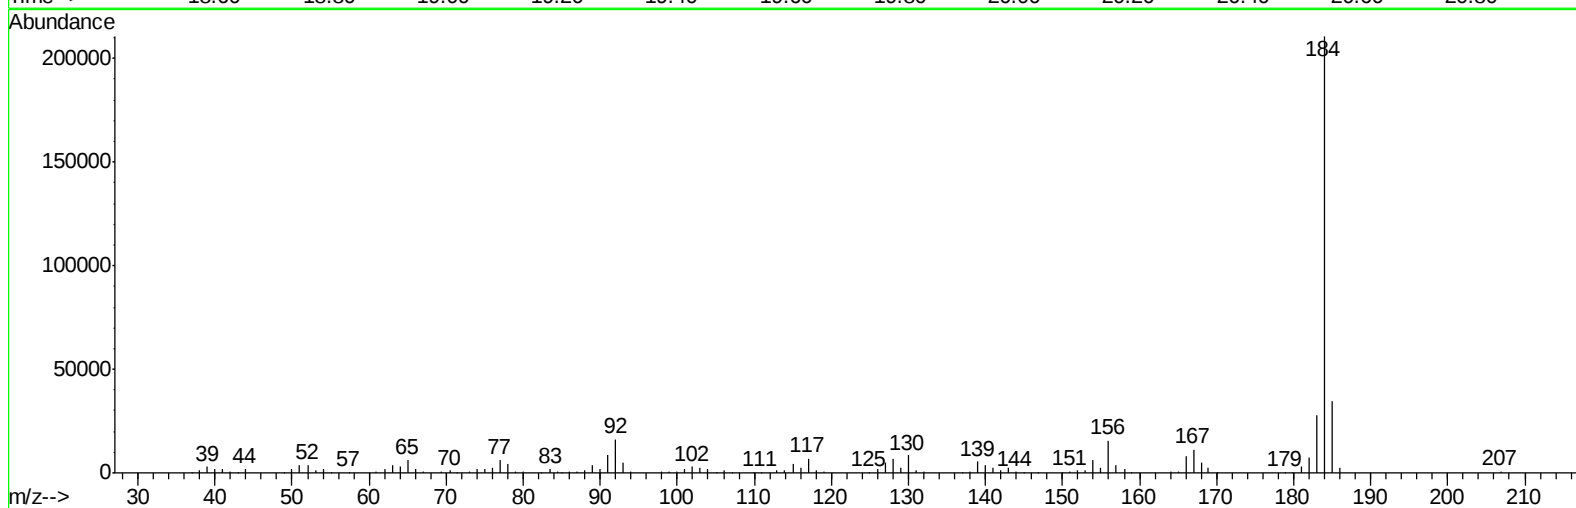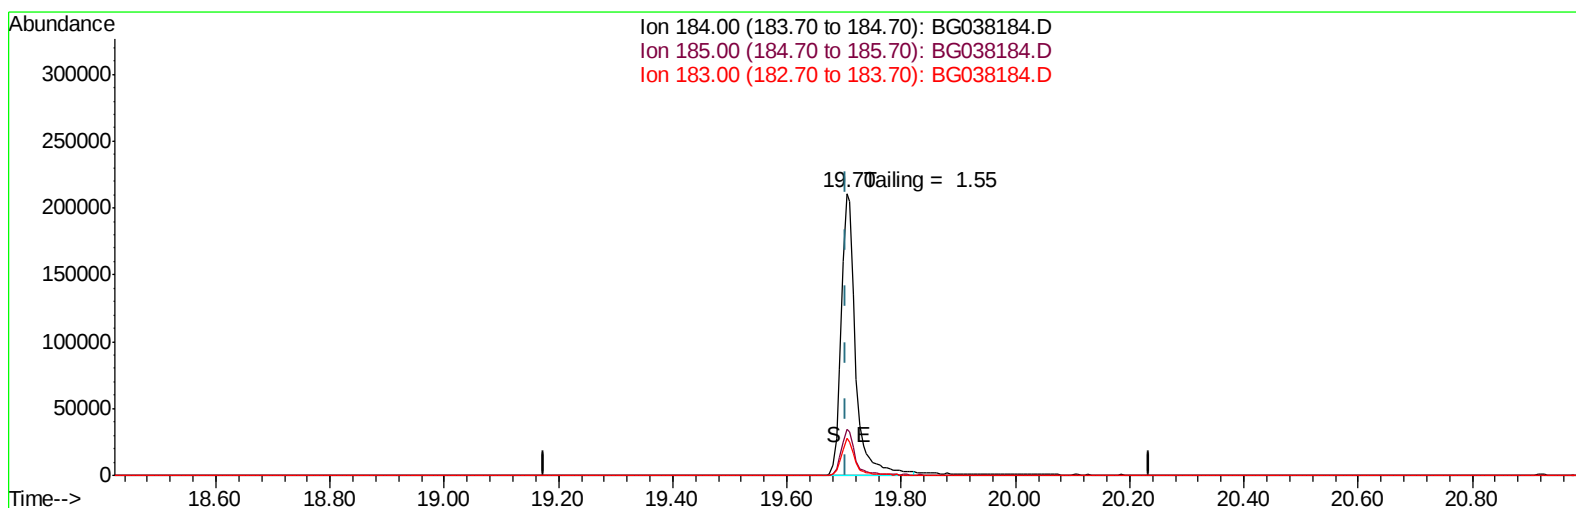

TIC: BG038184.D

(77) Benzidine

19.704min (-0.000) 0.00ng

response 375847

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.32
183.00	12.70	13.29
0.00	0.00	0.00