

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112718\
 Data File : BG038181.D
 Acq On : 28 Nov 2018 00:14
 Operator : JU/SJ
 Sample : J5774-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SU-03-112118-B

Quant Time: Nov 28 05:49:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	37482	20.00	ng	0.00
21) Naphthalene-d8	10.90	136	160199	20.00	ng	0.00
39) Acenaphthene-d10	14.72	164	97537	20.00	ng	0.00
64) Phenanthrene-d10	17.47	188	219173	20.00	ng	0.00
76) Chrysene-d12	21.76	240	203980	20.00	ng	0.00
87) Perylene-d12	25.09	264	163307	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	263691	121.47	ng	0.00
7) Phenol-d6	7.24	99	340564	109.90	ng	0.00
23) Nitrobenzene-d5	9.26	82	258589	86.41	ng	0.00
42) 2,4,6-Tribromophenol	16.21	330	102193	91.87	ng	0.00
45) 2-Fluorobiphenyl	13.34	172	526007	78.57	ng	0.00
79) Terphenyl-d14	20.07	244	833604	96.16	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112718\
Data File : BG038181.D
Acq On : 28 Nov 2018 00:14
Operator : JU/SJ
Sample : J5774-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SU-03-112118-B

Quant Time: Nov 28 05:49:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

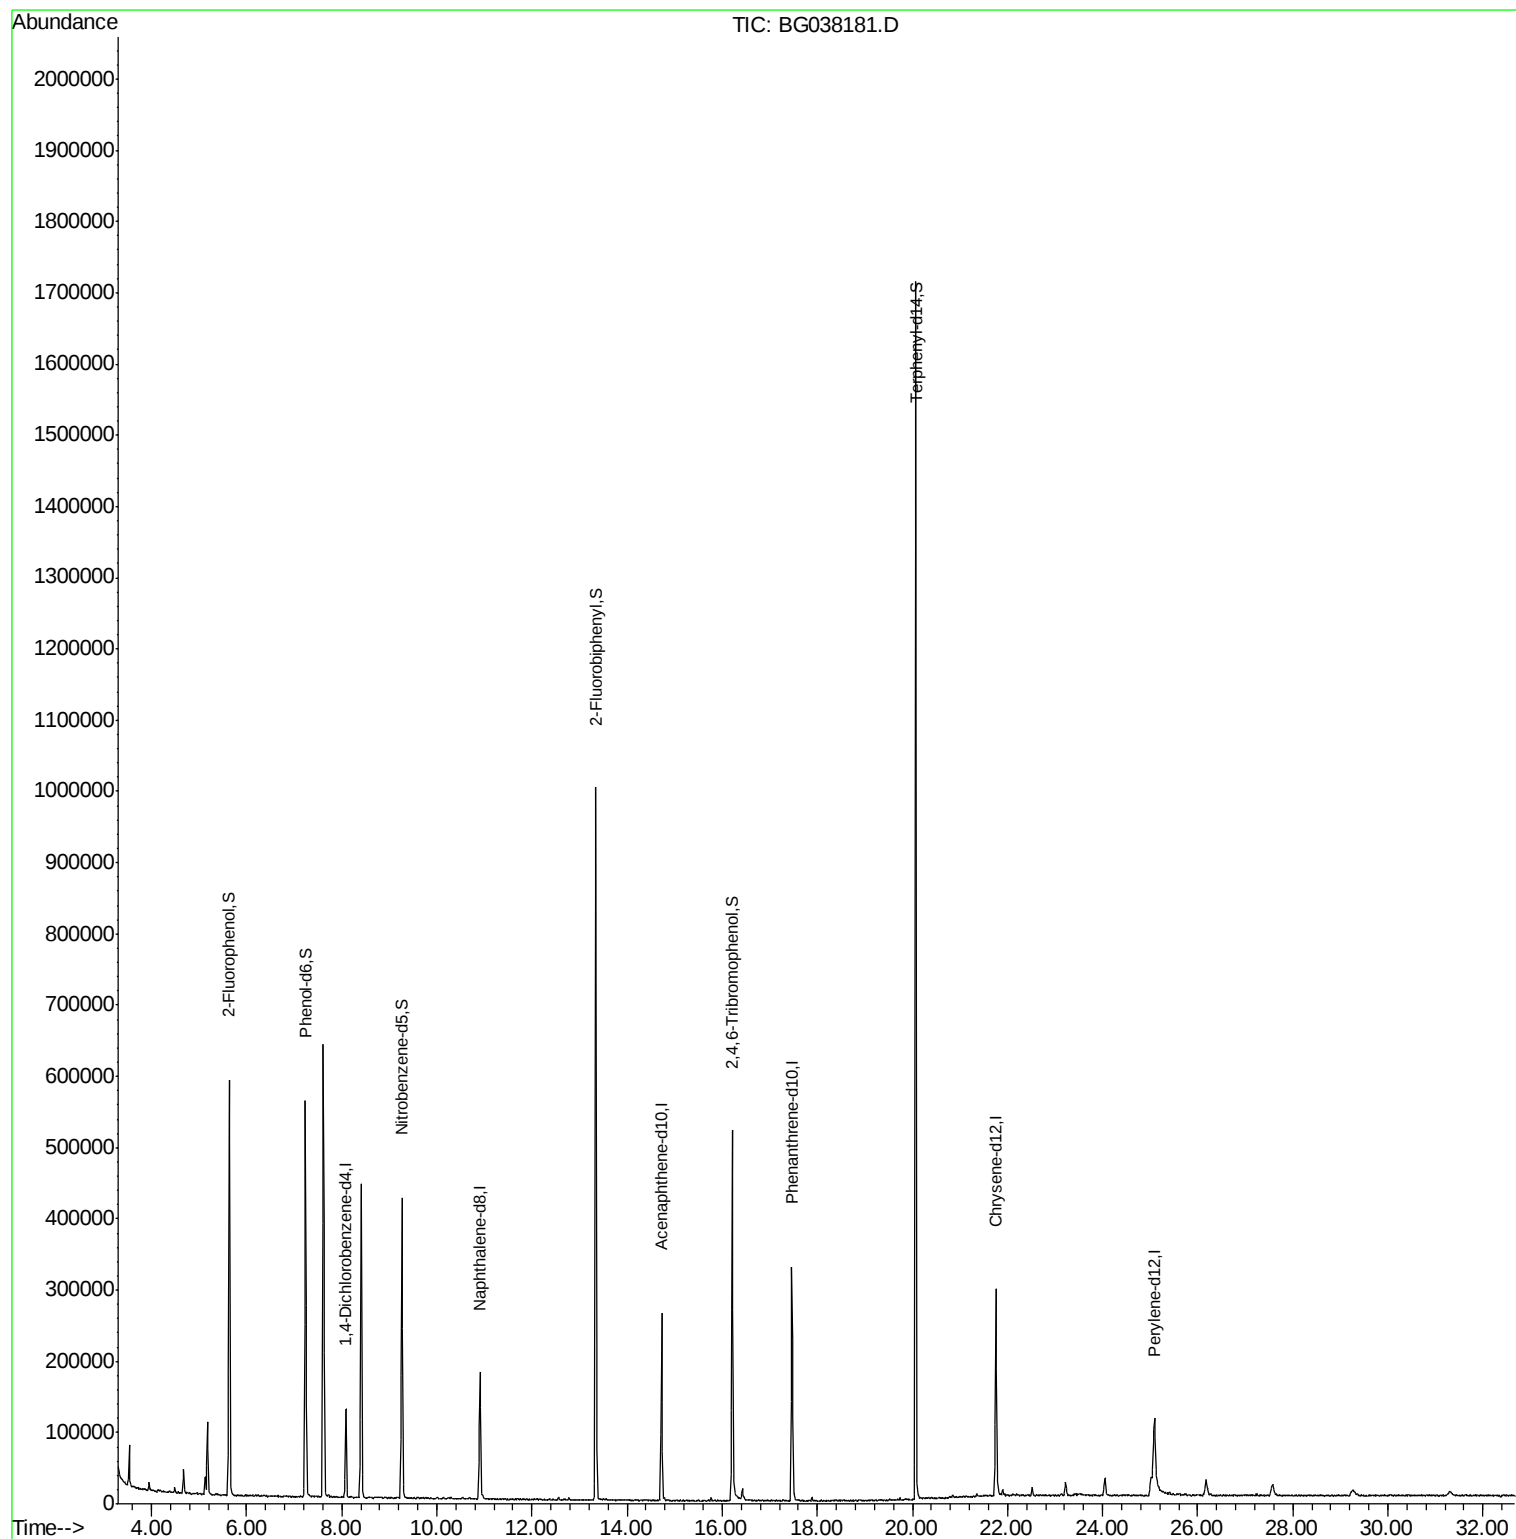

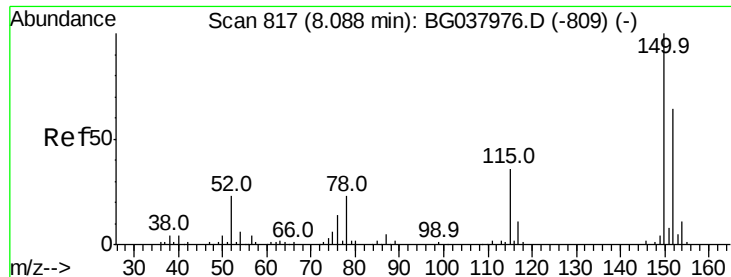


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.08 min Scan# 816
Delta R.T. -0.00 min
Lab File: BG038181.D
Acq: 28 Nov 2018 00:14

Instrument :
BNA_G
ClientSampleId :
SU-03-112118-B

Tot Ion:152 Resp: 37482
Ion Ratio Lower Upper
152 100
150 156.2 126.0 189.0
115 57.0 45.5 68.3

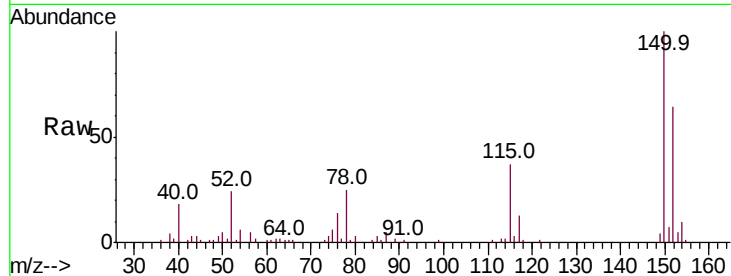


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

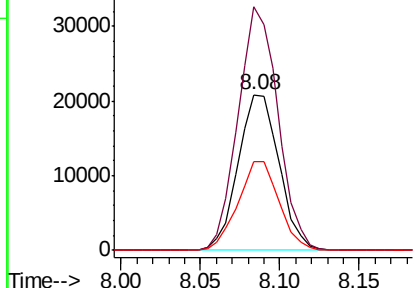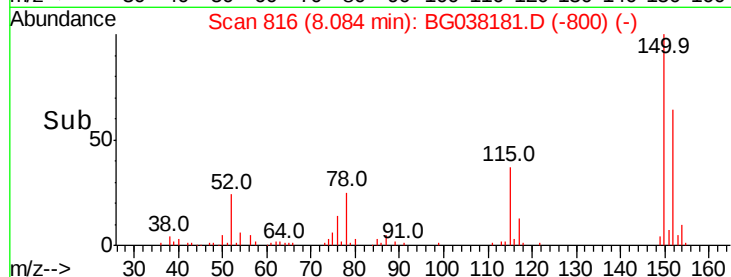



#5


2-Fluorophenol
Concen: 121.466 ng
RT: 5.63 min Scan# 399
Delta R.T. 0.00 min
Lab File: BG038181.D
Acq: 28 Nov 2018 00:14

Tgt Ion:112 Resp: 263691
Ion Ratio Lower Upper
112 100
64 66.4 53.1 79.7
63 36.5 27.3 40.9

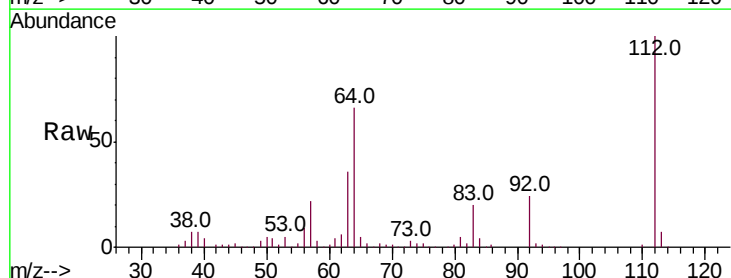

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

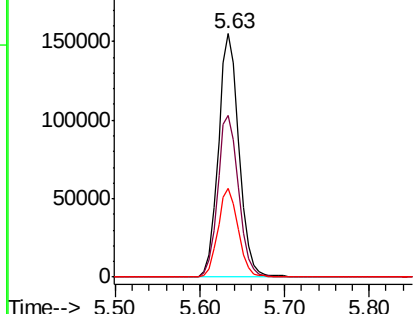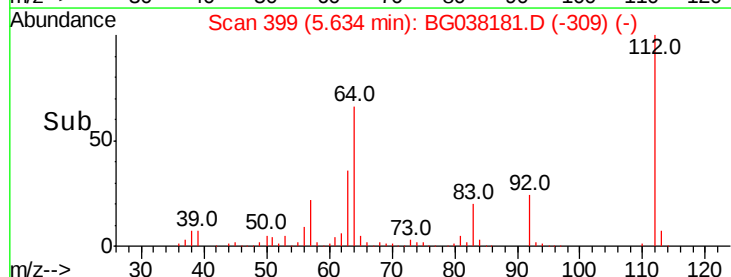

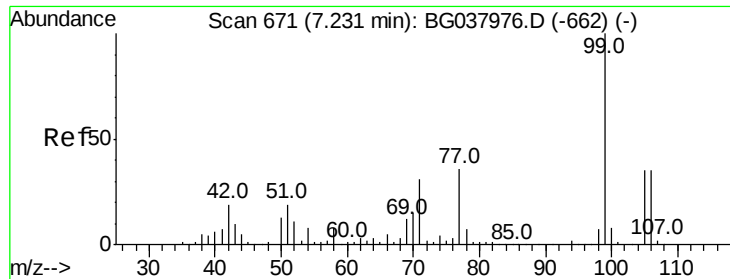

#7

Phenol-d6

Concen: 109.901 ng

RT: 7.24 min Scan# 672

Delta R.T. 0.01 min

Lab File: BG038181.D

Acq: 28 Nov 2018 00:14

Instrument :

BNA_G

ClientSampleId :

SU-03-112118-B


Tot Ion: 99 Resp: 340564

Ion Ratio Lower Upper




99 100

42 20.2 15.0 22.4

71 33.3 25.5 38.3

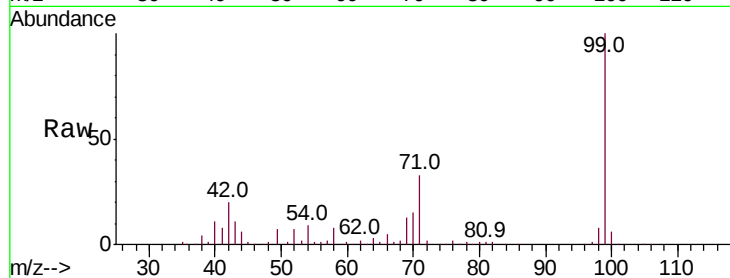

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

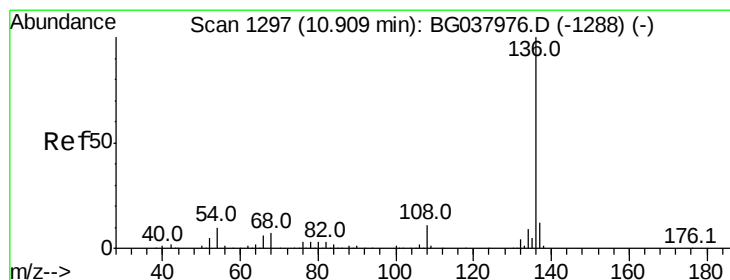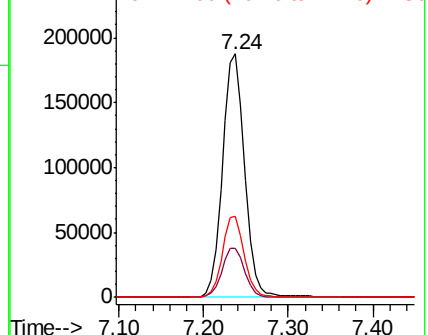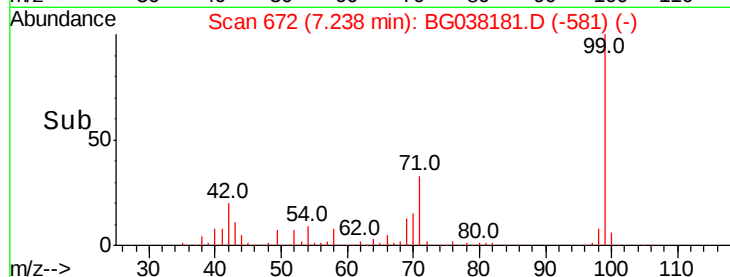

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.90 min Scan# 1296

Delta R.T. -0.00 min

Lab File: BG038181.D

Acq: 28 Nov 2018 00:14

Tgt Ion: 136 Resp: 160199


Ion Ratio Lower Upper

136 100



137 11.4 9.6 14.4


54 11.6 7.9 11.9

68 5.9 4.8 7.2

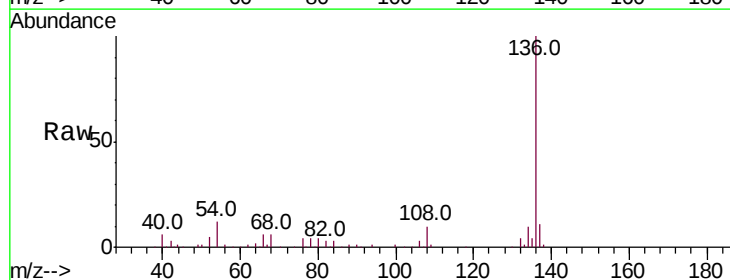

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

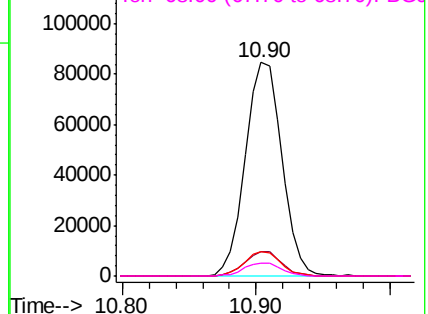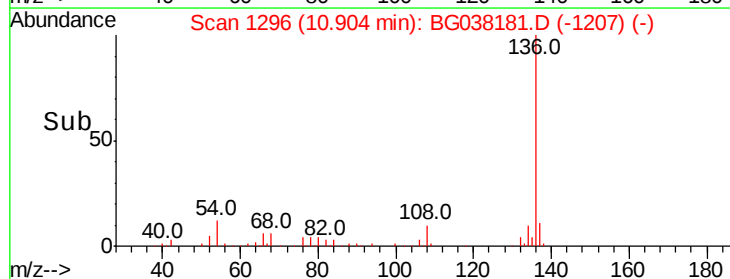


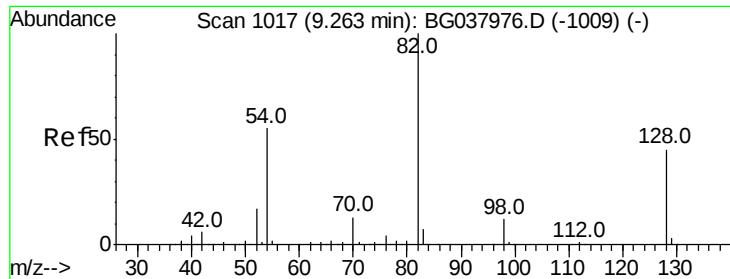




#23
Nitrobenzene-d5
Concen: 86.407 ng
RT: 9.26 min Scan# 1017
Delta R.T. 0.00 min
Lab File: BG038181.D
Acq: 28 Nov 2018 00:14

Instrument :
BNA_G
ClientSampleId :
SU-03-112118-B

Tot Ion	82	Resp	258589
Ion Ratio	Lower	Upper	
82	100		
128	43.8	34.6	51.8
54	59.1	45.3	67.9

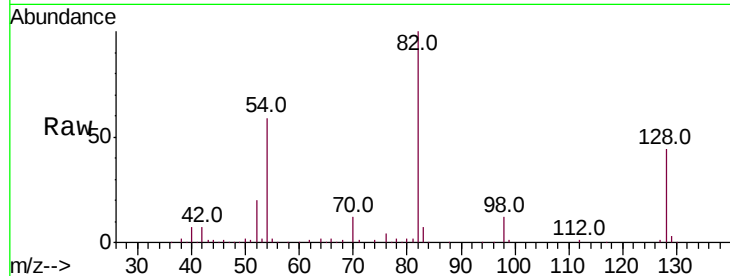


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

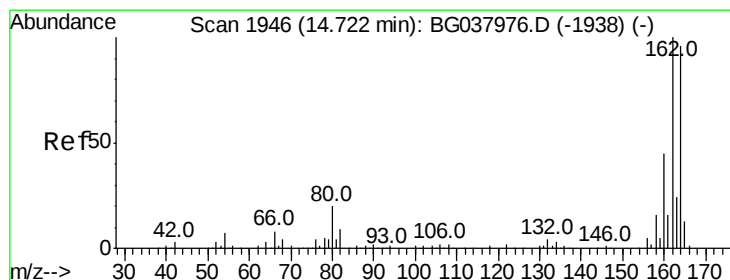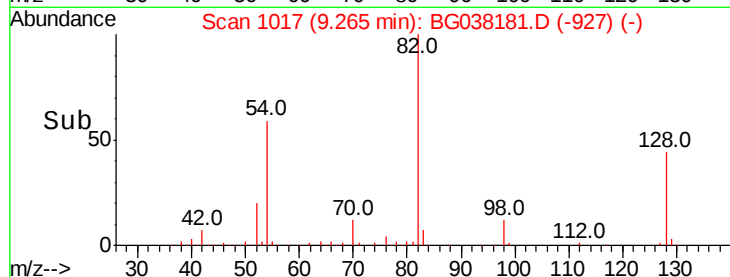
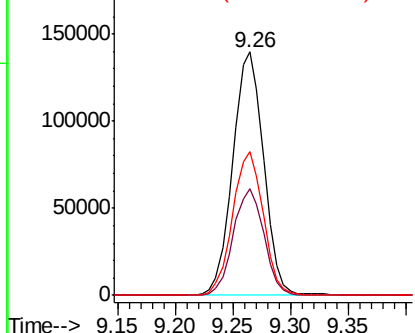


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.72 min Scan# 1946
Delta R.T. 0.00 min
Lab File: BG038181.D
Acq: 28 Nov 2018 00:14

Tgt Ion	164	Resp	97537
Ion Ratio	Lower	Upper	
164	100		
162	104.9	81.3	121.9
160	43.1	36.3	54.5

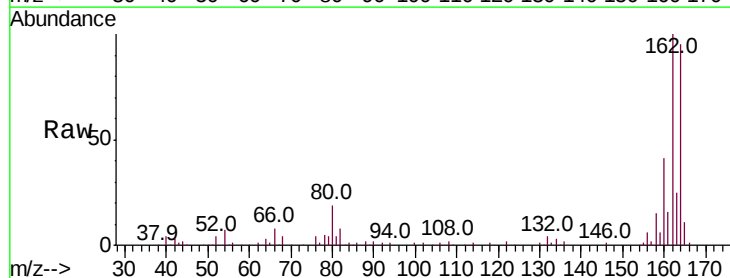

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

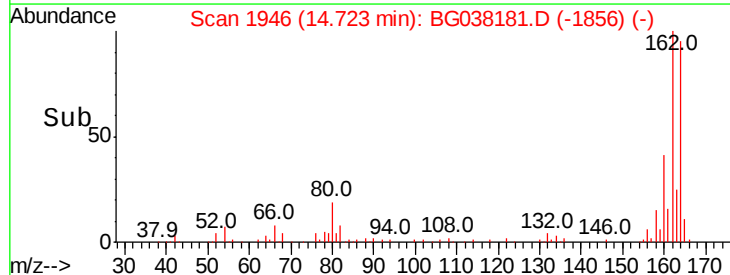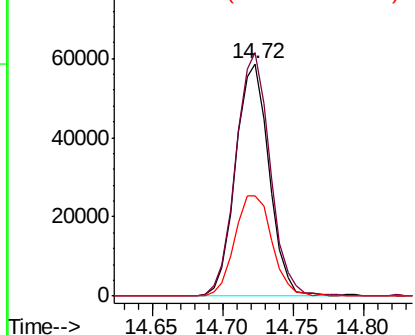






#42
 2,4,6-Tribromophenol
 Concen: 91.868 ng
 RT: 16.21 min Scan# 2199
 Delta R.T. -0.00 min
 Lab File: BG038181.D
 Acq: 28 Nov 2018 00:14

Instrument :
 BNA_G
 ClientSampleId :
 SU-03-112118-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.2	78.4	117.6
141	40.8	32.2	48.2

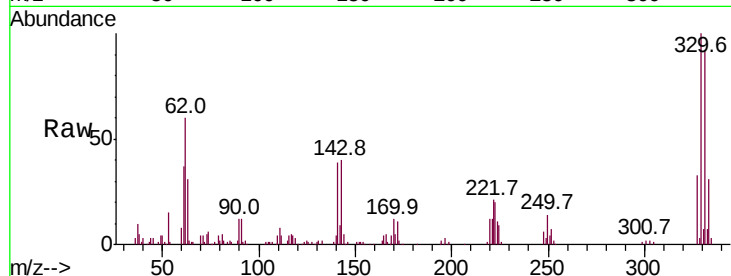


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

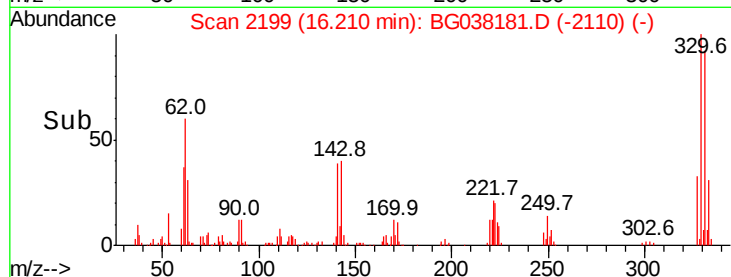
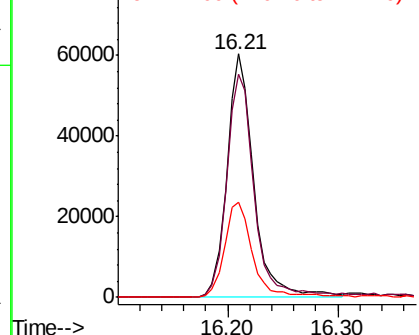



#45
 2-Fluorobiphenyl
 Concen: 78.566 ng
 RT: 13.34 min Scan# 1711
 Delta R.T. -0.00 min
 Lab File: BG038181.D
 Acq: 28 Nov 2018 00:14

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	31.0	46.4
170	24.3	20.2	30.2

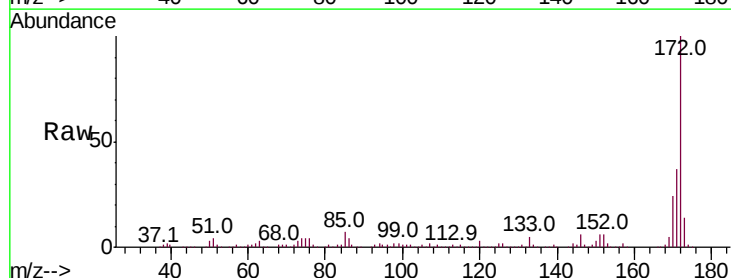

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

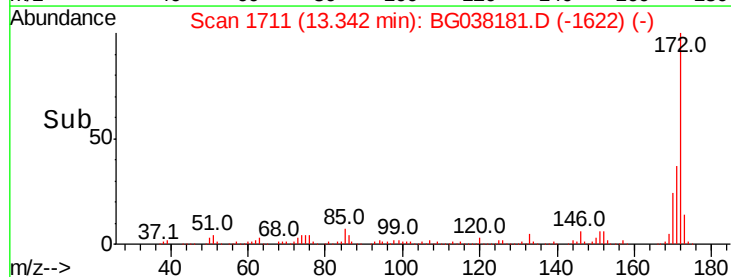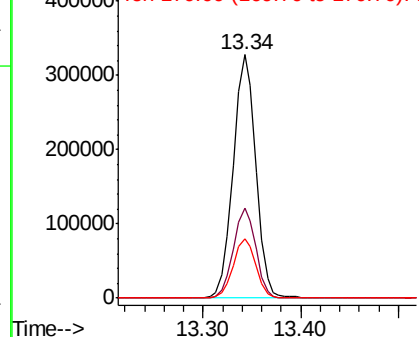


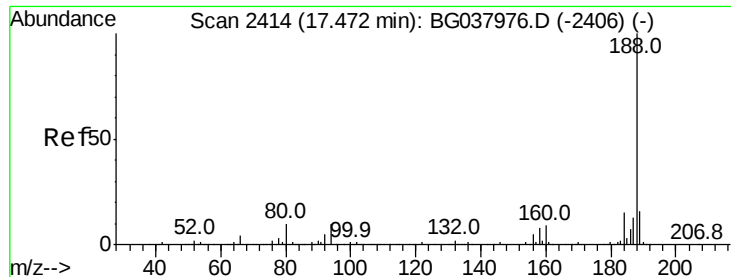




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.47 min Scan# 2413
Delta R.T. -0.00 min
Lab File: BG038181.D
Acq: 28 Nov 2018 00:14

Instrument :
BNA_G
ClientSampleId :
SU-03-112118-B

Tot Ion:188 Resp: 219173
Ion Ratio Lower Upper
188 100
94 8.8 7.2 10.8
80 9.9 7.7 11.5

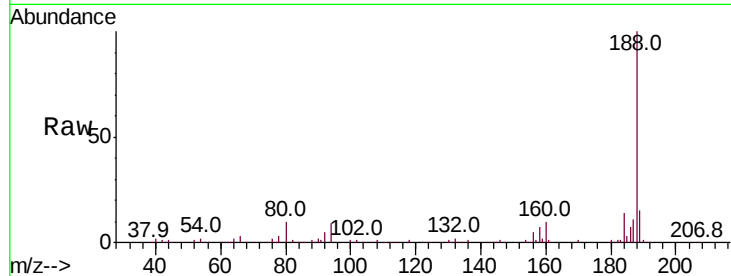


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BG
Ion 80.00 (79.70 to 80.70): BG

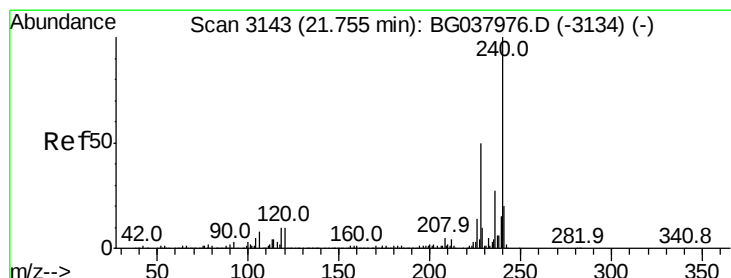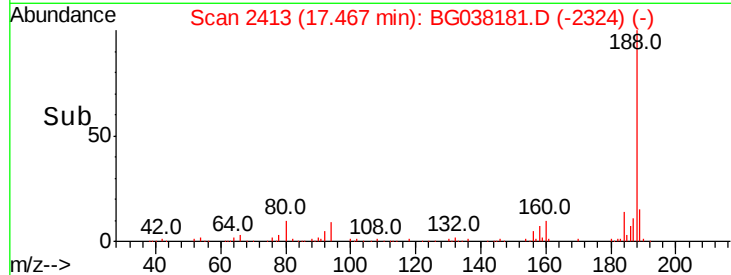
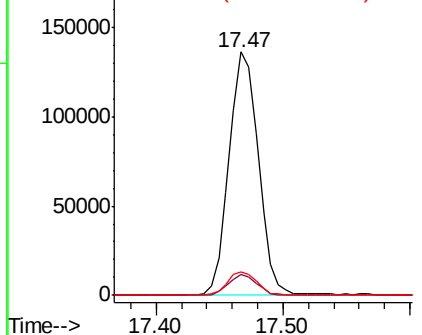


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.76 min Scan# 3143
Delta R.T. 0.00 min
Lab File: BG038181.D
Acq: 28 Nov 2018 00:14

Tgt Ion:240 Resp: 203980
Ion Ratio Lower Upper
240 100
120 10.3 8.1 12.1
236 26.1 21.4 32.0

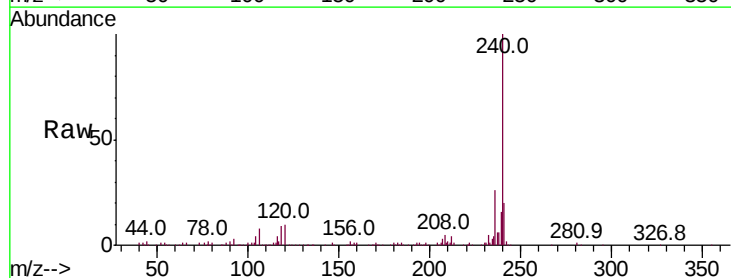

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

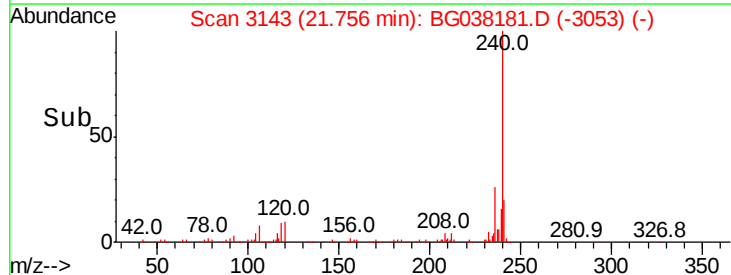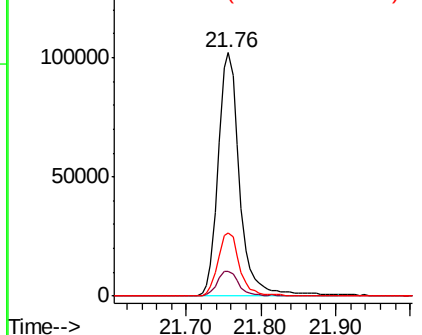



#79

Terphenyl-d14

Concen: 96.160 ng

RT: 20.07 min Scan# 2856

Delta R.T. 0.00 min

Lab File: BG038181.D

Acq: 28 Nov 2018 00:14

Instrument :

BNA_G

ClientSampleId :

SU-03-112118-B


Tot Ion:244 Resp: 833604

Ion Ratio Lower Upper

244 100

212 8.1 6.5 9.7




122 10.5 9.0 13.4

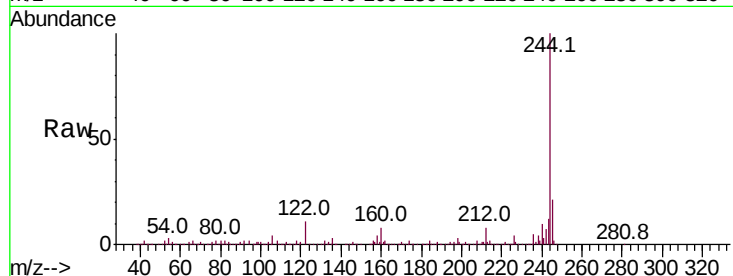

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

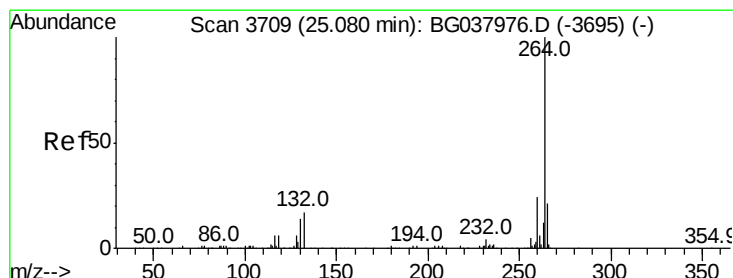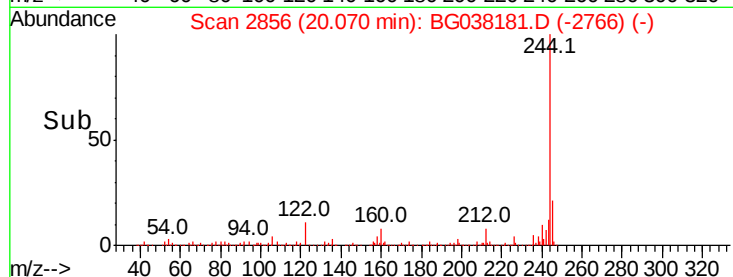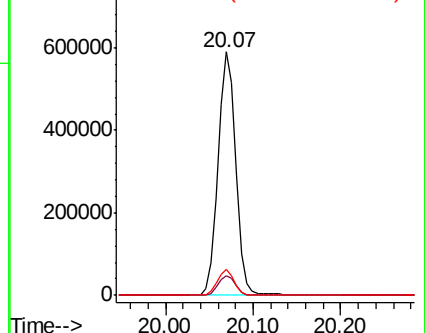

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.09 min Scan# 3710

Delta R.T. 0.01 min

Lab File: BG038181.D

Acq: 28 Nov 2018 00:14


Tgt Ion:264 Resp: 163307

Ion Ratio Lower Upper

264 100

260 24.1 18.2 27.4

265 23.0 17.9 26.9

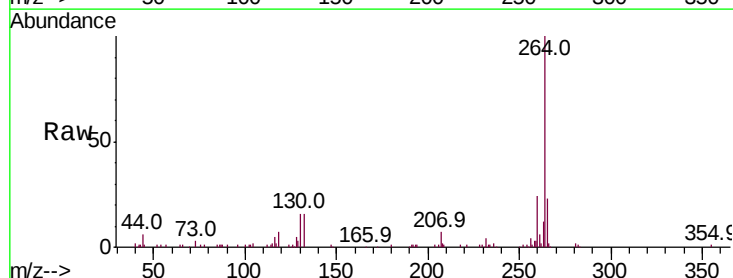

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

