

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112718\
 Data File : BG038187.D
 Acq On : 28 Nov 2018 5:30
 Operator : JU/SJ
 Sample : J6028-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMP-1

Quant Time: Nov 28 06:56:36 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	35774	20.00	ng	0.00
21) Naphthalene-d8	10.91	136	158054	20.00	ng	0.00
39) Acenaphthene-d10	14.72	164	97067	20.00	ng	0.00
64) Phenanthrene-d10	17.47	188	224010	20.00	ng	0.00
76) Chrysene-d12	21.75	240	212591	20.00	ng	0.00
87) Perylene-d12	25.09	264	177807	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	234948	113.39	ng	0.00
7) Phenol-d6	7.24	99	293274	99.16	ng	0.00
23) Nitrobenzene-d5	9.26	82	243747	82.55	ng	0.00
42) 2,4,6-Tribromophenol	16.21	330	99289	89.69	ng	0.00
45) 2-Fluorobiphenyl	13.34	172	500869	75.17	ng	0.00
79) Terphenyl-d14	20.07	244	846002	93.64	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112718\
Data File : BG038187.D
Acq On : 28 Nov 2018 5:30
Operator : JU/SJ
Sample : J6028-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-1

Quant Time: Nov 28 06:56:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

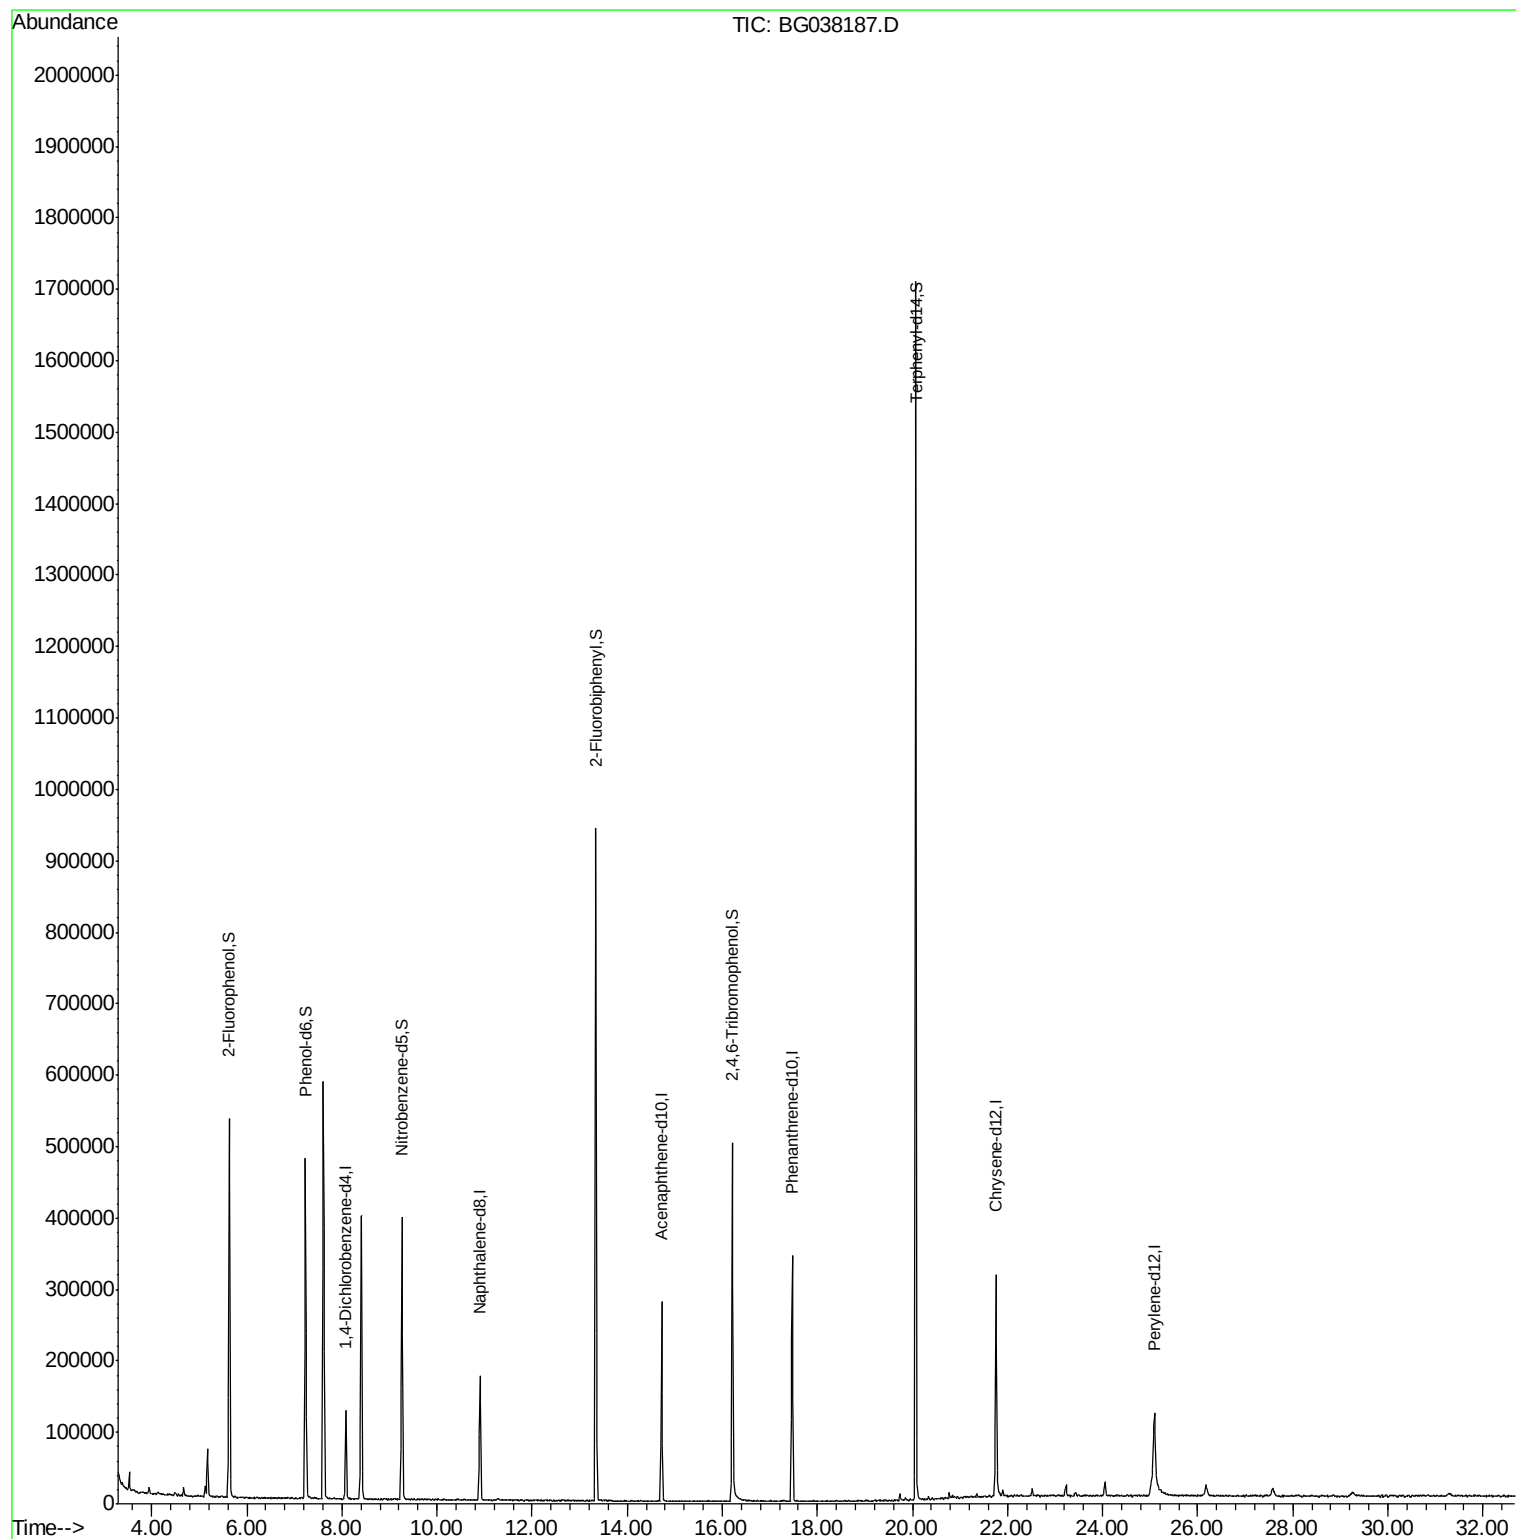

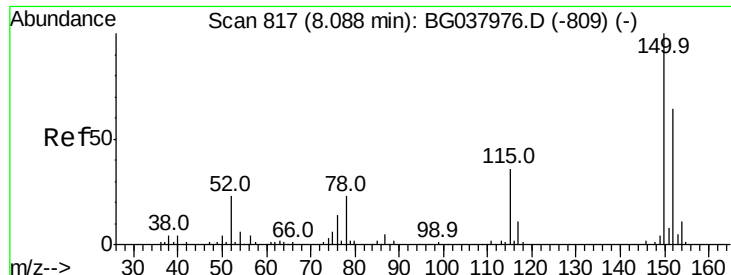


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.08 min Scan# 816
 Delta R.T. -0.01 min
 Lab File: BG038187.D
 Acq: 28 Nov 2018 5:30

Instrument :
 BNA_G
 ClientSampleId :
 COMP-1

Tot Ion:152 Resp: 35774
 Ion Ratio Lower Upper
 152 100
 150 163.1 126.0 189.0
 115 59.3 45.5 68.3

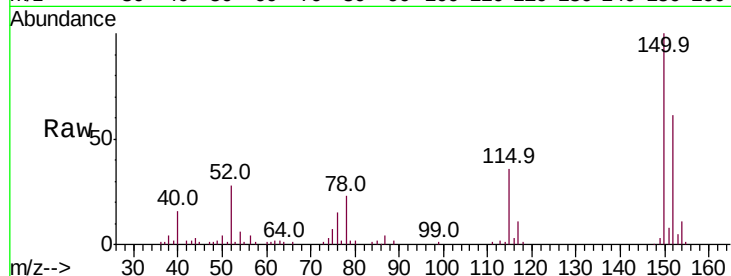


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

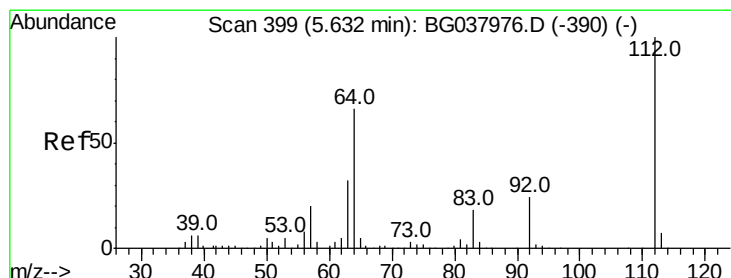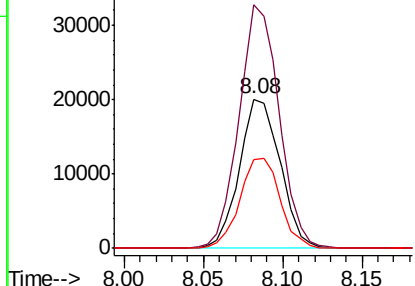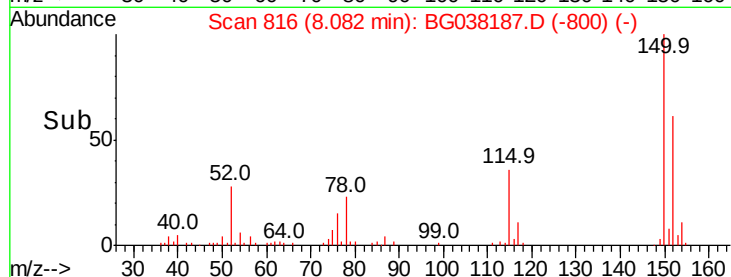



#5


2-Fluorophenol
 Concen: 113.393 ng
 RT: 5.63 min Scan# 399
 Delta R.T. -0.00 min
 Lab File: BG038187.D
 Acq: 28 Nov 2018 5:30

Tgt Ion:112 Resp: 234948
 Ion Ratio Lower Upper
 112 100
 64 68.3 53.1 79.7
 63 34.6 27.3 40.9

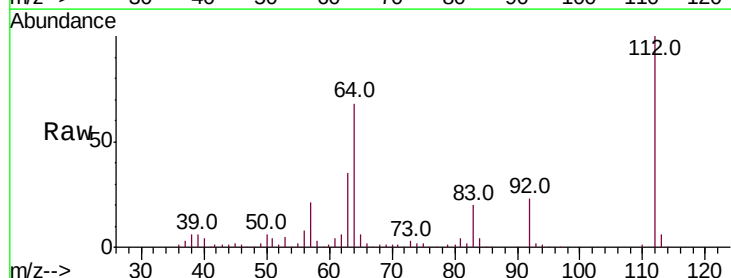

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

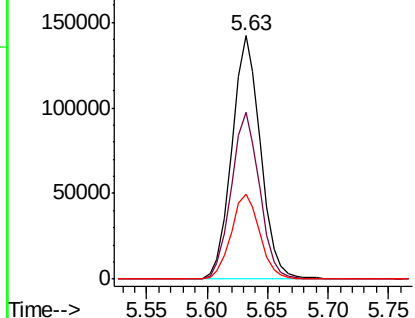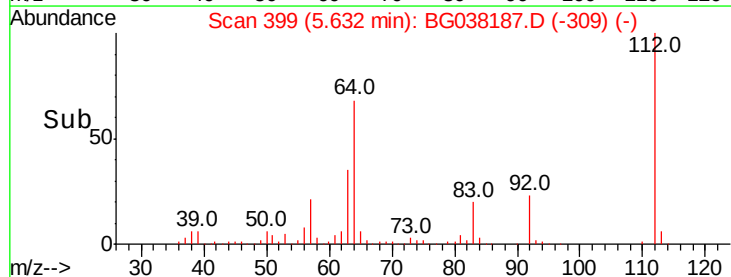

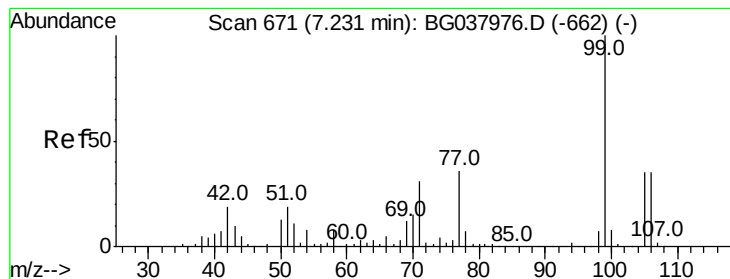

#7

Phenol-d6

Concen: 99.159 ng

RT: 7.24 min Scan# 672

Delta R.T. 0.01 min

Lab File: BG038187.D

Acq: 28 Nov 2018 5:30

Instrument :

BNA_G

ClientSampleId :

COMP-1


Tot Ion: 99 Resp: 293274

Ion Ratio Lower Upper




99 100

42 20.6 15.0 22.4

71 35.2 25.5 38.3

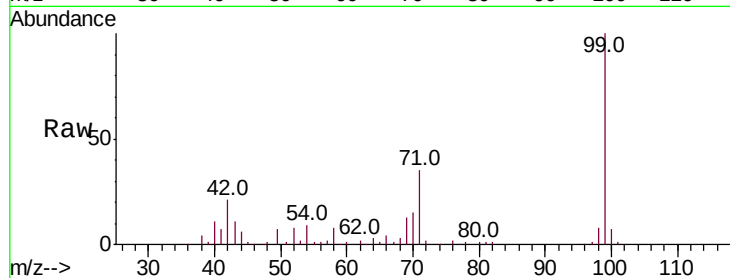

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

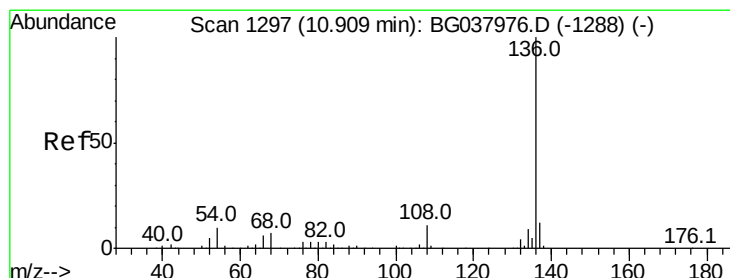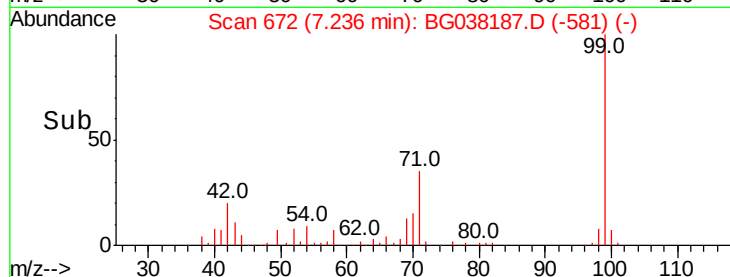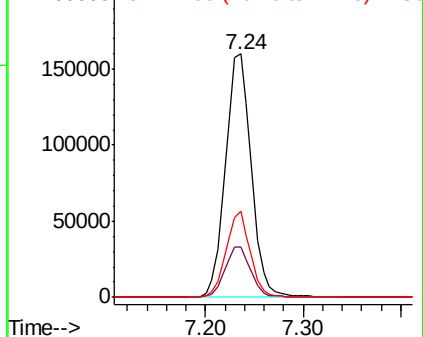

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.91 min Scan# 1297

Delta R.T. -0.00 min

Lab File: BG038187.D

Acq: 28 Nov 2018 5:30

Tgt Ion: 136 Resp: 158054


Ion Ratio Lower Upper

136 100



137 10.4 9.6 14.4


54 11.3 7.9 11.9

68 6.7 4.8 7.2

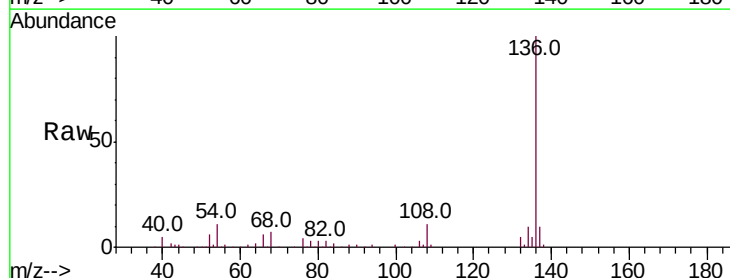

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

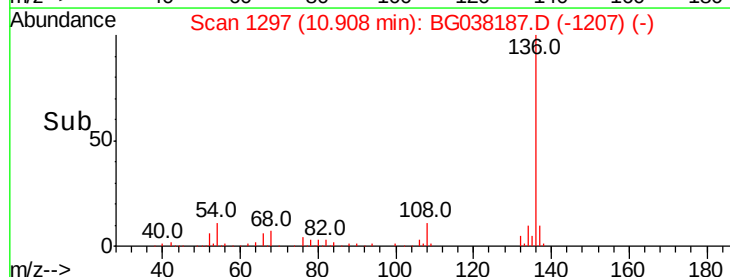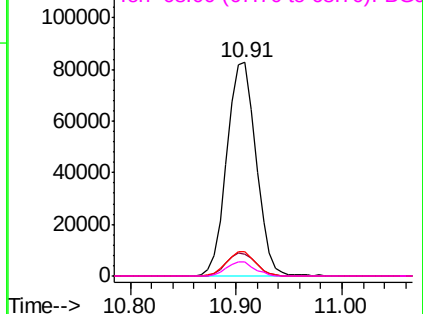

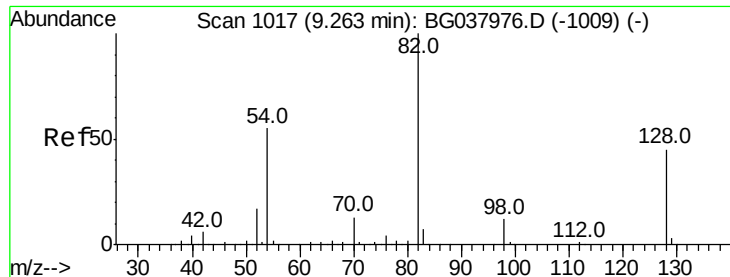

#23

Nitrobenzene-d5

Concen: 82.553 ng

RT: 9.26 min Scan# 1017

Delta R.T. -0.00 min

Lab File: BG038187.D

Acq: 28 Nov 2018 5:30

Instrument :

BNA_G

ClientSampleId :

COMP-1


Tot Ion: 82 Resp: 243747

Ion Ratio Lower Upper




82 100

128 42.6 34.6 51.8

54 57.5 45.3 67.9

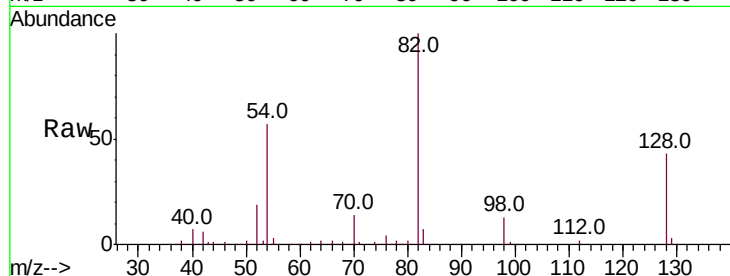

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

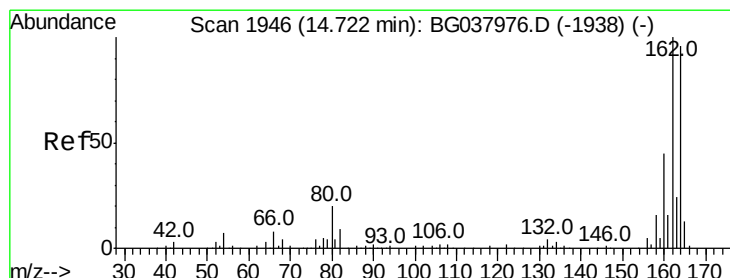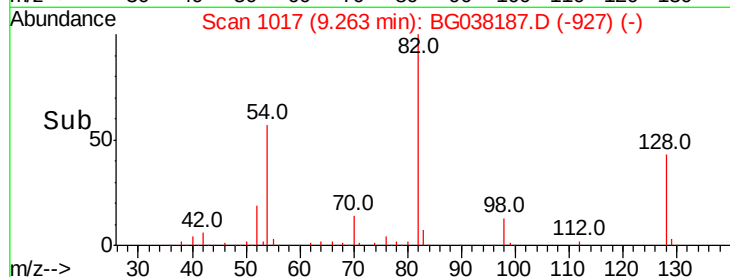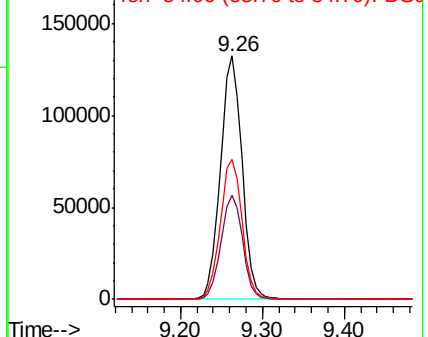

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.72 min Scan# 1946

Delta R.T. -0.00 min

Lab File: BG038187.D

Acq: 28 Nov 2018 5:30


Tgt Ion:164 Resp: 97067

Ion Ratio Lower Upper



164 100


162 110.7 81.3 121.9

160 47.9 36.3 54.5

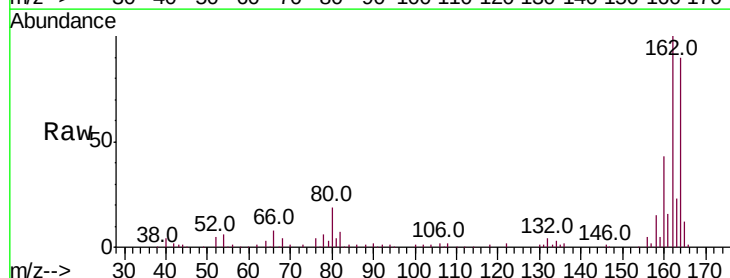

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

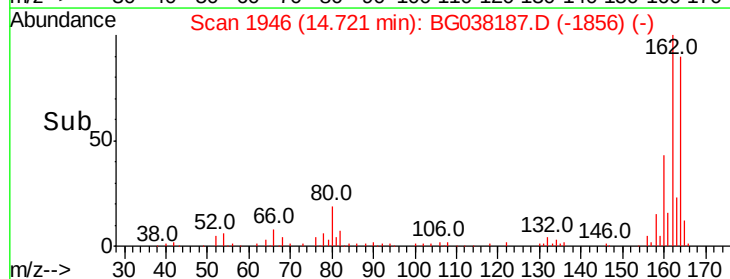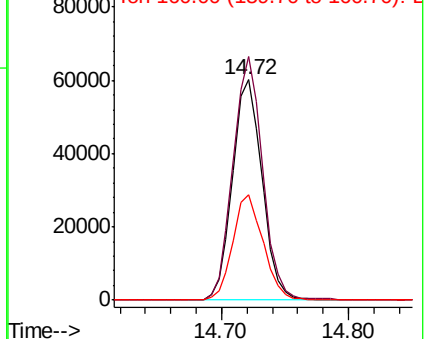


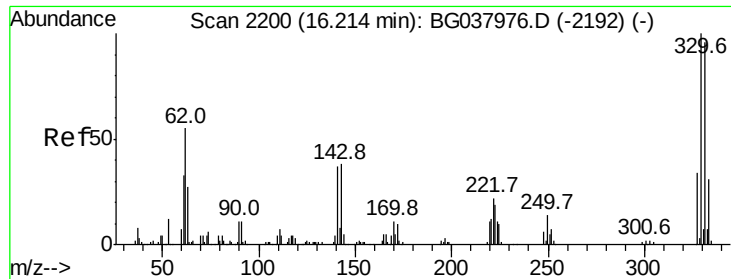




#42
 2,4,6-Tribromophenol
 Concen: 89.690 ng
 RT: 16.21 min Scan# 2199
 Delta R.T. -0.01 min
 Lab File: BG038187.D
 Acq: 28 Nov 2018 5:30

Instrument :
 BNA_G
 ClientSampleId :
 COMP-1

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.3	78.4	117.6
141	41.9	32.2	48.2

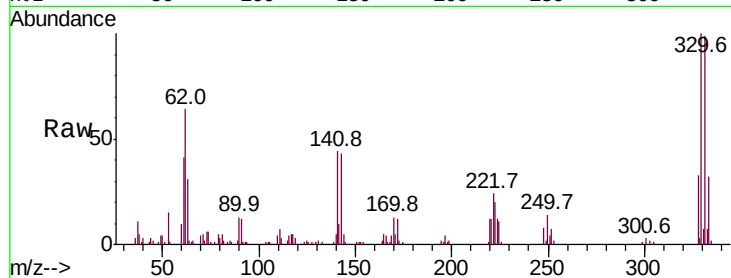


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

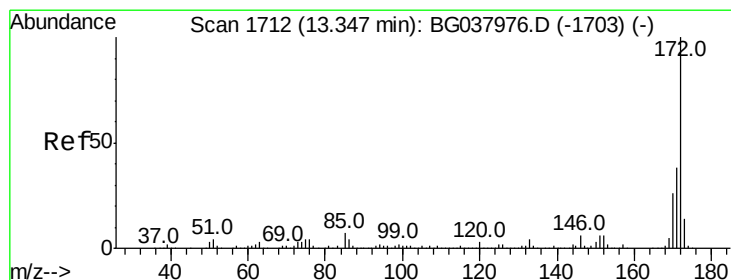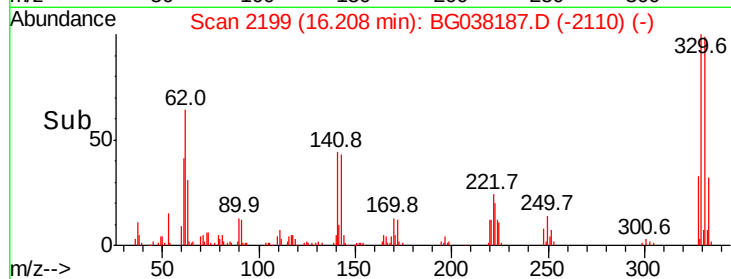
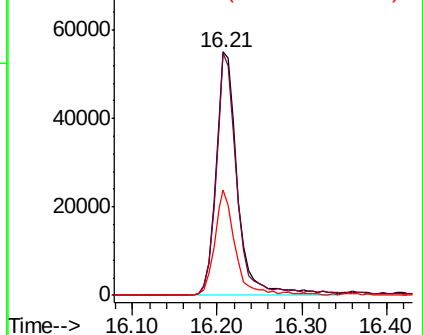



#45
 2-Fluorobiphenyl
 Concen: 75.174 ng
 RT: 13.34 min Scan# 1711
 Delta R.T. -0.01 min
 Lab File: BG038187.D
 Acq: 28 Nov 2018 5:30

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	31.0	46.4
170	24.8	20.2	30.2

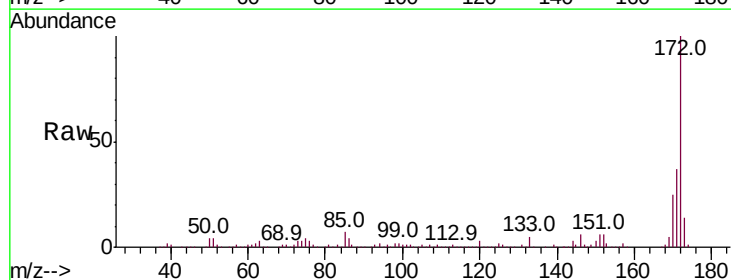

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

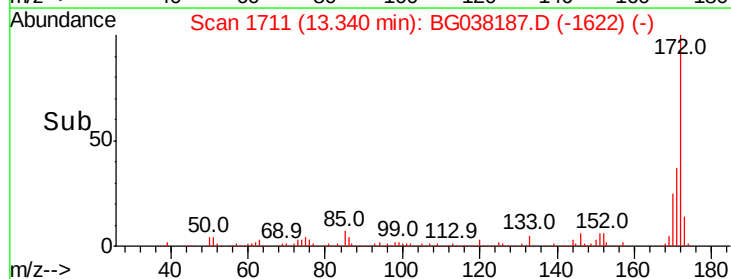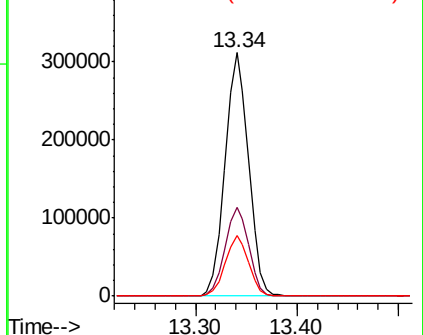


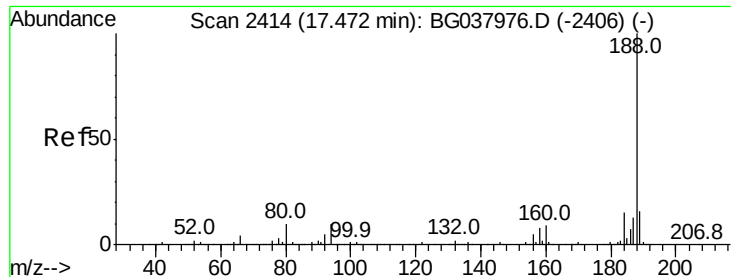




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.47 min Scan# 2414
Delta R.T. -0.00 min
Lab File: BG038187.D
Acq: 28 Nov 2018 5:30

Instrument :
BNA_G
ClientSampleId :
COMP-1

Tot Ion:188 Resp: 224010
Ion Ratio Lower Upper
188 100
94 9.9 7.2 10.8
80 9.9 7.7 11.5

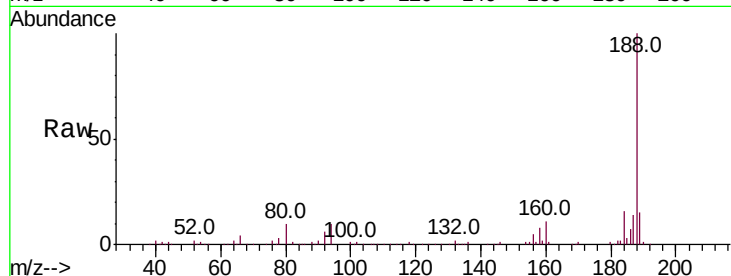


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGO
Ion 80.00 (79.70 to 80.70): BGO

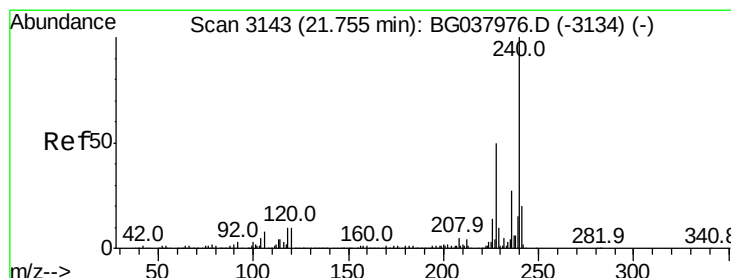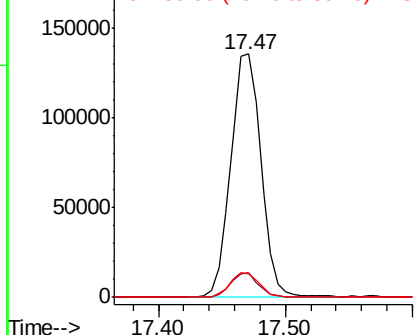
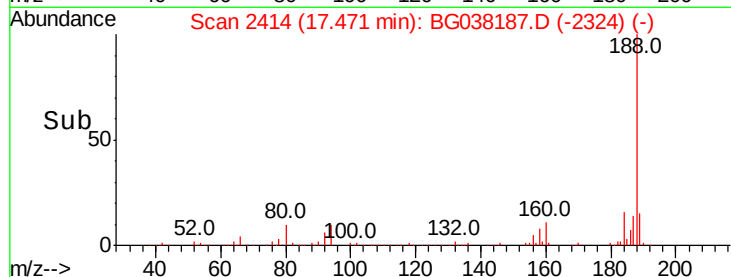



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.75 min Scan# 3143
Delta R.T. -0.00 min
Lab File: BG038187.D
Acq: 28 Nov 2018 5:30

Tgt Ion:240 Resp: 212591
Ion Ratio Lower Upper
240 100
120 10.4 8.1 12.1
236 25.0 21.4 32.0

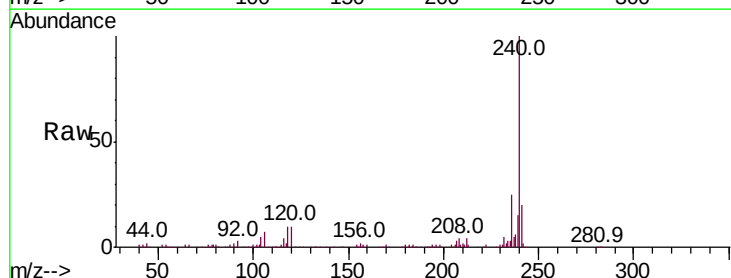

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



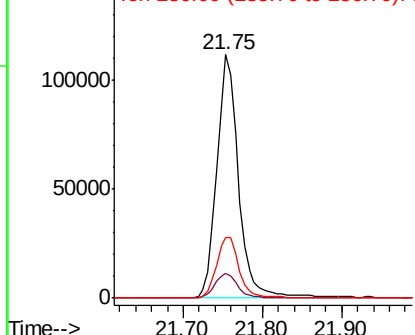
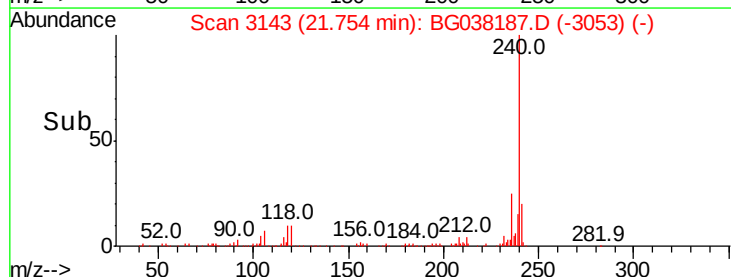


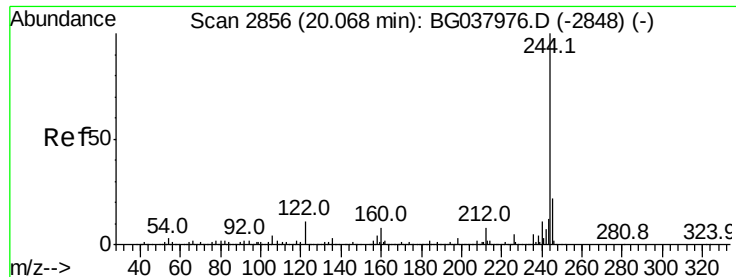

#79
 Terphenyl-d14
 Concen: 93.638 ng
 RT: 20.07 min Scan# 2856
 Delta R.T. -0.00 min
 Lab File: BG038187.D
 Acq: 28 Nov 2018 5:30

Instrument :
 BNA_G
 ClientSampleId :
 COMP-1

Tot Ion:244 Resp: 846002
 Ion Ratio Lower Upper
 244 100
 212 7.9 6.5 9.7
 122 10.4 9.0 13.4

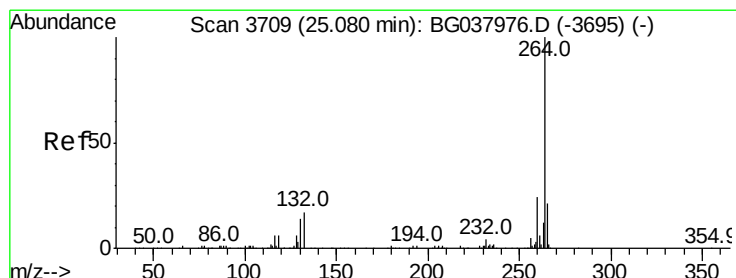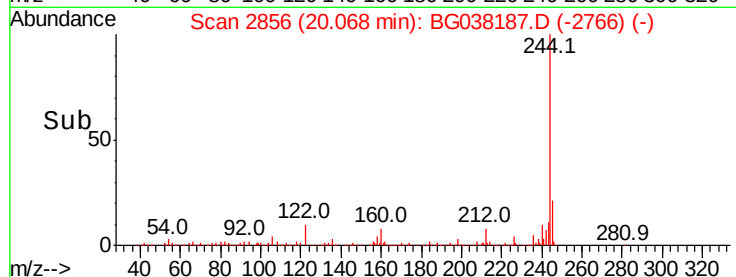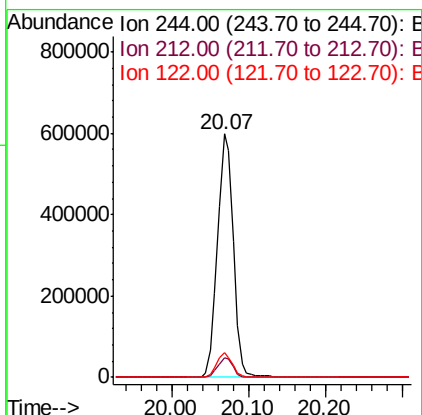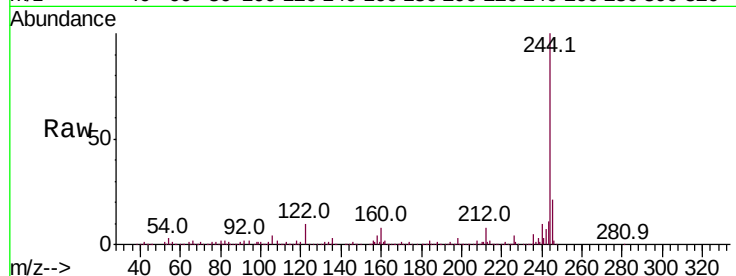

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.09 min Scan# 3710
 Delta R.T. 0.01 min
 Lab File: BG038187.D
 Acq: 28 Nov 2018 5:30

Tgt Ion:264 Resp: 177807
 Ion Ratio Lower Upper
 264 100
 260 25.3 18.2 27.4
 265 21.2 17.9 26.9

