

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112718\
 Data File : BG038189.D
 Acq On : 28 Nov 2018 6:48
 Operator : JU/SJ
 Sample : J6028-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMP-3

Quant Time: Nov 28 07:27:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	38117	20.00	ng	0.00
21) Naphthalene-d8	10.90	136	165795	20.00	ng	0.00
39) Acenaphthene-d10	14.72	164	107289	20.00	ng	0.00
64) Phenanthrene-d10	17.47	188	240891	20.00	ng	0.00
76) Chrysene-d12	21.75	240	223745	20.00	ng	0.00
87) Perylene-d12	25.09	264	193485	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	255064	115.53	ng	0.00
7) Phenol-d6	7.23	99	326336	103.56	ng	0.00
23) Nitrobenzene-d5	9.27	82	255217	82.40	ng	0.00
42) 2,4,6-Tribromophenol	16.21	330	106398	86.95	ng	0.00
45) 2-Fluorobiphenyl	13.34	172	532618	72.32	ng	0.00
79) Terphenyl-d14	20.07	244	886590	93.24	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112718\
Data File : BG038189.D
Acq On : 28 Nov 2018 6:48
Operator : JU/SJ
Sample : J6028-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-3

Quant Time: Nov 28 07:27:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

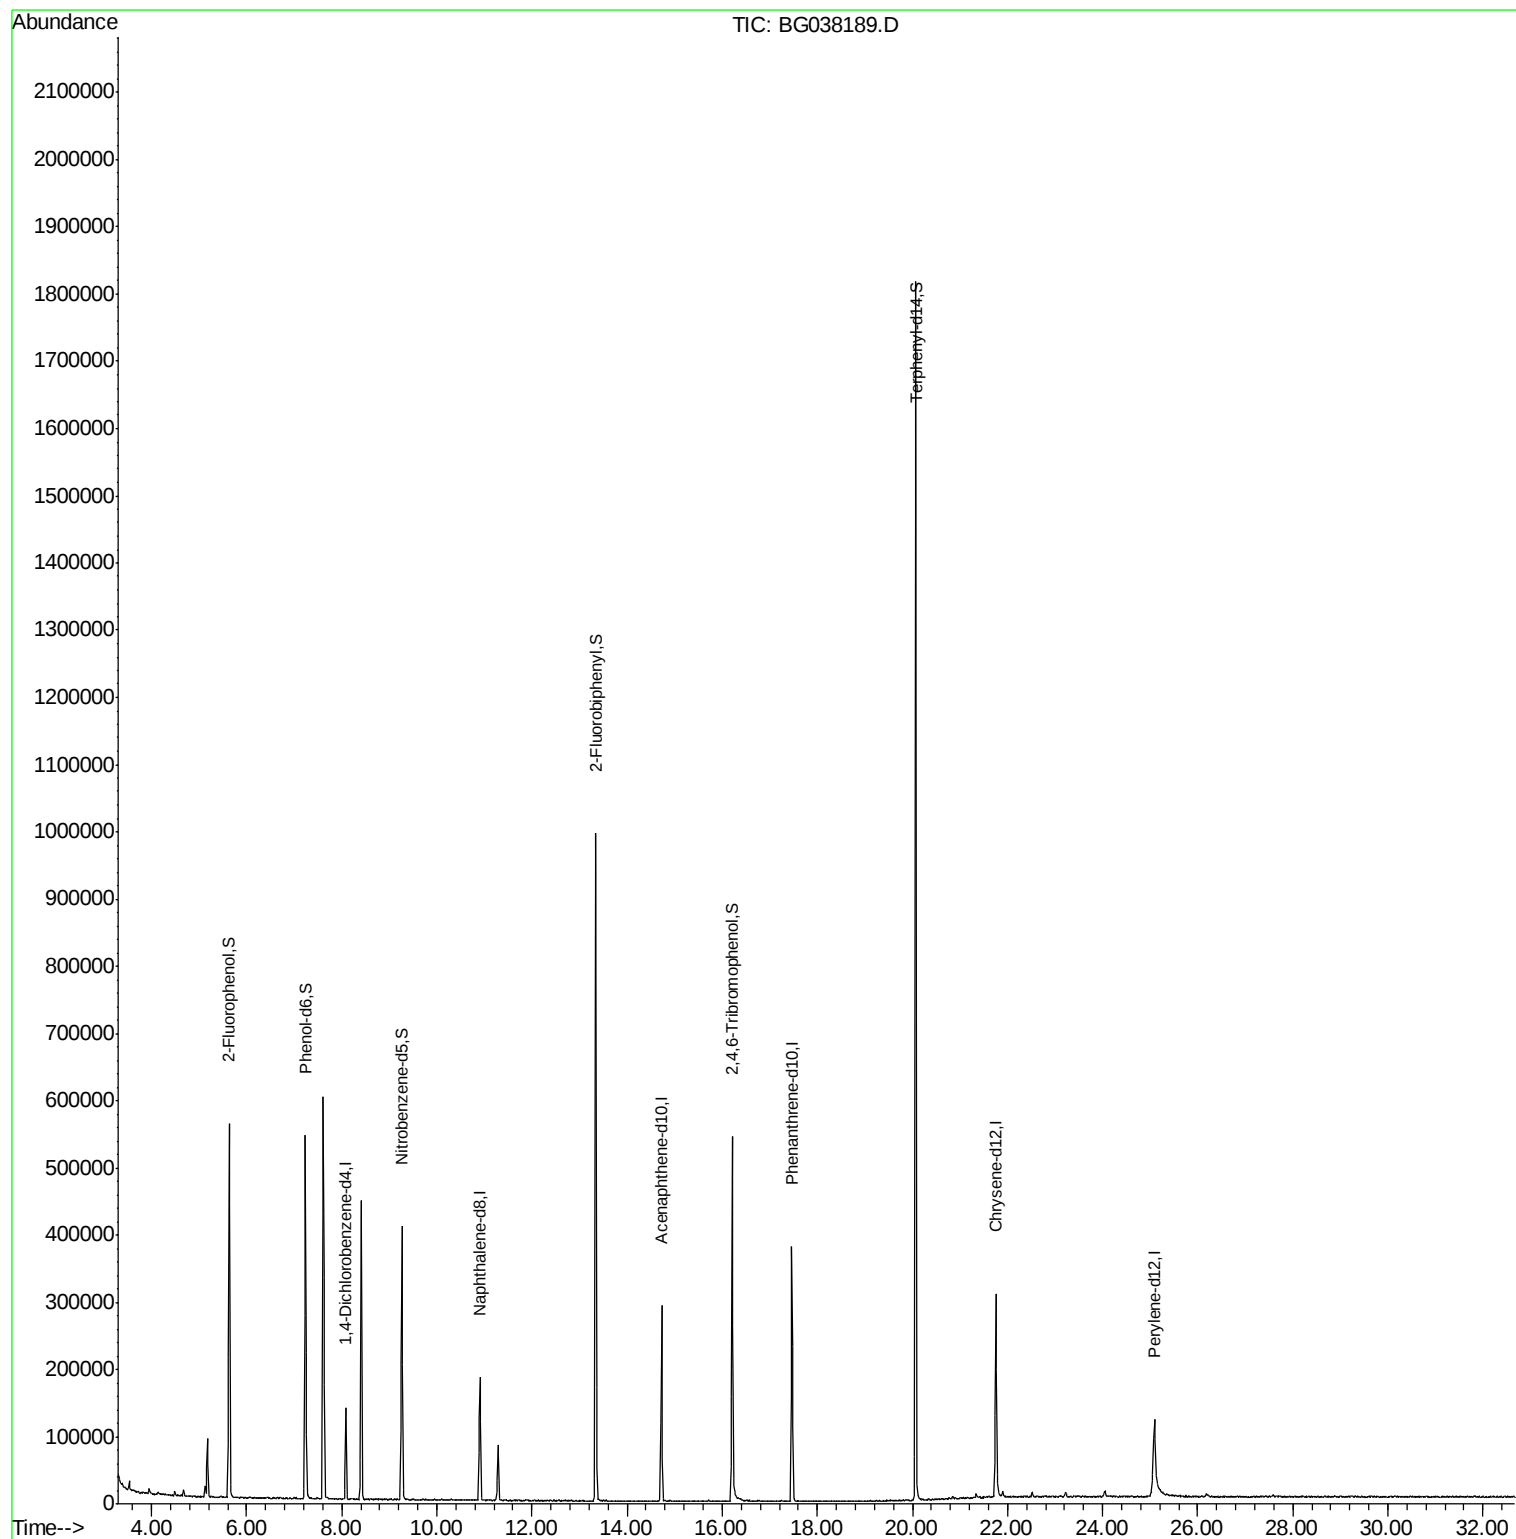

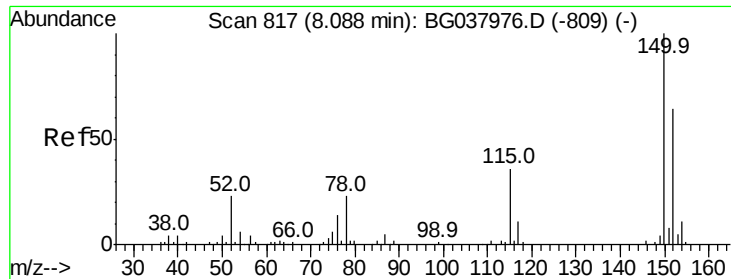

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.08 min Scan# 816

Delta R.T. -0.00 min

Lab File: BG038189.D

Acq: 28 Nov 2018 6:48

Instrument :

BNA_G

ClientSampleId :

COMP-3


Tot Ion:152 Resp: 38117

Ion Ratio Lower Upper

152 100

150 163.3 126.0 189.0




115 60.0 45.5 68.3

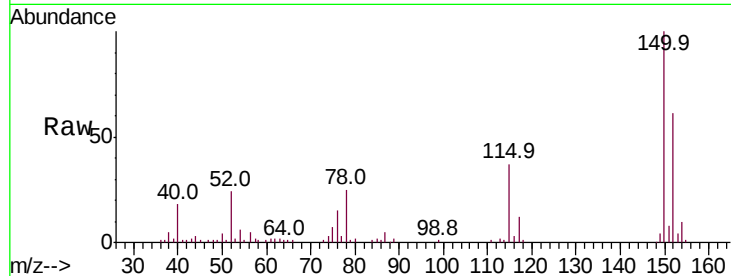

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

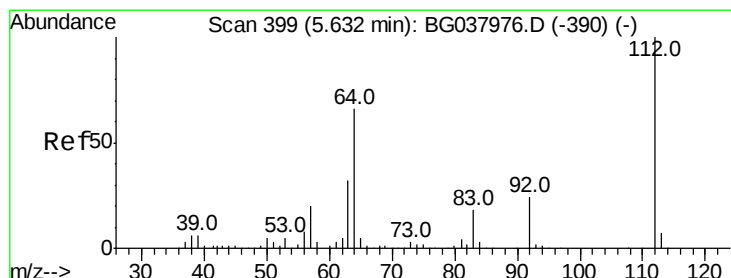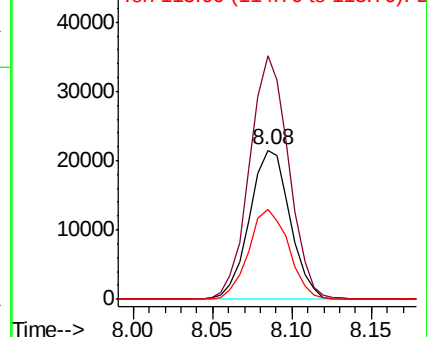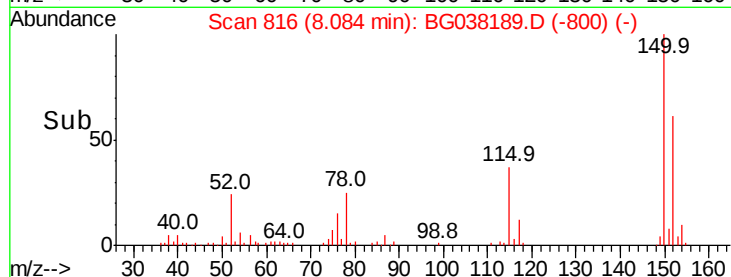

#5

2-Fluorophenol

Concen: 115.535 ng

RT: 5.63 min Scan# 399

Delta R.T. 0.00 min

Lab File: BG038189.D

Acq: 28 Nov 2018 6:48


Tgt Ion:112 Resp: 255064

Ion Ratio Lower Upper

112 100

64 67.0 53.1 79.7



63 34.6 27.3 40.9

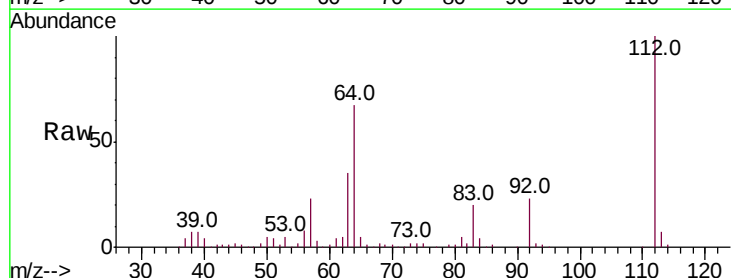


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

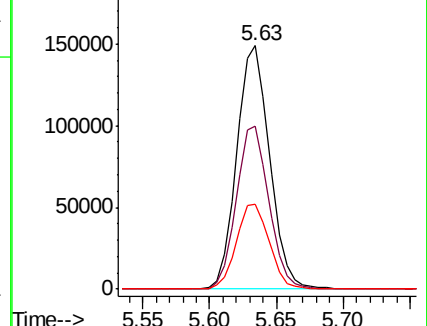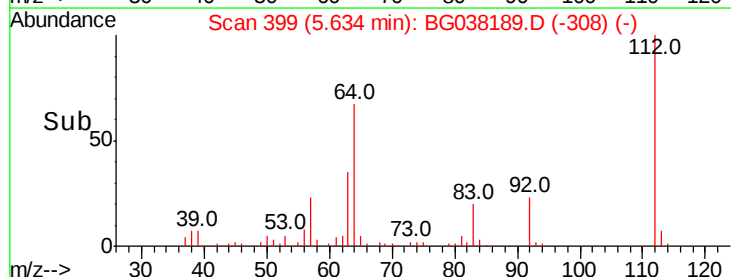

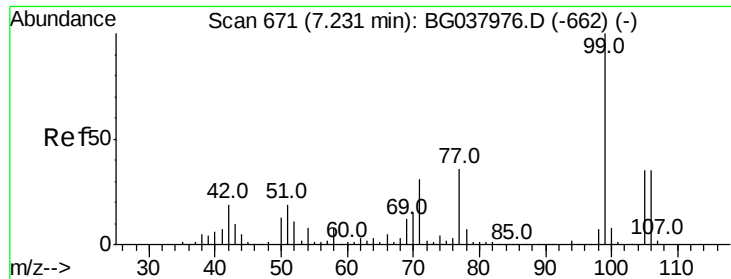

#7

Phenol-d6

Concen: 103.555 ng

RT: 7.23 min Scan# 671

Delta R.T. 0.00 min

Lab File: BG038189.D

Acq: 28 Nov 2018 6:48

Instrument :

BNA_G

ClientSampleId :

COMP-3


Tot Ion: 99 Resp: 326336

Ion Ratio Lower Upper




99 100

42 21.4 15.0 22.4

71 33.3 25.5 38.3

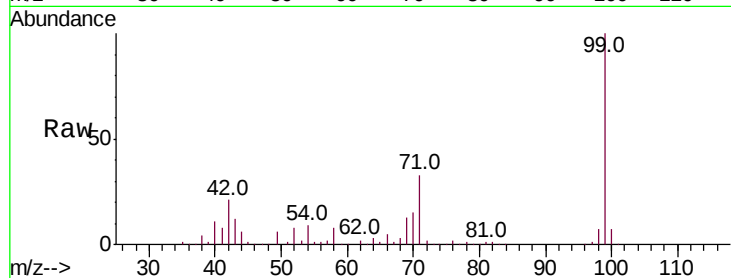

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

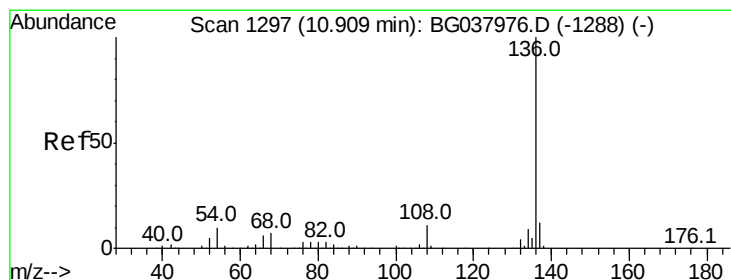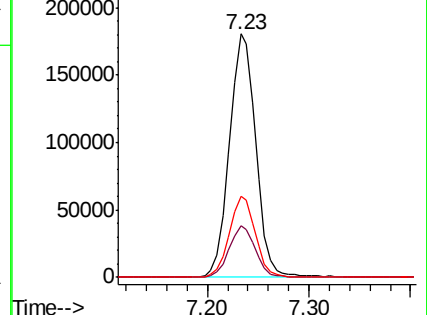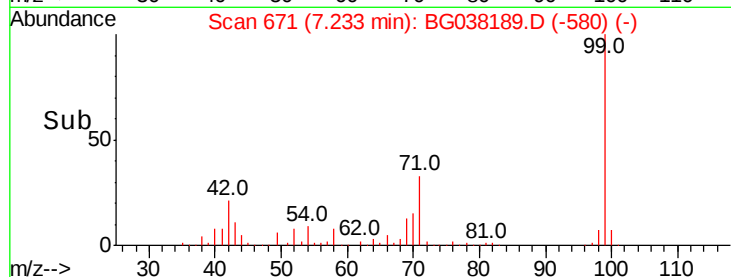

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.90 min Scan# 1296

Delta R.T. -0.00 min

Lab File: BG038189.D

Acq: 28 Nov 2018 6:48

Tgt Ion: 136 Resp: 165795


Ion Ratio Lower Upper

136 100



137 11.8 9.6 14.4


54 10.4 7.9 11.9

68 5.6 4.8 7.2

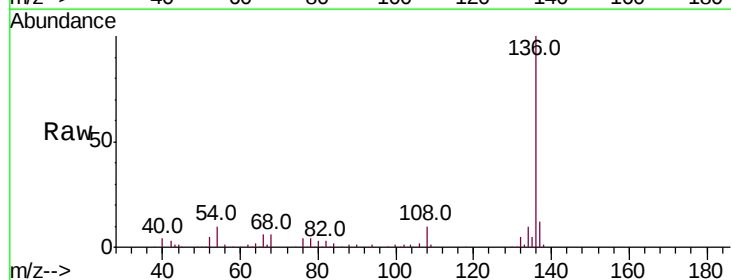

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

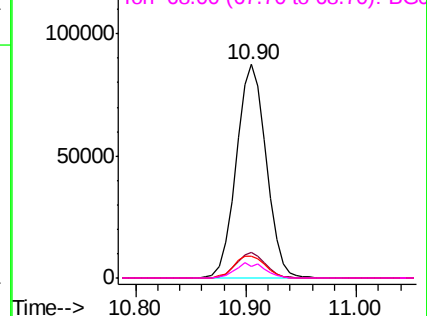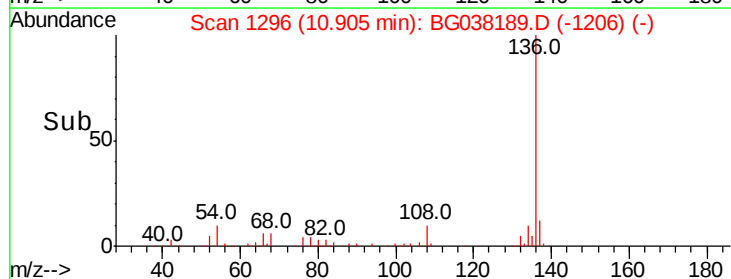


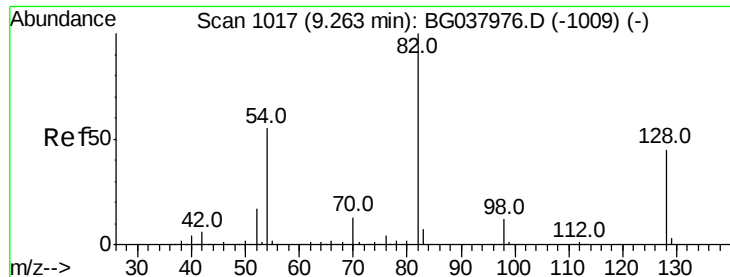




#23
Nitrobenzene-d5
Concen: 82.402 ng
RT: 9.27 min Scan# 1017
Delta R.T. 0.00 min
Lab File: BG038189.D
Acq: 28 Nov 2018 6:48

Instrument :
BNA_G
ClientSampleId :
COMP-3

Tot Ion	82	Resp	255217
Ion Ratio	100	Lower	Upper
128	44.4	34.6	51.8
54	58.5	45.3	67.9

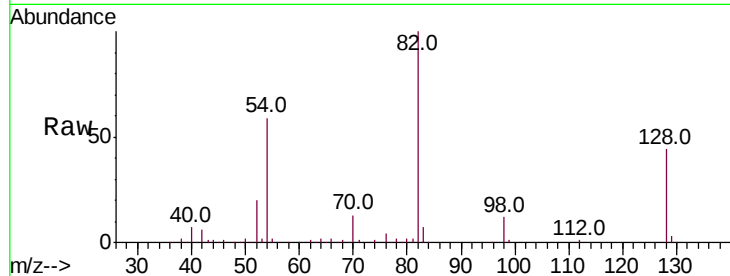


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

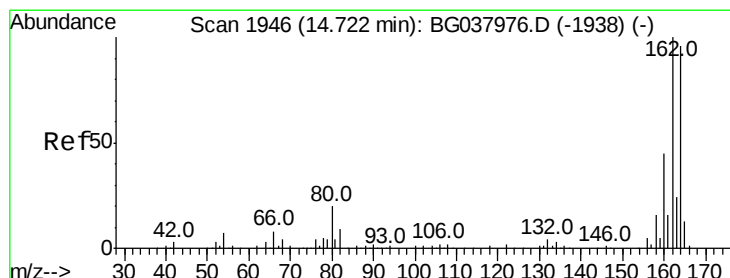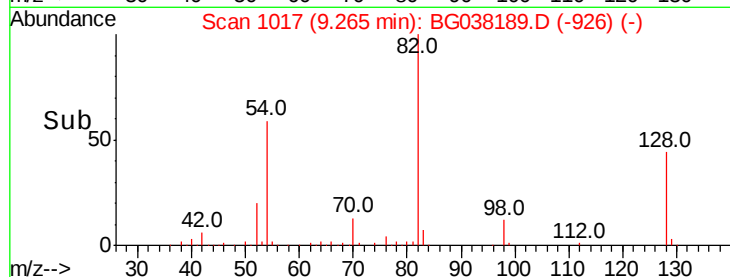
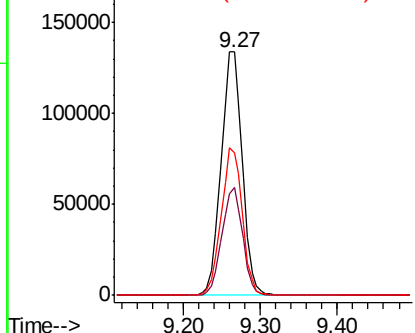



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.72 min Scan# 1946
Delta R.T. 0.00 min
Lab File: BG038189.D
Acq: 28 Nov 2018 6:48

Tgt Ion	164	Resp	107289
Ion Ratio	100	Lower	Upper
162	100.3	81.3	121.9
160	45.2	36.3	54.5

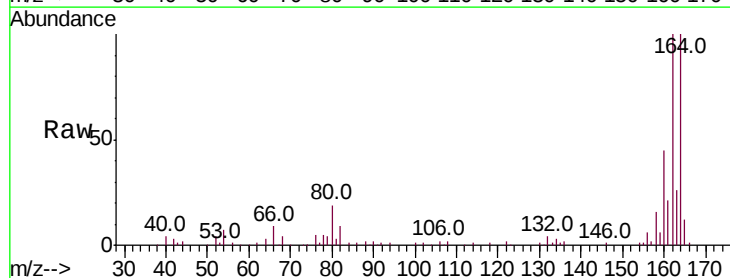

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

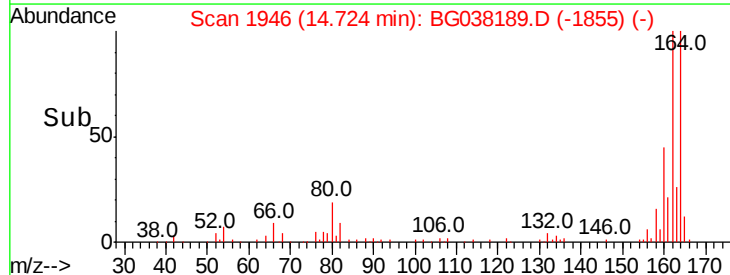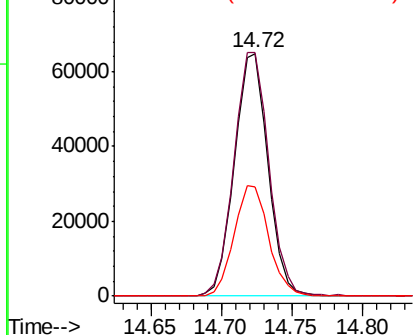


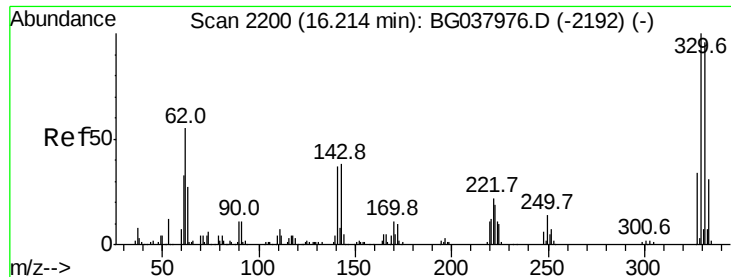




#42
 2,4,6-Tribromophenol
 Concen: 86.955 ng
 RT: 16.21 min Scan# 2199
 Delta R.T. -0.00 min
 Lab File: BG038189.D
 Acq: 28 Nov 2018 6:48

Instrument :
 BNA_G
 ClientSampleId :
 COMP-3

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	78.4	117.6
141	41.6	32.2	48.2

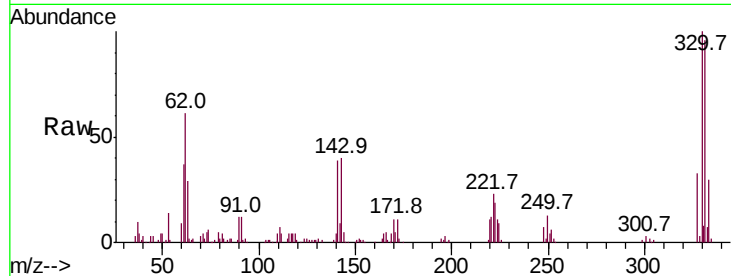


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

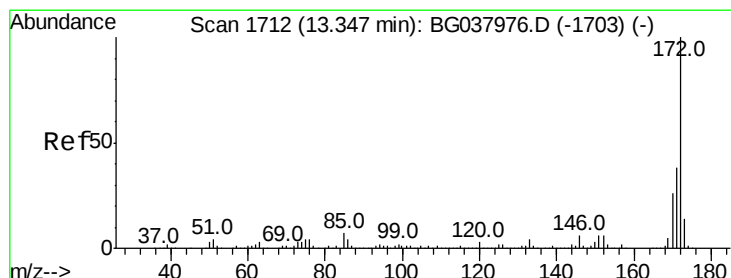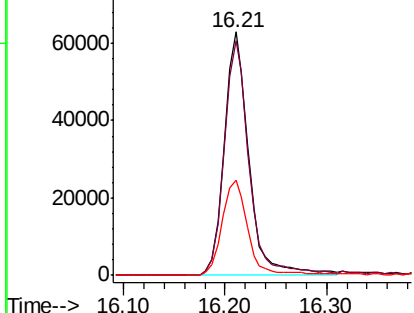
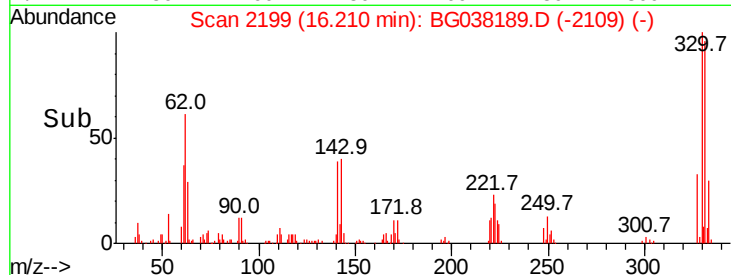



#45
 2-Fluorobiphenyl
 Concen: 72.323 ng
 RT: 13.34 min Scan# 1711
 Delta R.T. -0.00 min
 Lab File: BG038189.D
 Acq: 28 Nov 2018 6:48

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.9	31.0	46.4
170	24.4	20.2	30.2

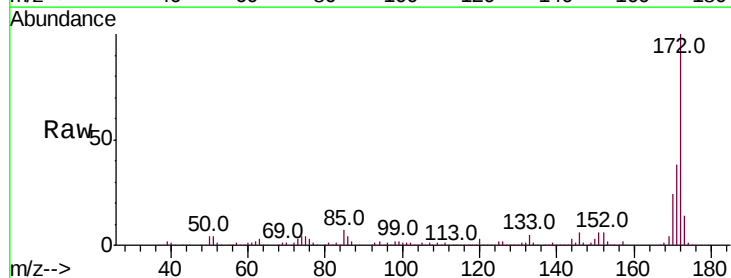

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

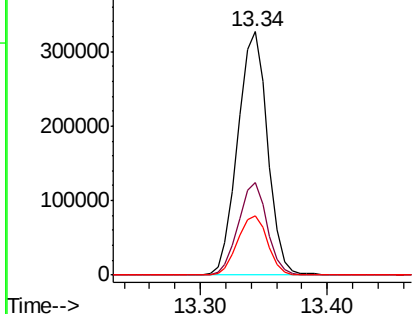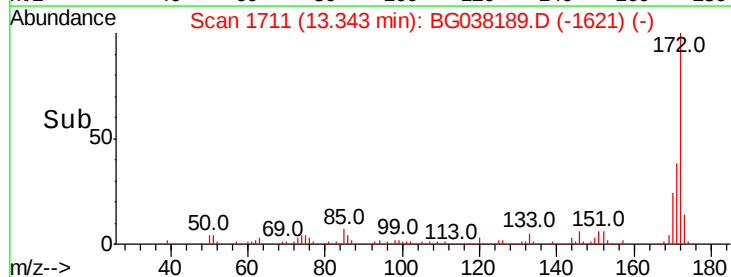

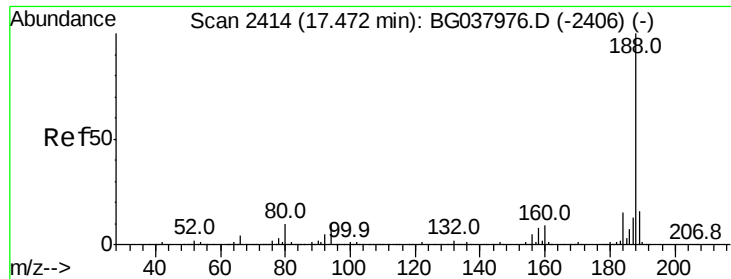

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.47 min Scan# 2413

Delta R.T. -0.00 min

Lab File: BG038189.D

Acq: 28 Nov 2018 6:48

Instrument :

BNA_G

ClientSampleId :

COMP-3


Tot Ion:188 Resp: 240891

Ion Ratio Lower Upper

188 100

94 8.2 7.2 10.8




80 10.4 7.7 11.5

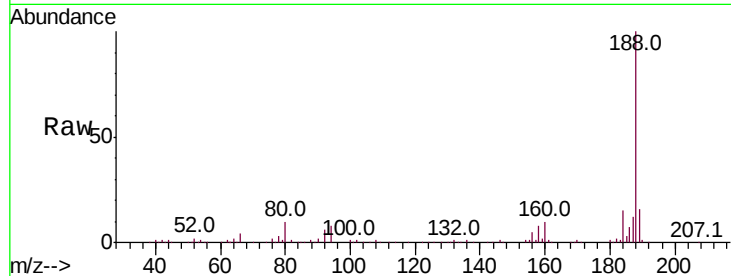

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

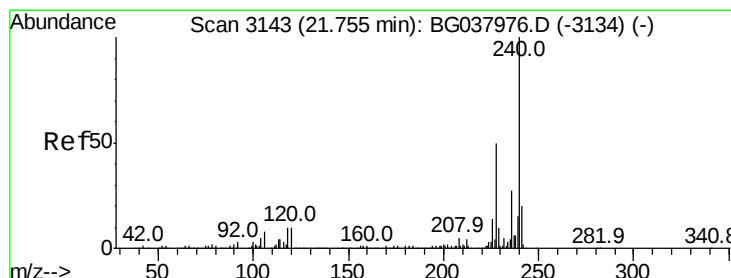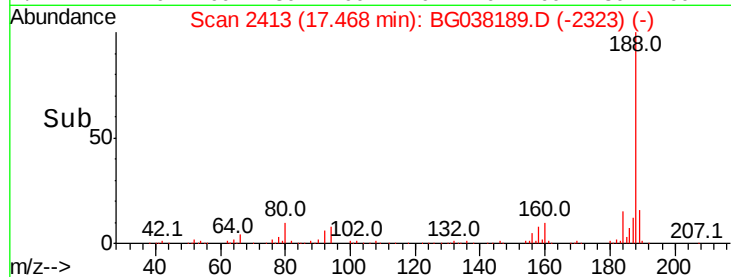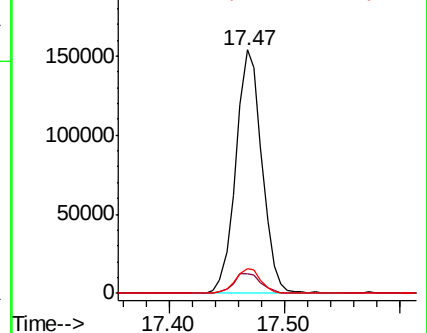

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.75 min Scan# 3142

Delta R.T. -0.00 min

Lab File: BG038189.D

Acq: 28 Nov 2018 6:48


Tgt Ion:240 Resp: 223745

Ion Ratio Lower Upper

240 100

120 10.7 8.1 12.1



236 26.0 21.4 32.0

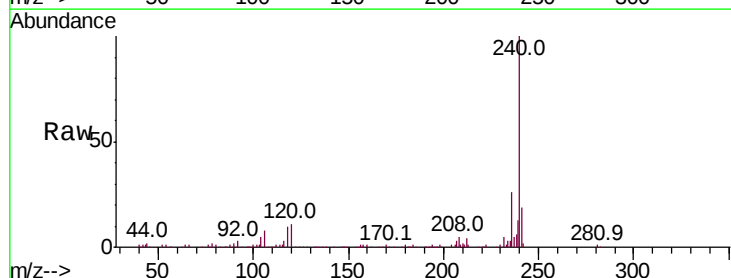

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

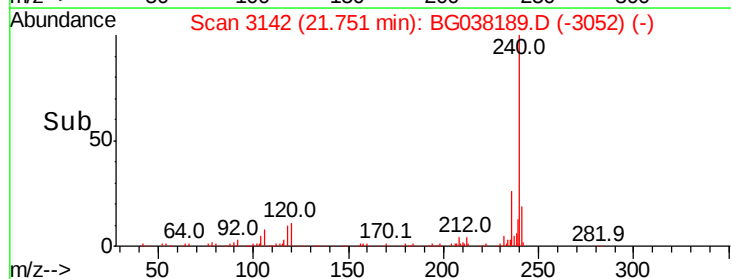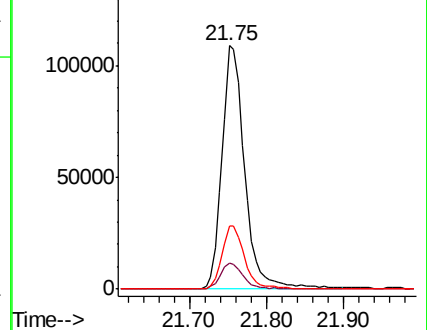



#79

Terphenyl-d14

Concen: 93.238 ng

RT: 20.07 min Scan# 2856

Delta R.T. 0.00 min

Lab File: BG038189.D

Acq: 28 Nov 2018 6:48

Instrument :


BNA_G

ClientSampleId :

COMP-3

Tot Ion:244 Resp: 886590


Ion	Ratio	Lower	Upper
244	100		
212	8.0	6.5	9.7
122	10.2	9.0	13.4

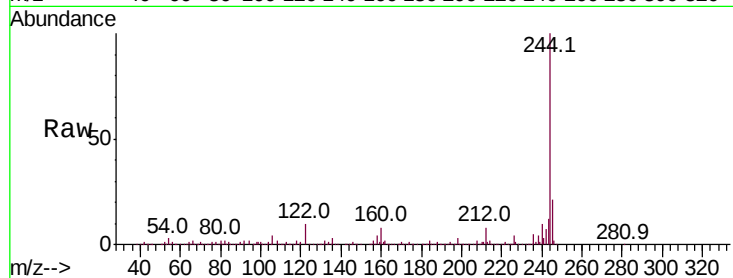



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

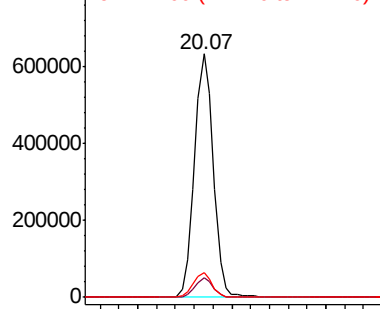

Time-->

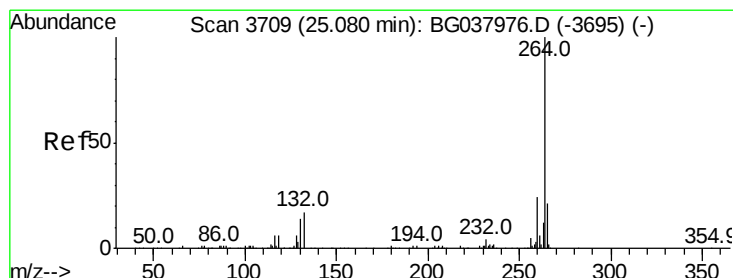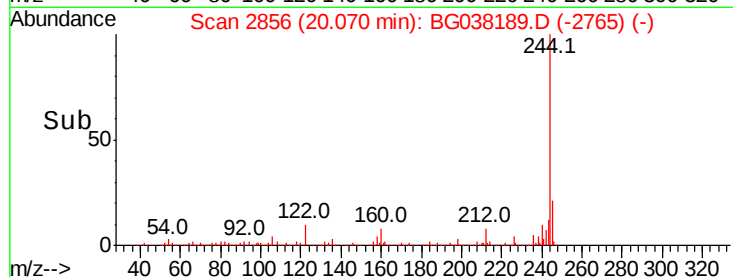

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.09 min Scan# 3711


Delta R.T. 0.01 min

Lab File: BG038189.D

Acq: 28 Nov 2018 6:48

Tgt Ion:264 Resp: 193485


Ion	Ratio	Lower	Upper
264	100		
260	21.7	18.2	27.4
265	19.3	17.9	26.9

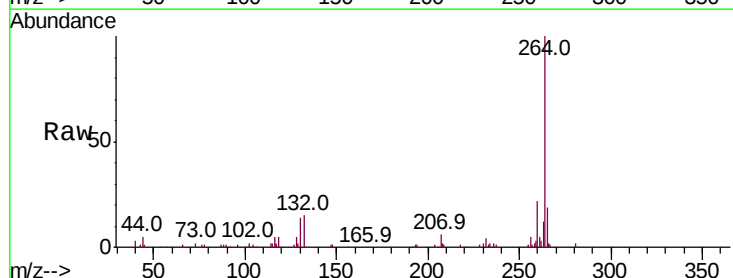

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

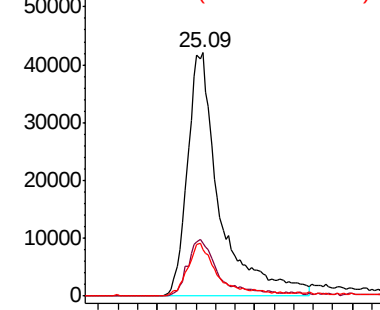

Time-->

