


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112718\
 Data File : BG038165.D
 Acq On : 27 Nov 2018 13:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

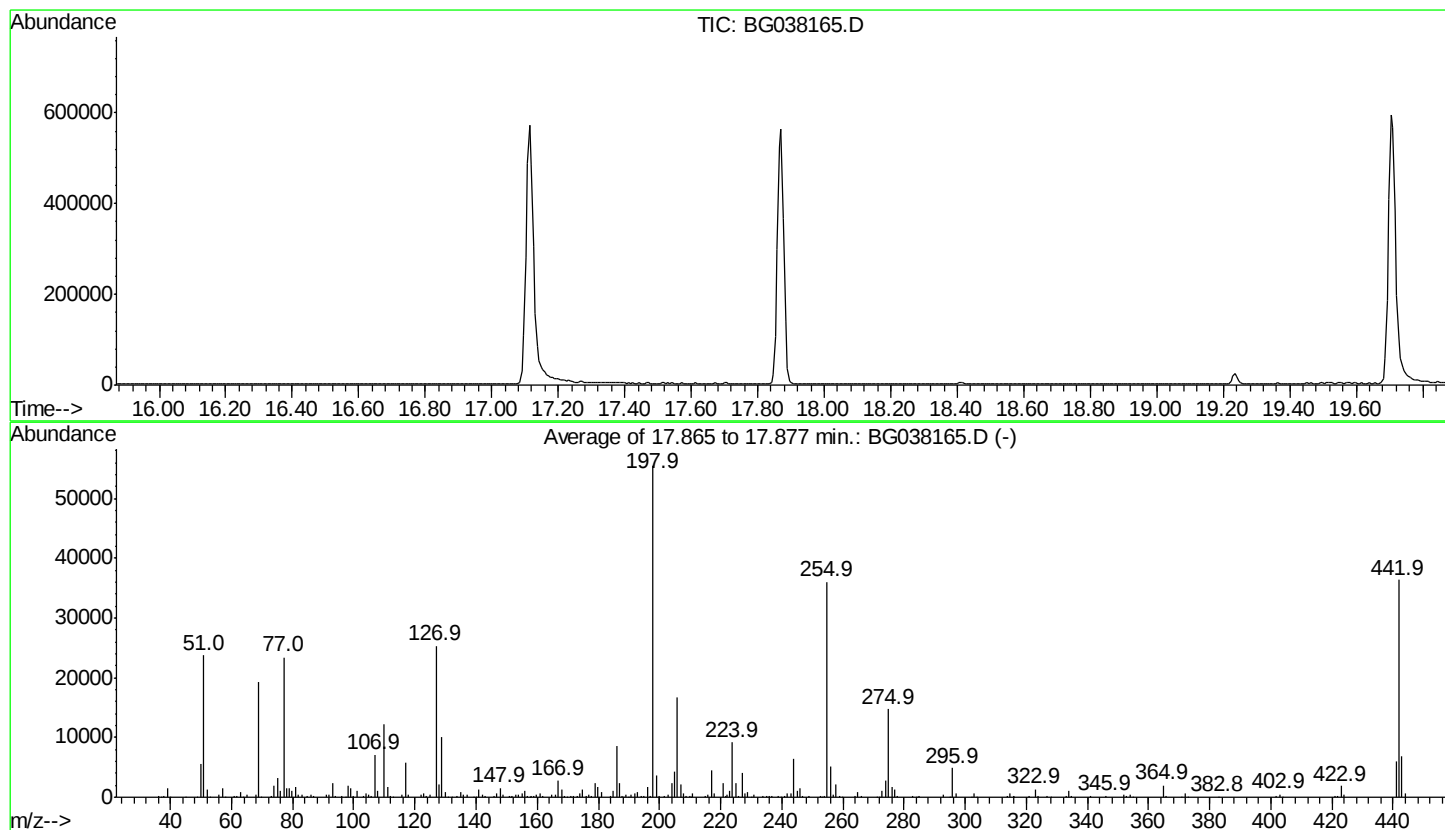

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	23732	PASS
68	69	0.00	2	1.9	366	PASS
69	198	0.00	100	34.8	19311	PASS
70	69	0.00	2	0.6	112	PASS
127	198	10	80	45.6	25282	PASS
197	198	0.00	2	0.4	230	PASS
198	198	100	100	100.0	55490	PASS
199	198	5	9	6.7	3734	PASS
275	198	10	60	26.5	14728	PASS
365	198	1	100	3.5	1950	PASS
441	198	0.01	100	10.9	6030	PASS
442	198	50	100	65.6	36397	PASS
443	442	15	24	18.8	6827	PASS