


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112718\
 Data File : BG038184.D
 Acq On : 28 Nov 2018 3:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

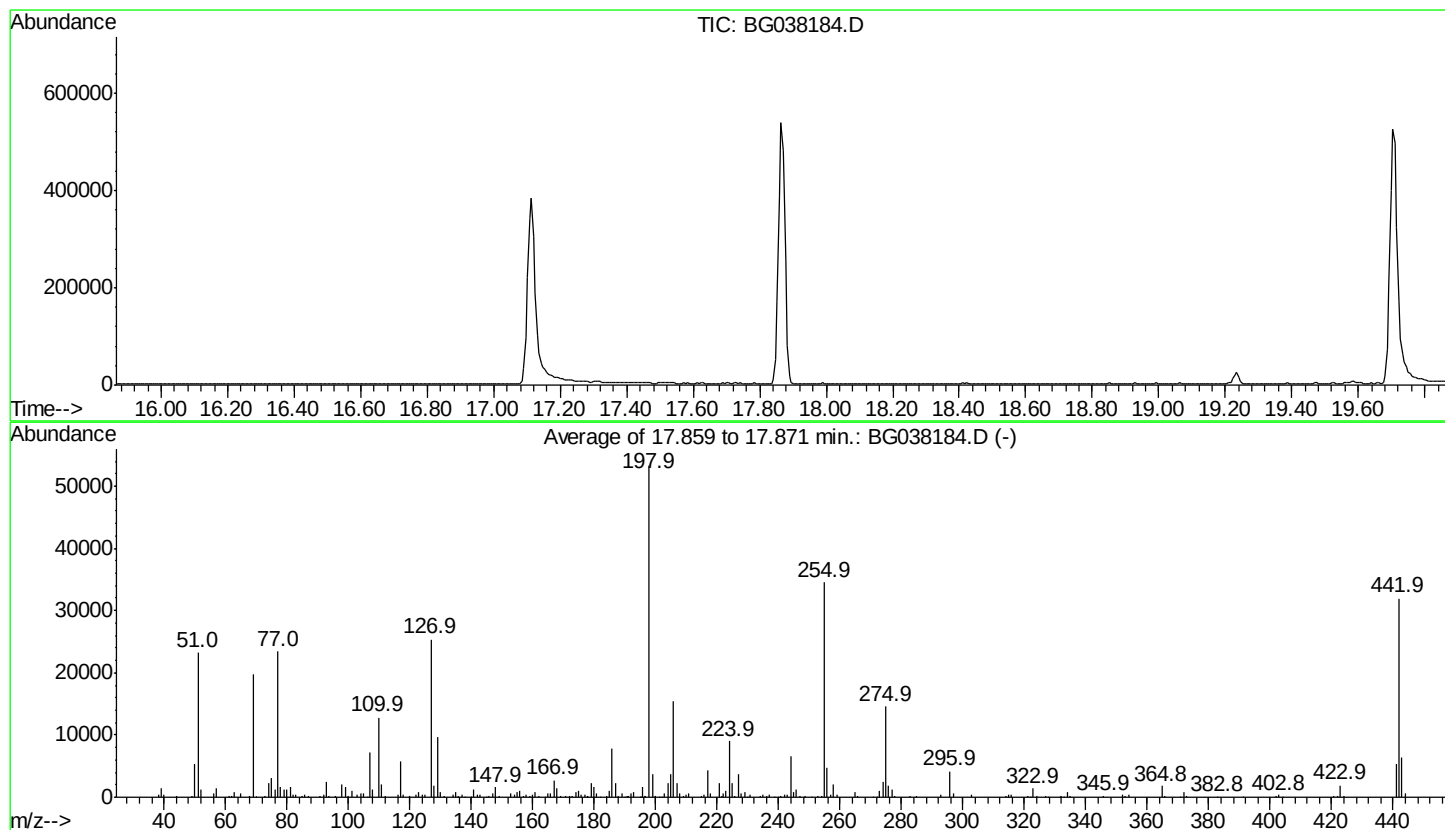

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	23197	PASS
68	69	0.00	2	1.4	271	PASS
69	198	0.00	100	36.9	19656	PASS
70	69	0.00	2	0.3	64	PASS
127	198	10	80	47.5	25325	PASS
197	198	0.00	2	0.4	212	PASS
198	198	100	100	100.0	53298	PASS
199	198	5	9	7.0	3752	PASS
275	198	10	60	27.2	14518	PASS
365	198	1	100	3.3	1768	PASS
441	198	0.01	100	10.0	5345	PASS
442	198	50	100	59.9	31904	PASS
443	442	15	24	19.9	6351	PASS