
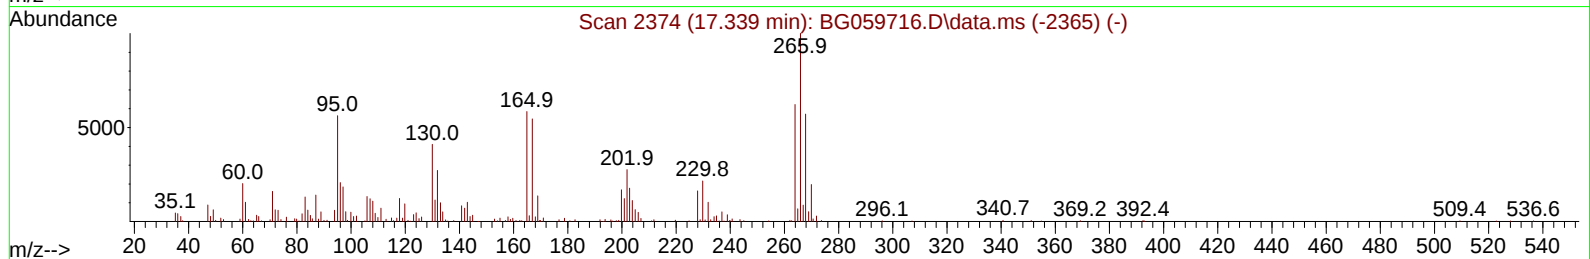
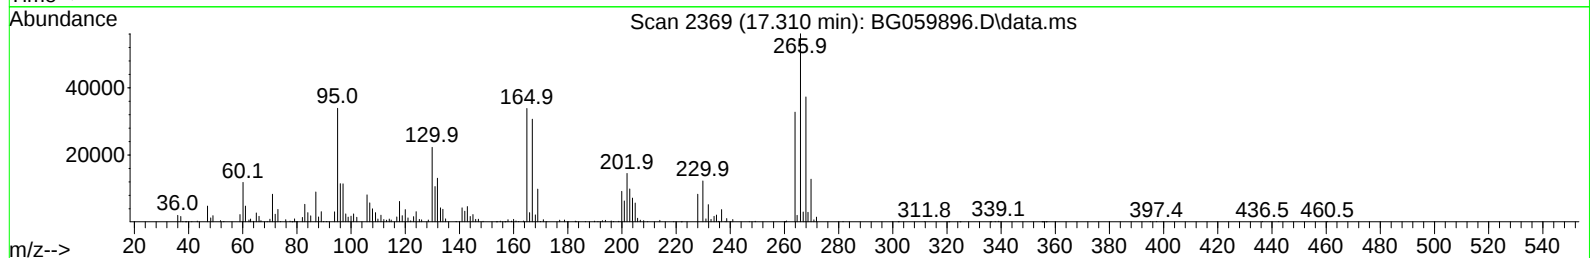


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112723\
Data File : BG059896.D
Acq On : 27 Nov 2023 10:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 12:41:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:11:07 2023
Response via : Initial Calibration

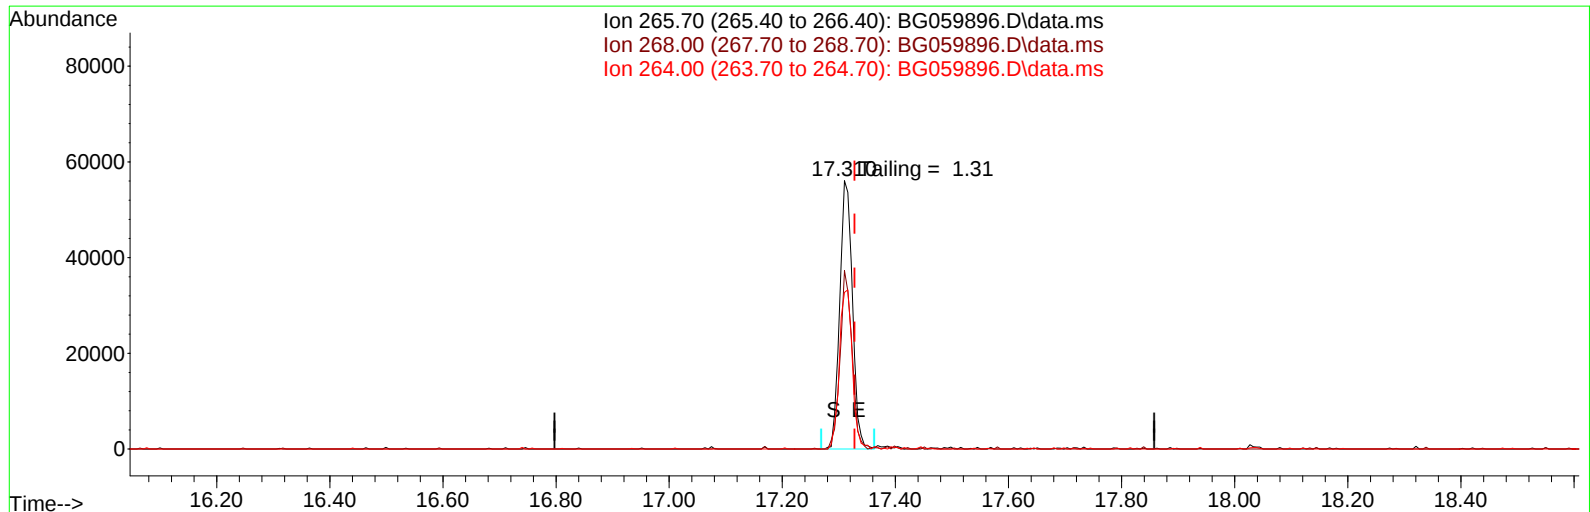

TIC: BG059896.D\data.ms

(70) Pentachlorophenol (C)




17.310min (-0.018) 83390.17 ng

response 87393

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	71.72#
264.00	62.30	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112723\
Data File : BG059896.D
Acq On : 27 Nov 2023 10:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 12:41:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:11:07 2023
Response via : Initial Calibration

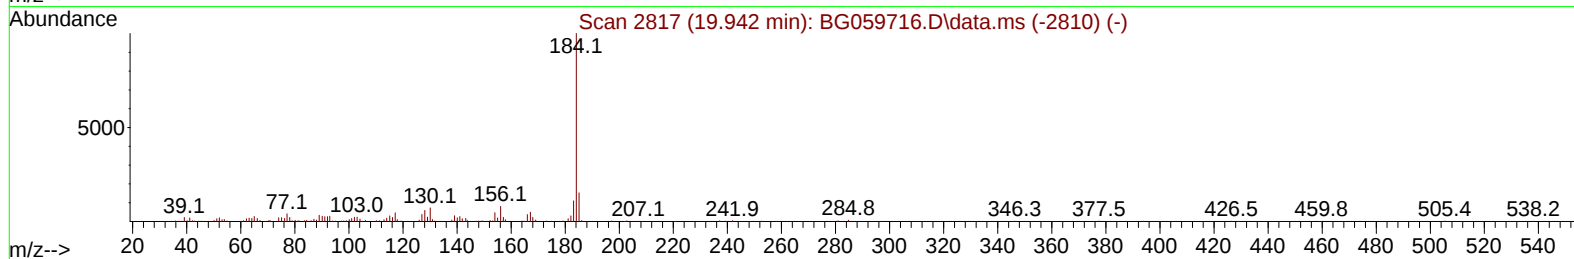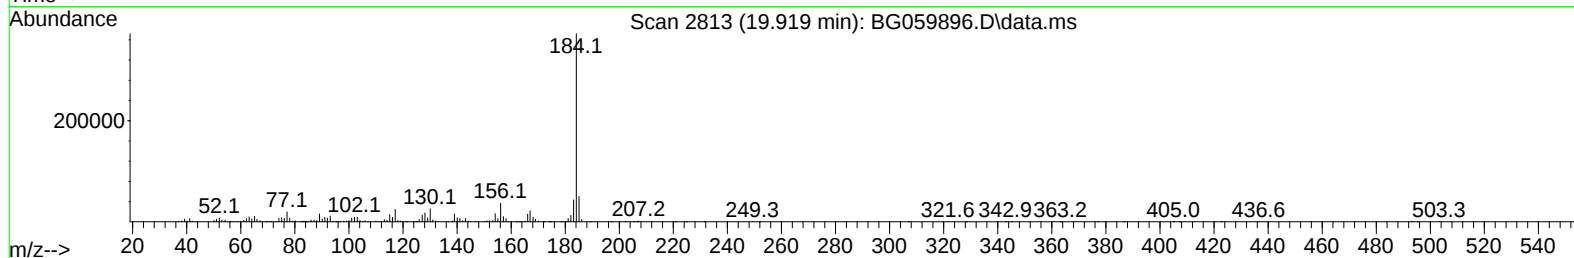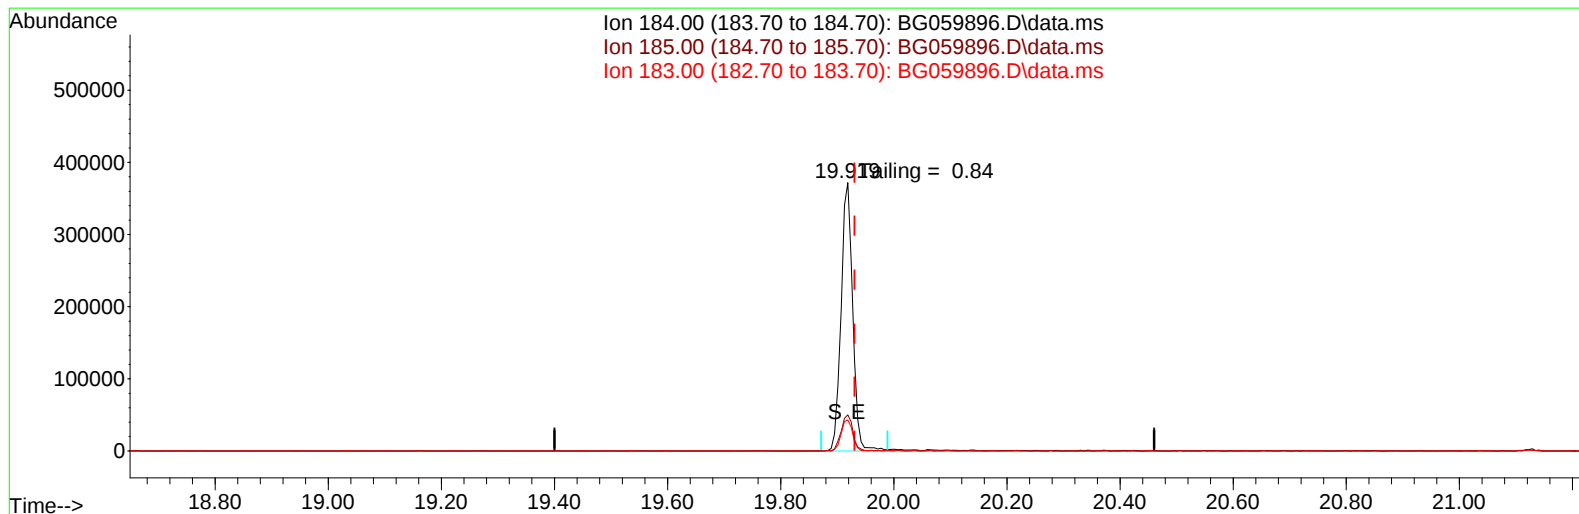

TIC: BG059896.D\data.ms

(77) Benzidine**19.919min (-0.012) 186778.16 ng****response 529417**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.50
183.00	11.00	11.58
0.00	0.00	0.00