


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112723\
Data File : BG059896.D
Acq On : 27 Nov 2023 10:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 27 13:17:45 2023

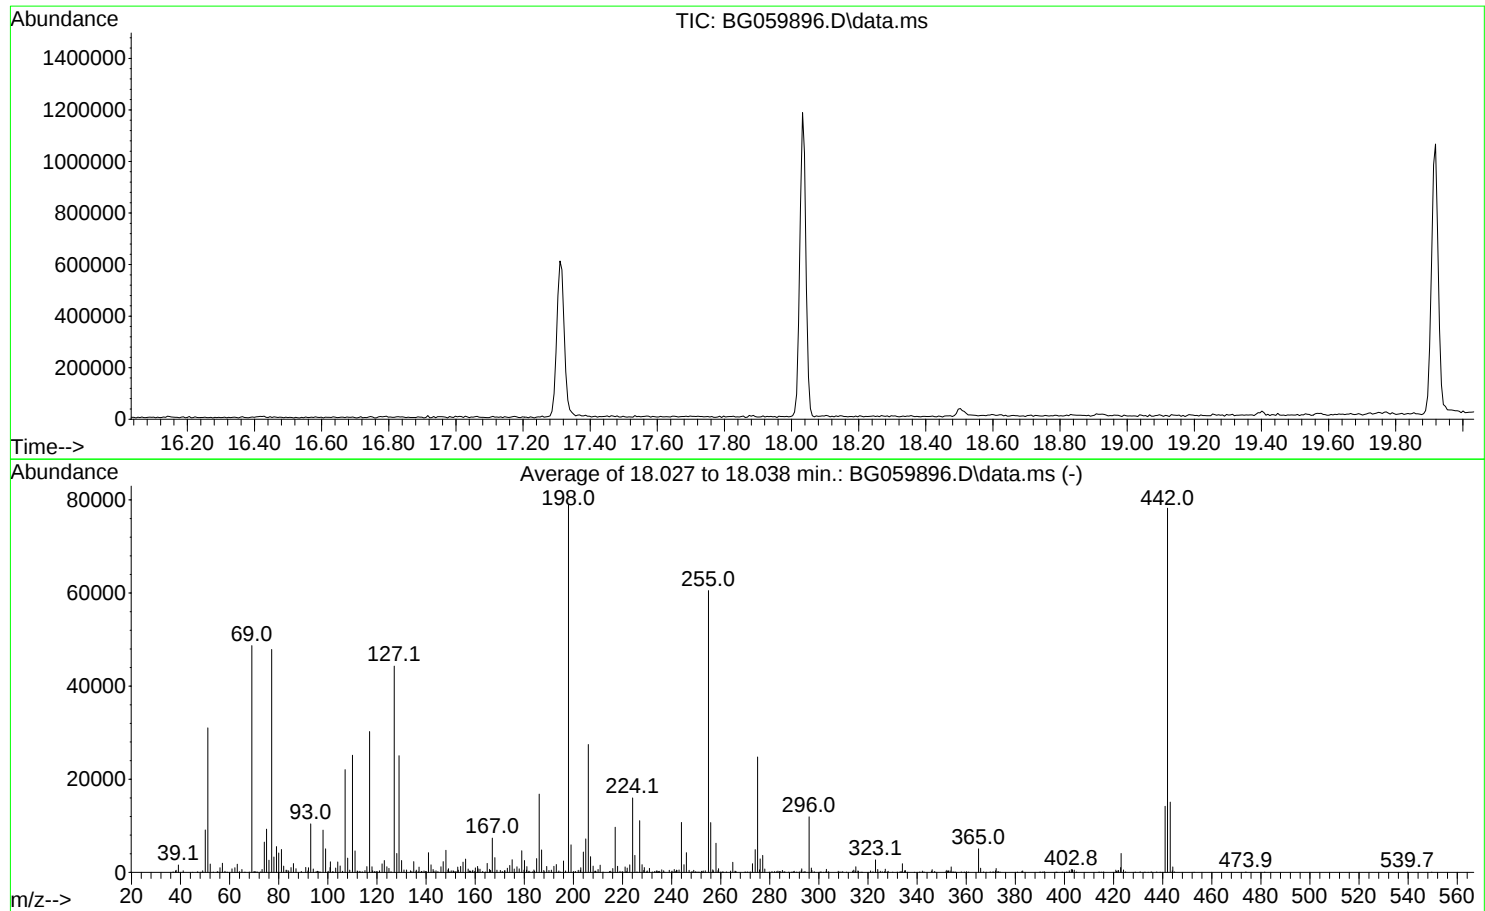




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	31035	PASS
68	69	0.00	2	0.1	72	PASS
69	198	0.00	100	61.6	48691	PASS
70	69	0.00	2	0.3	147	PASS
127	198	10	80	56.1	44315	PASS
197	198	0.00	2	0.4	304	PASS
198	198	100	100	100.0	79021	PASS
199	198	5	9	7.5	5920	PASS
275	198	10	60	31.4	24792	PASS
365	198	1	100	6.4	5045	PASS
441	198	0.01	100	18.0	14191	PASS
442	442	50	100	100.0	78216	PASS
443	442	15	24	19.3	15106	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112723\
Data File : BG059896.D
Acq On : 27 Nov 2023 10:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 27 12:41:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:11:07 2023
Response via : Initial Calibration

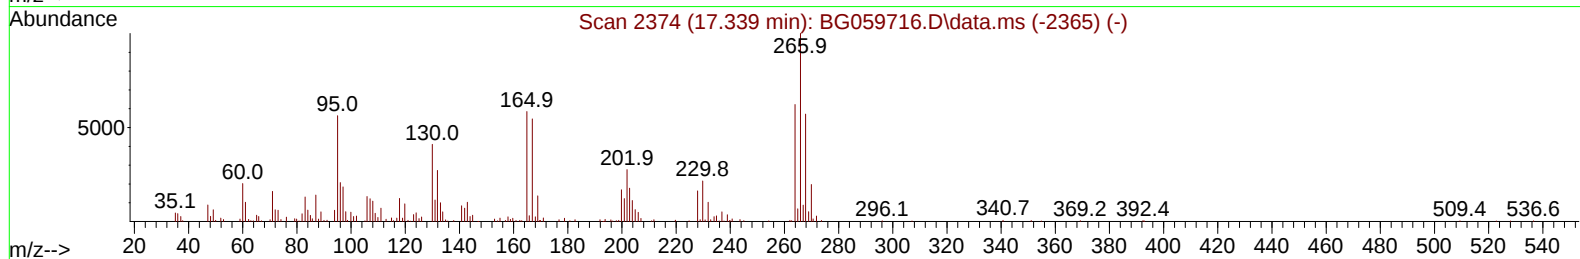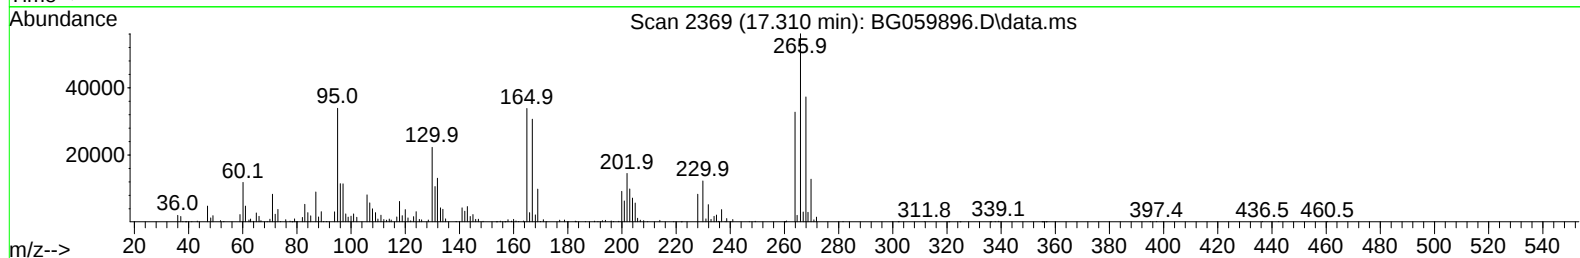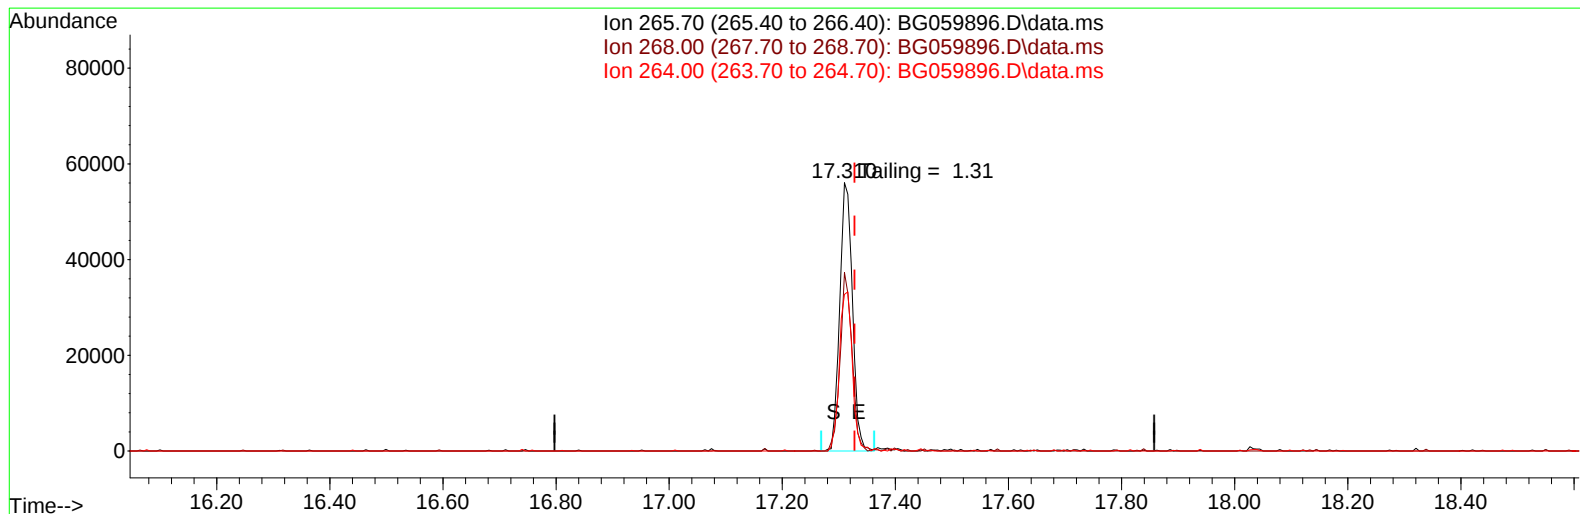

TIC: BG059896.D\data.ms

(70) Pentachlorophenol (C)

17.310min (-0.018) 83390.17 ng




response 87393

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	71.72#
264.00	62.30	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112723\
Data File : BG059896.D
Acq On : 27 Nov 2023 10:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 27 12:41:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:11:07 2023
Response via : Initial Calibration

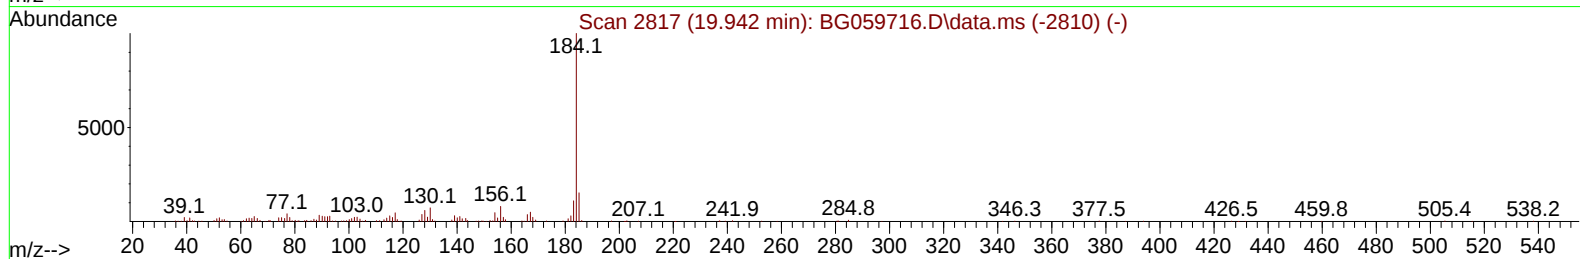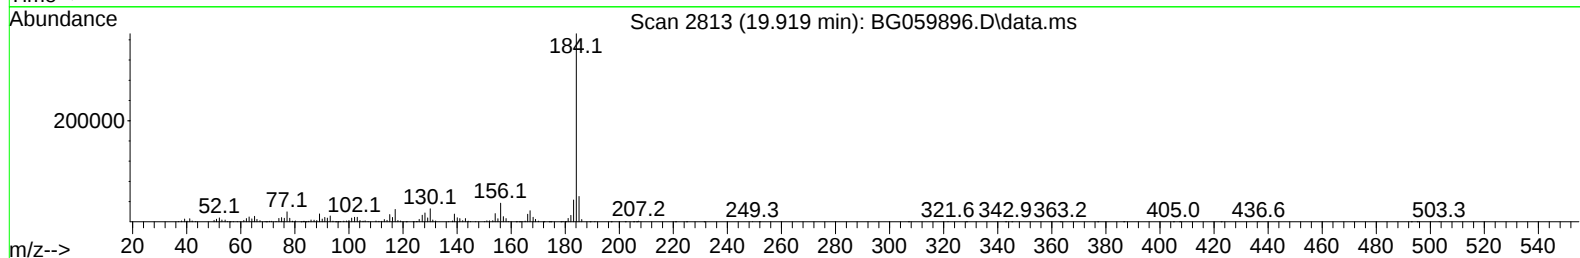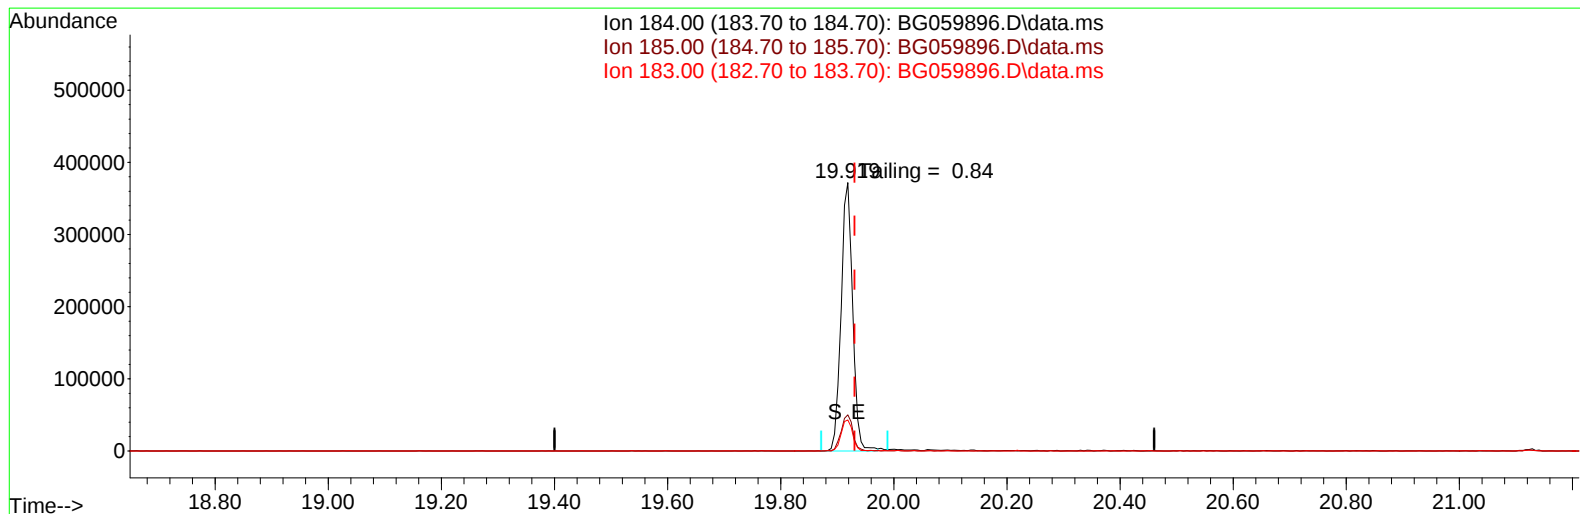

TIC: BG059896.D\data.ms

(77) Benzidine

19.919min (-0.012) 186778.16 ng

response 529417

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.50
183.00	11.00	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/27/2023	BNA_G	<u>BG059896.D</u>
Compound Name	Response	Retention Time
DDT	258172	21.123
DDD	p	20.665
DDE	0	19.901
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
#VALUE!	#VALUE!	#VALUE!

Instrument :
BNA_G
ClientSampleId :
DFTPP