
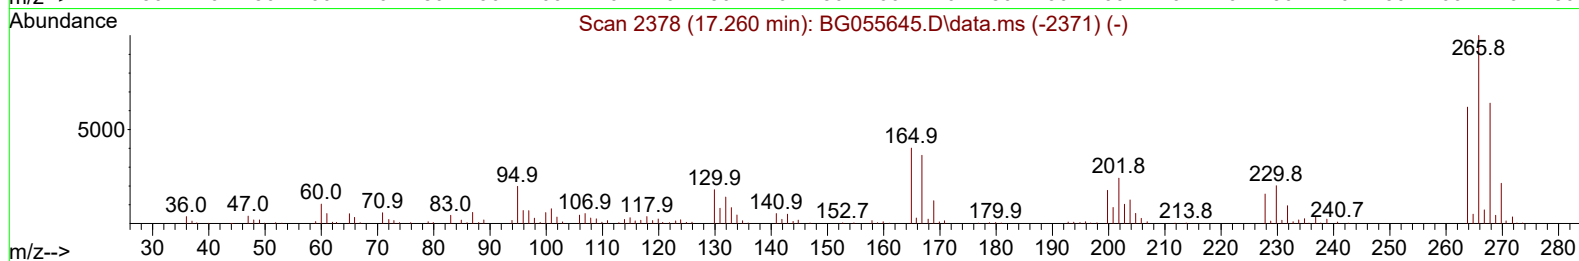
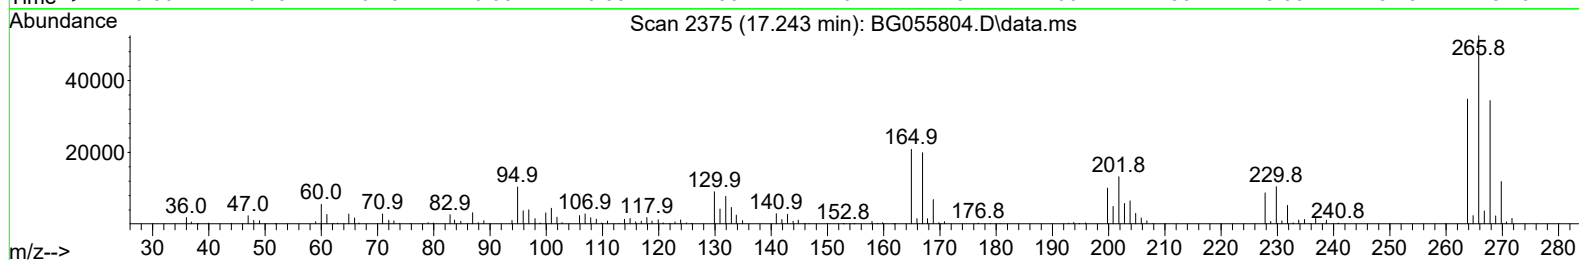


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112822\
Data File : BG055804.D
Acq On : 28 Nov 2022 14:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 07:18:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 02:02:15 2022
Response via : Initial Calibration

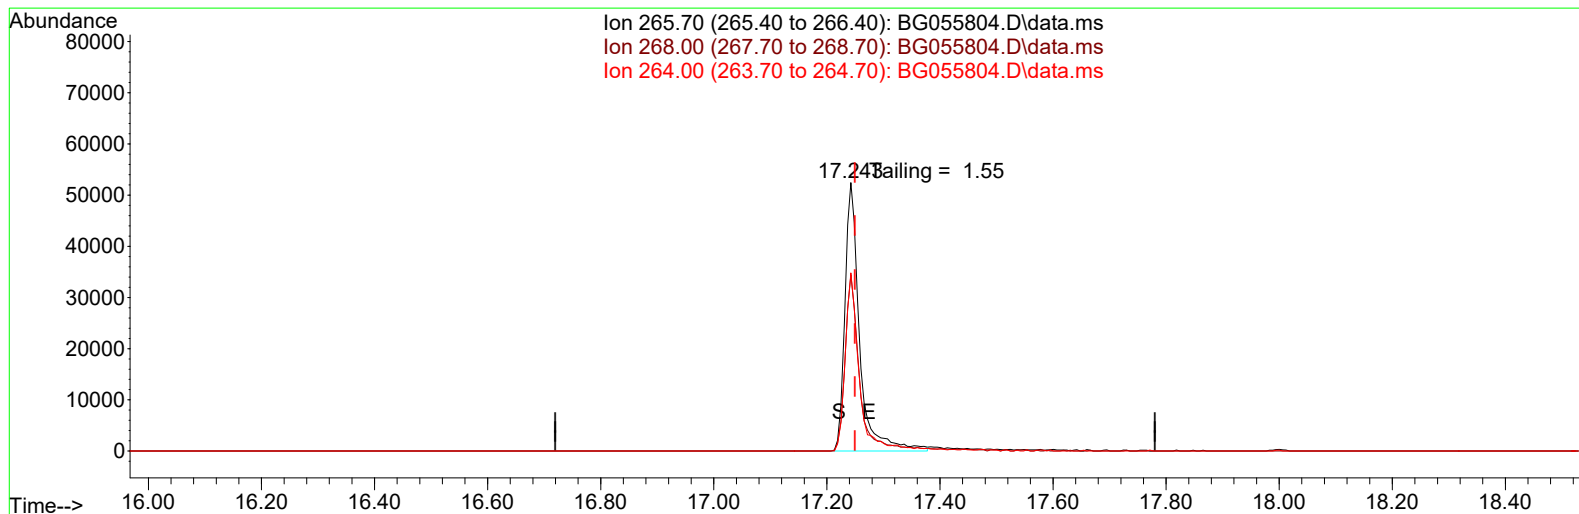

TIC: BG055804.D\data.ms

(70) Pentachlorophenol (C)




17.243min (-0.008) 28608.44 ng

response 93526

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.62
264.00	61.90	66.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112822\
Data File : BG055804.D
Acq On : 28 Nov 2022 14:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 07:18:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 02:02:15 2022
Response via : Initial Calibration

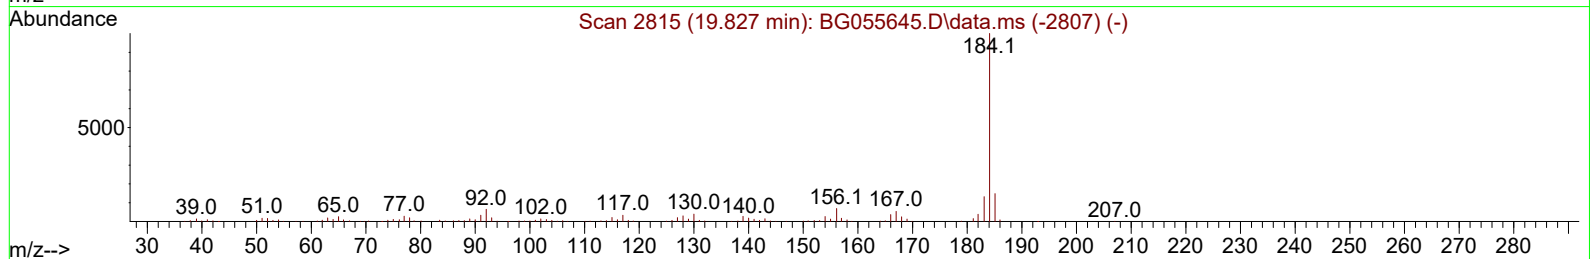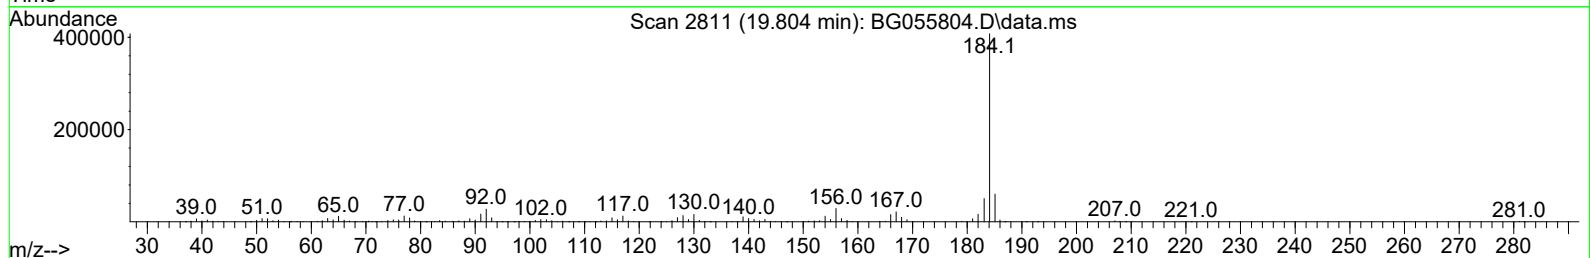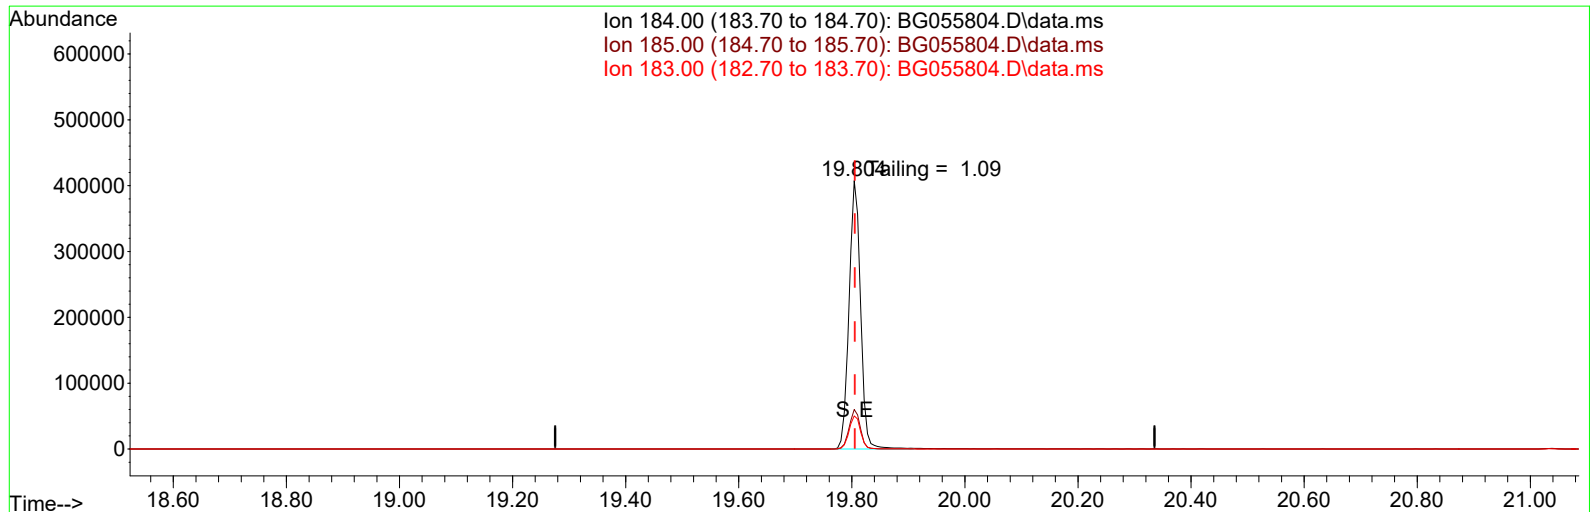

TIC: BG055804.D\data.ms

(77) Benzidine

19.804min (-0.002) 0.00 ng

response 578303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.76
183.00	13.20	12.35
0.00	0.00	0.00