
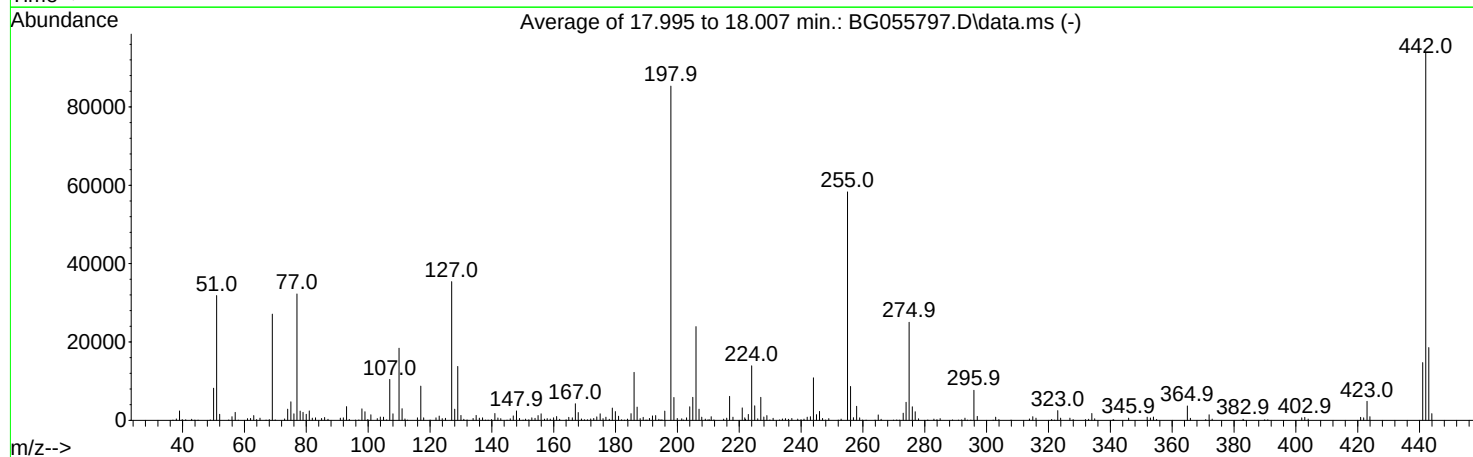


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112822\
 Data File : BG055797.D
 Acq On : 28 Nov 2022 9:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 02:02:15 2022

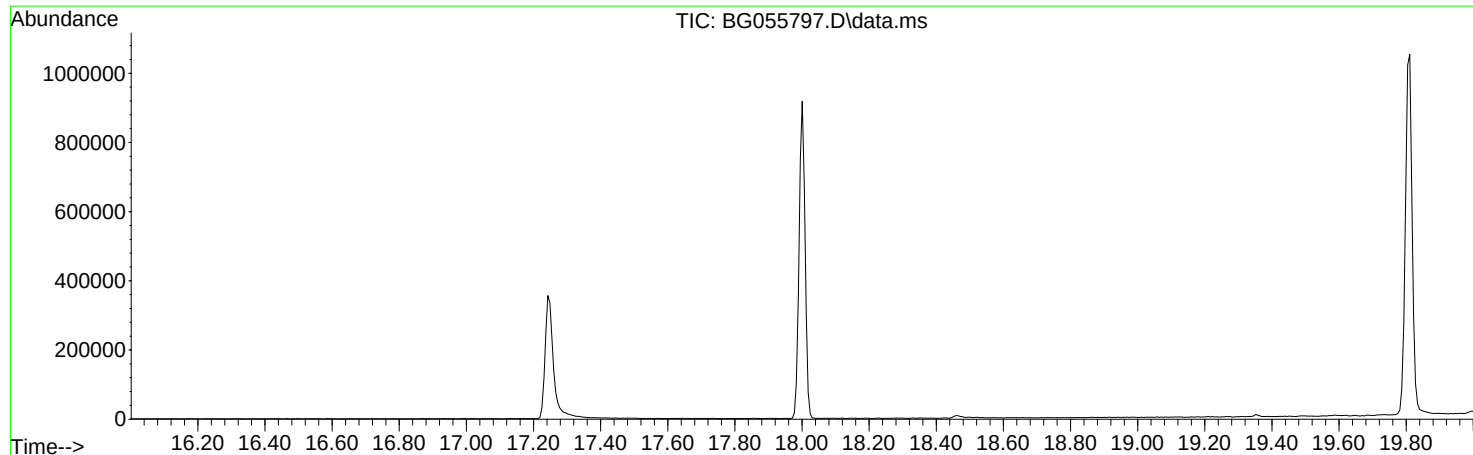




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	31835	PASS
68	69	0.00	2	0.6	175	PASS
69	198	0.00	100	31.8	27125	PASS
70	69	0.00	2	0.4	121	PASS
127	198	10	80	41.5	35387	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85317	PASS
199	198	5	9	6.8	5823	PASS
275	198	10	60	29.3	25019	PASS
365	198	1	100	4.3	3648	PASS
441	198	0.01	100	17.3	14745	PASS
442	442	50	100	100.0	93920	PASS
443	442	15	24	19.8	18578	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112822\
Data File : BG055797.D
Acq On : 28 Nov 2022 9:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 29 07:16:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 02:02:15 2022
Response via : Initial Calibration

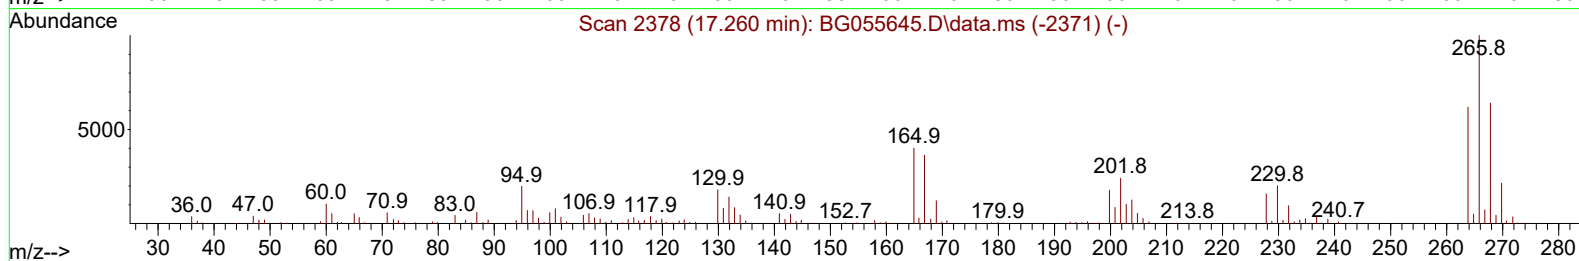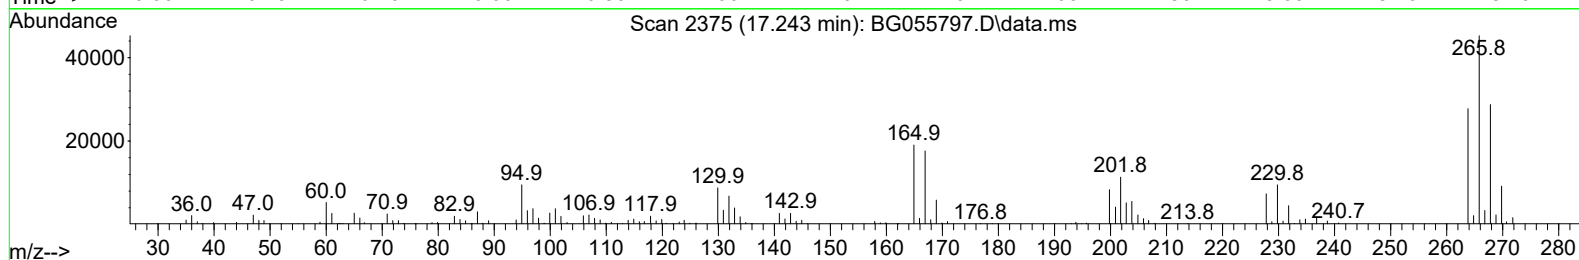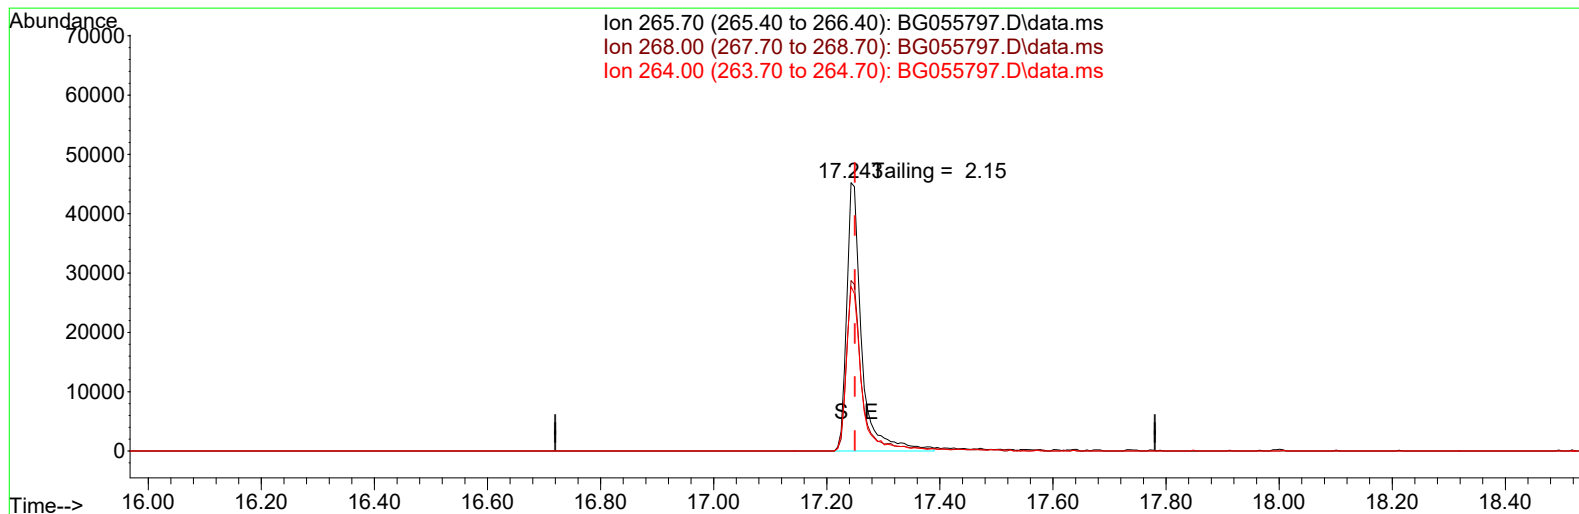

TIC: BG055797.D\data.ms

(70) Pentachlorophenol (C)

17.243min (-0.007) 17591.79 ng




response 82799

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.51
264.00	61.90	61.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112822\
Data File : BG055797.D
Acq On : 28 Nov 2022 9:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 29 07:16:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 02:02:15 2022
Response via : Initial Calibration

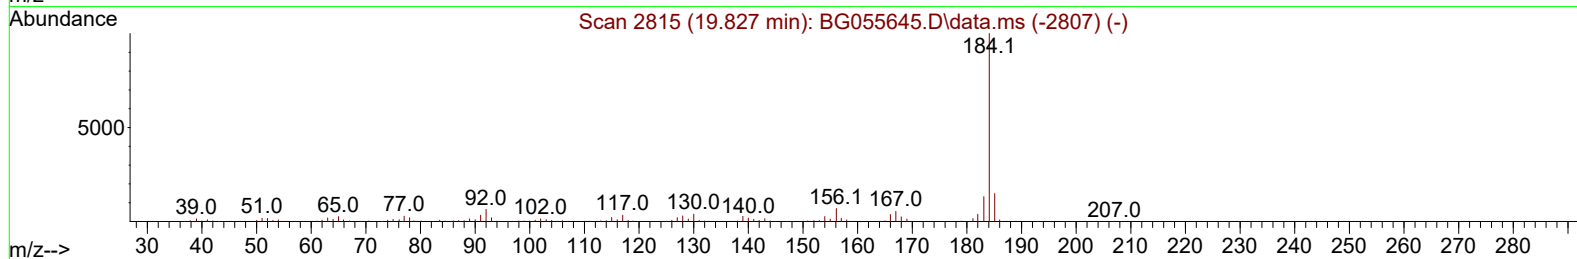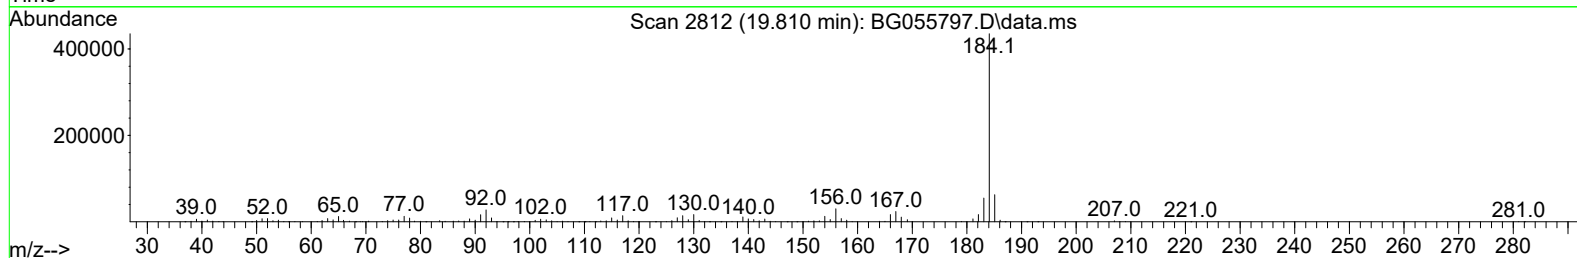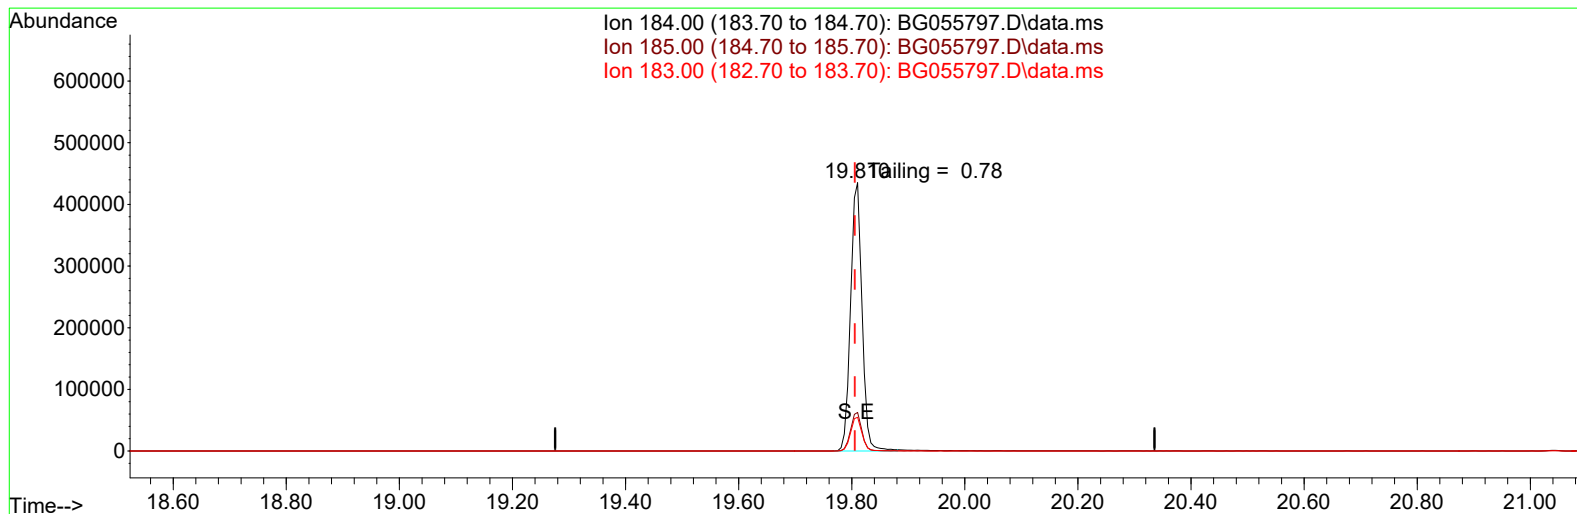

TIC: BG055797.D\data.ms

(77) Benzidine

19.810min (+ 0.005) 0.00 ng

response 620628

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.38
183.00	13.20	12.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/28/2022	BNA_G	BG055797.D
Compound Name	Response	Retention Time
DDT	292542	21.038
DDD	5024	20.645
DDE	54	20.092
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5078	297620	1.71

Instrument :
BNA_G
ClientSampleId :
DFTPP