


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112822\
Data File : BG055804.D
Acq On : 28 Nov 2022 14:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 29 02:02:15 2022

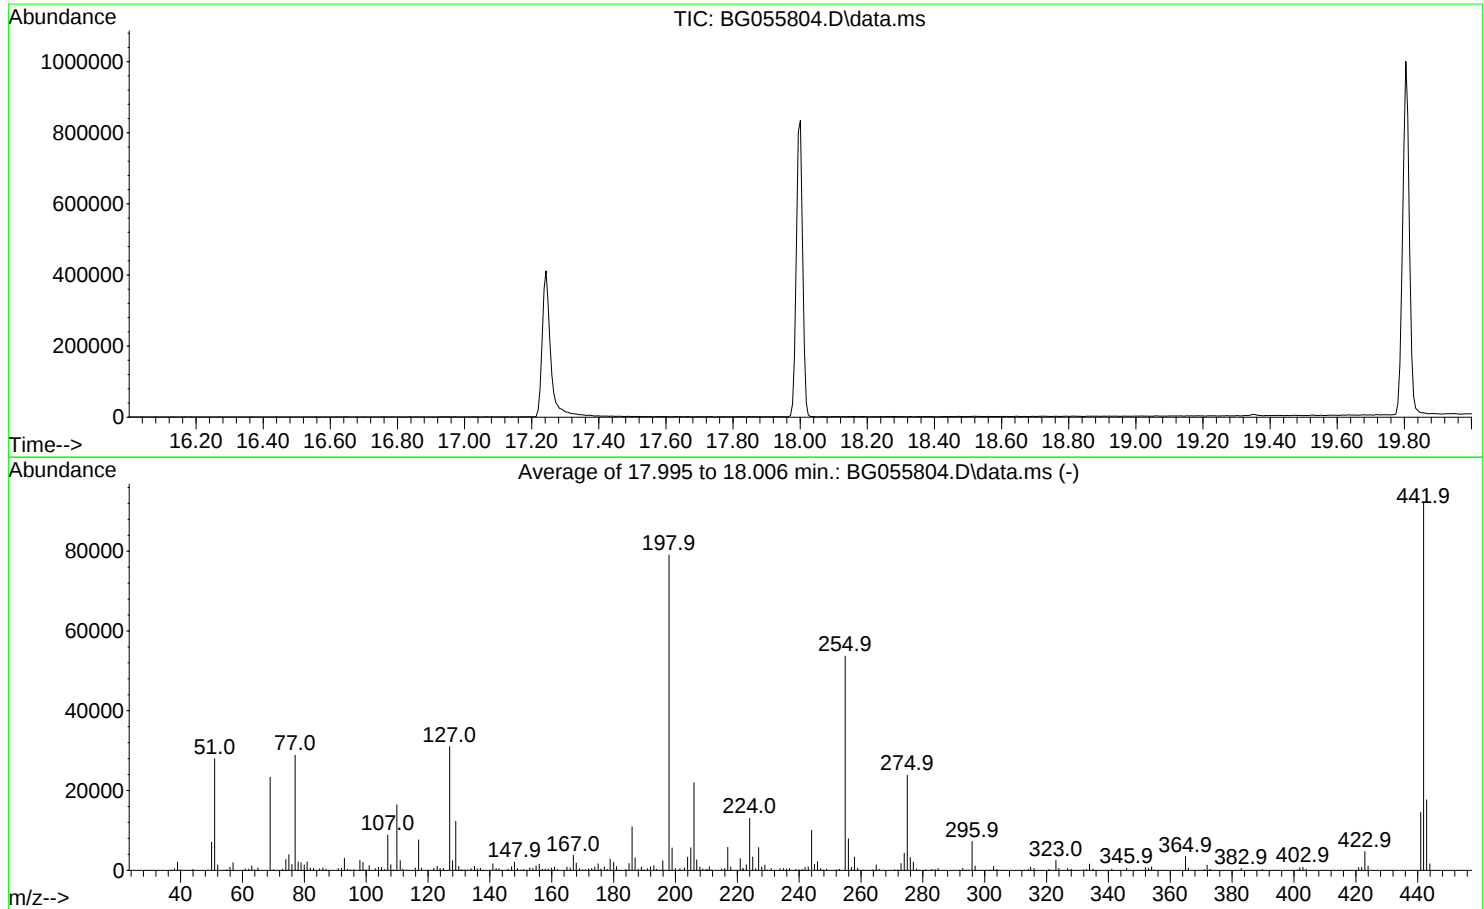




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	27996	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.5	23328	PASS
70	69	0.00	2	0.6	142	PASS
127	198	10	80	39.3	31043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79069	PASS
199	198	5	9	7.1	5590	PASS
275	198	10	60	30.2	23861	PASS
365	198	1	100	4.4	3491	PASS
441	198	0.01	100	18.3	14497	PASS
442	442	50	100	100.0	92235	PASS
443	442	15	24	19.2	17672	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112822\
Data File : BG055804.D
Acq On : 28 Nov 2022 14:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 29 07:18:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 02:02:15 2022
Response via : Initial Calibration

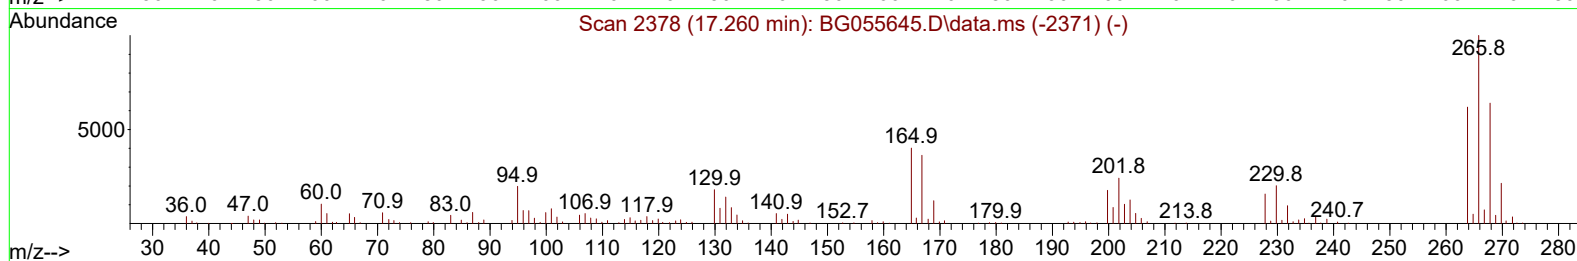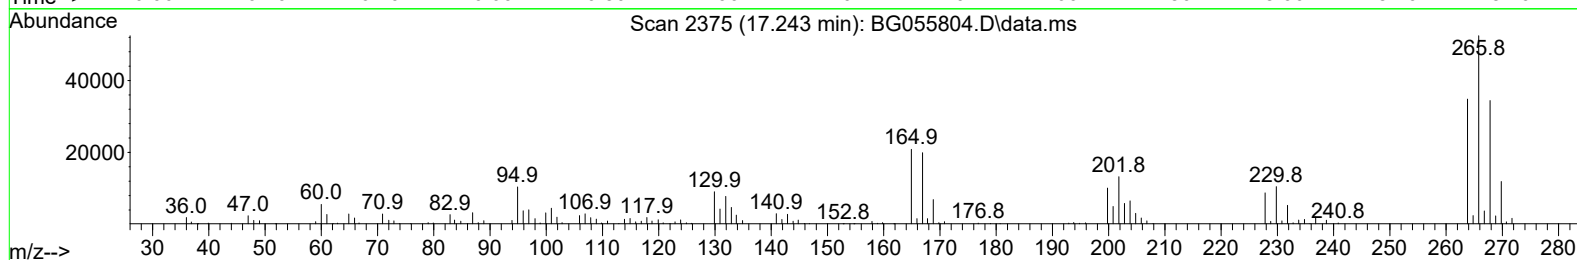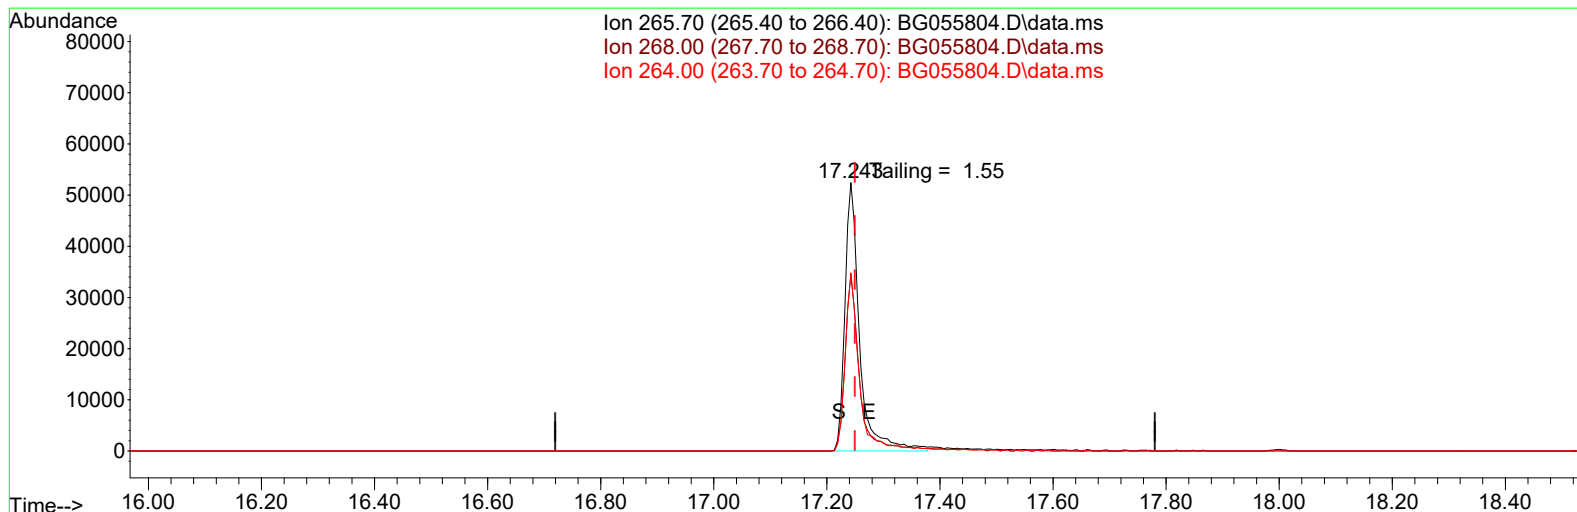

TIC: BG055804.D\data.ms

(70) Pentachlorophenol (C)

17.243min (-0.008) 28608.44 ng




response 93526

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.62
264.00	61.90	66.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112822\
Data File : BG055804.D
Acq On : 28 Nov 2022 14:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 29 07:18:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 02:02:15 2022
Response via : Initial Calibration

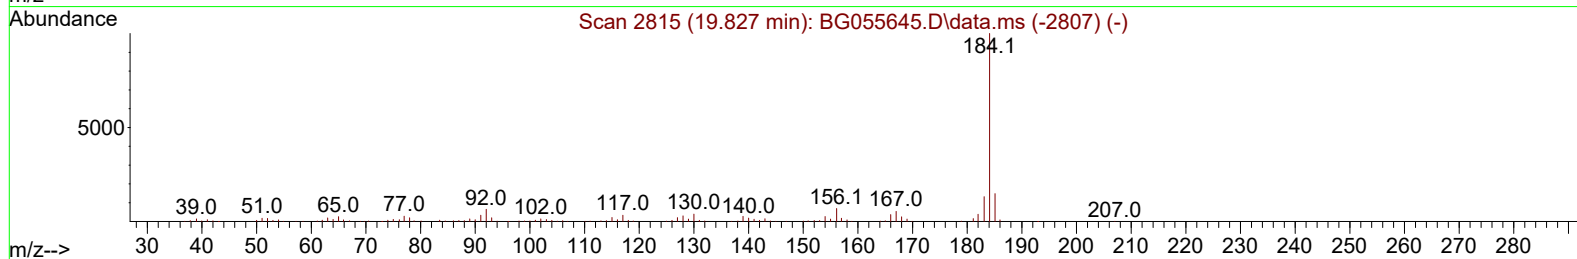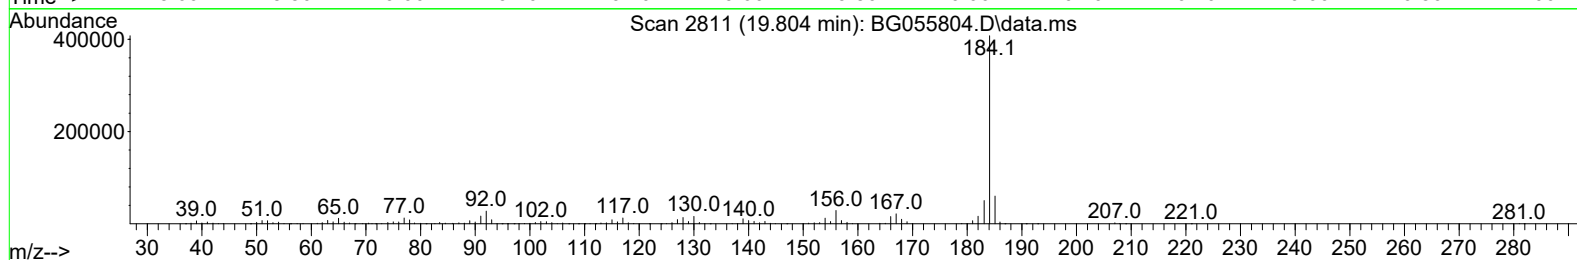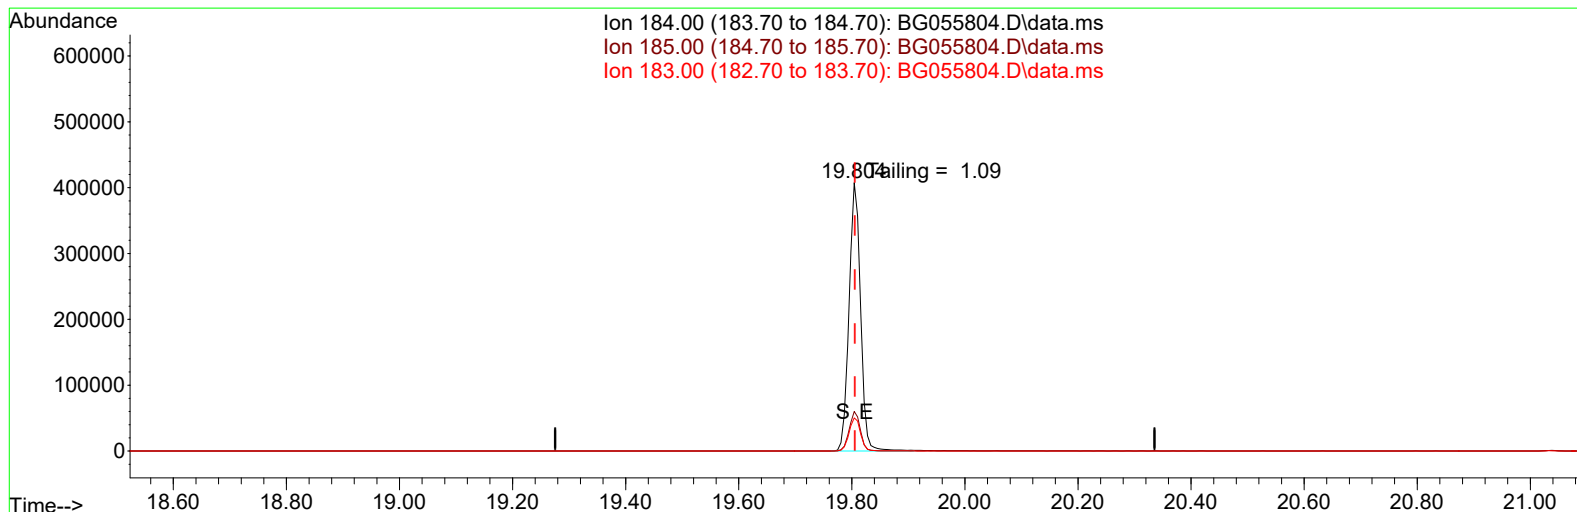

TIC: BG055804.D\data.ms

(77) Benzidine

19.804min (-0.002) 0.00 ng

response 578303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.76
183.00	13.20	12.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/28/2022	BNA_G	BG055804.D
Compound Name	Response	Retention Time
DDT	285696	21.038
DDD	6421	20.586
DDE	518	20.086
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6939	292635	2.37

Instrument :
BNA_G
ClientSampleId :
DFTPP