
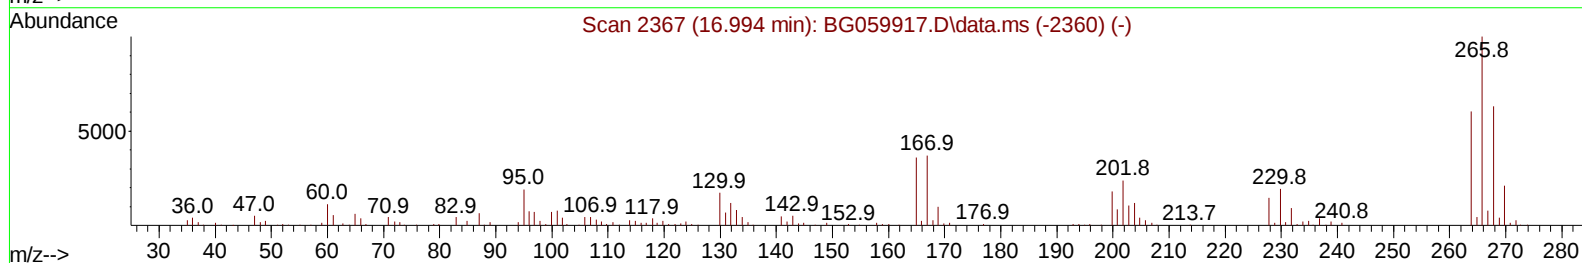
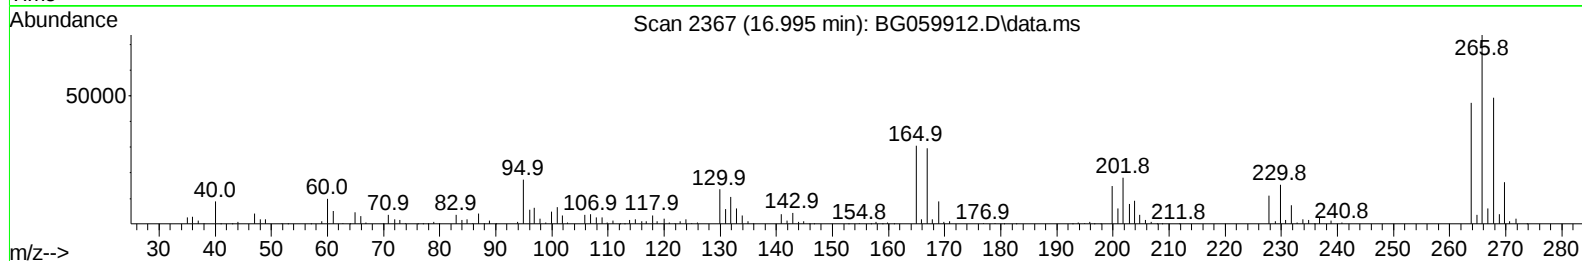


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113023\
Data File : BG059912.D
Acq On : 30 Nov 2023 16:23
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 03:57:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG113023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 03:37:46 2023
Response via : Initial Calibration

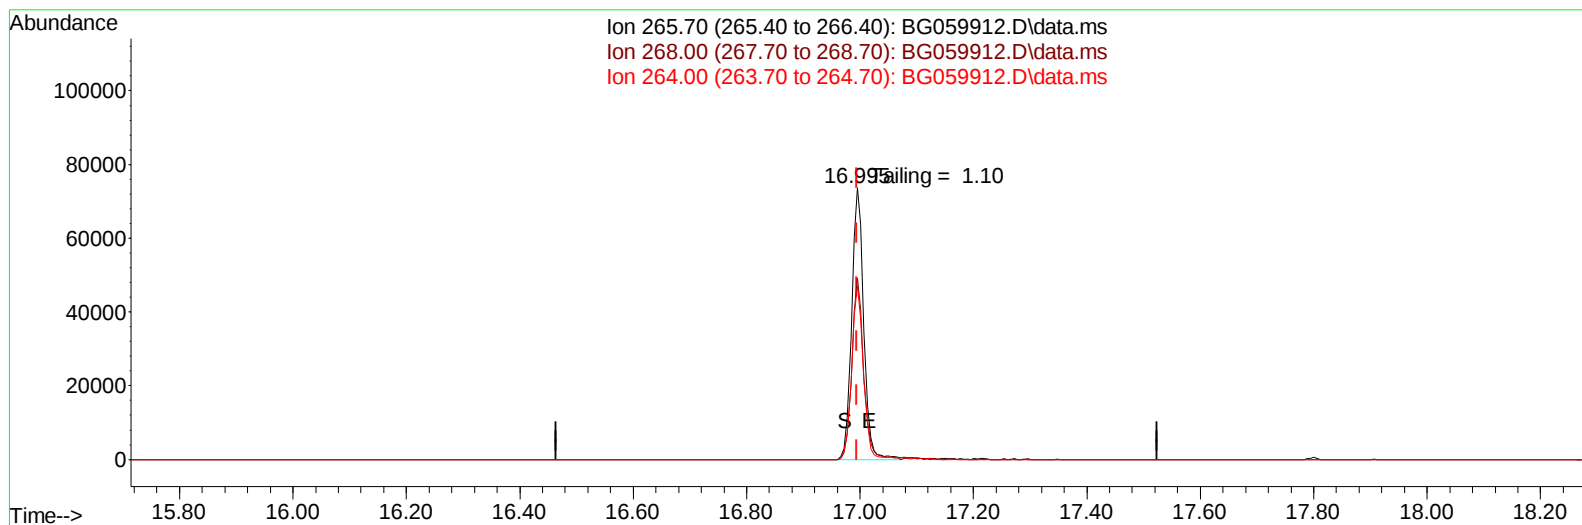

TIC: BG059912.D\data.ms

(70) Pentachlorophenol (C)




16.995min (+ 0.001) 120072.13 ng

response 109048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	66.74
264.00	60.30	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113023\
Data File : BG059912.D
Acq On : 30 Nov 2023 16:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 03:57:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG113023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 03:37:46 2023
Response via : Initial Calibration

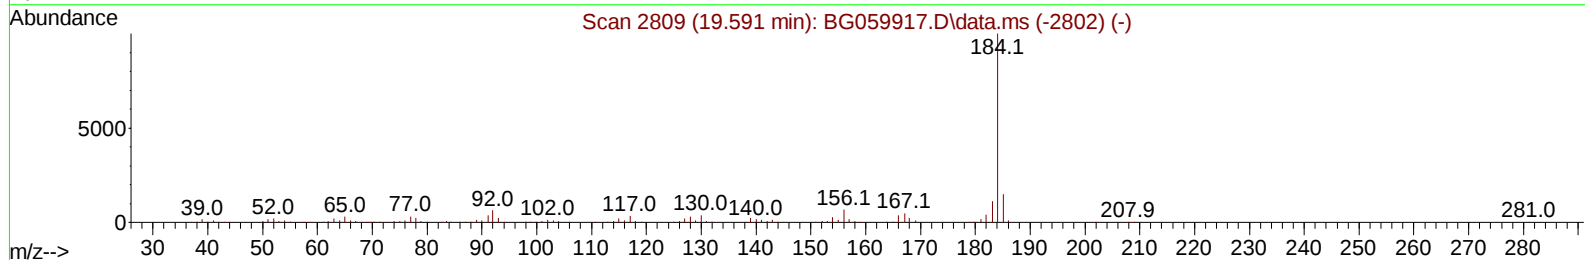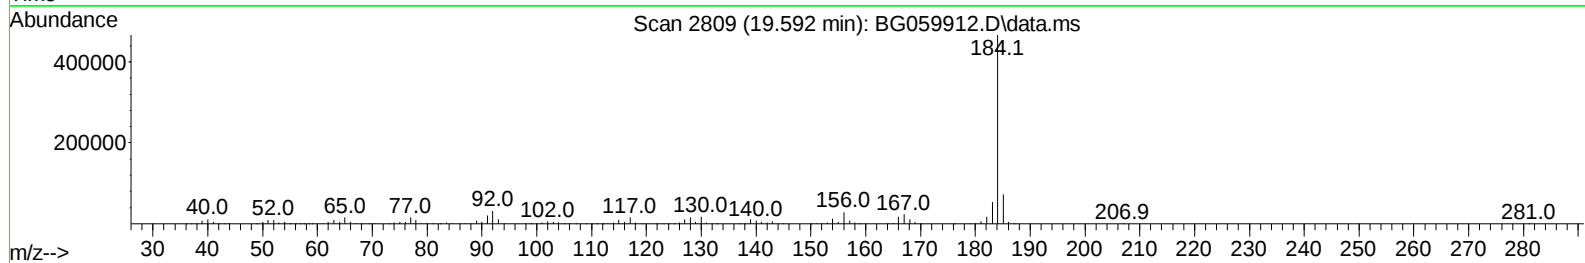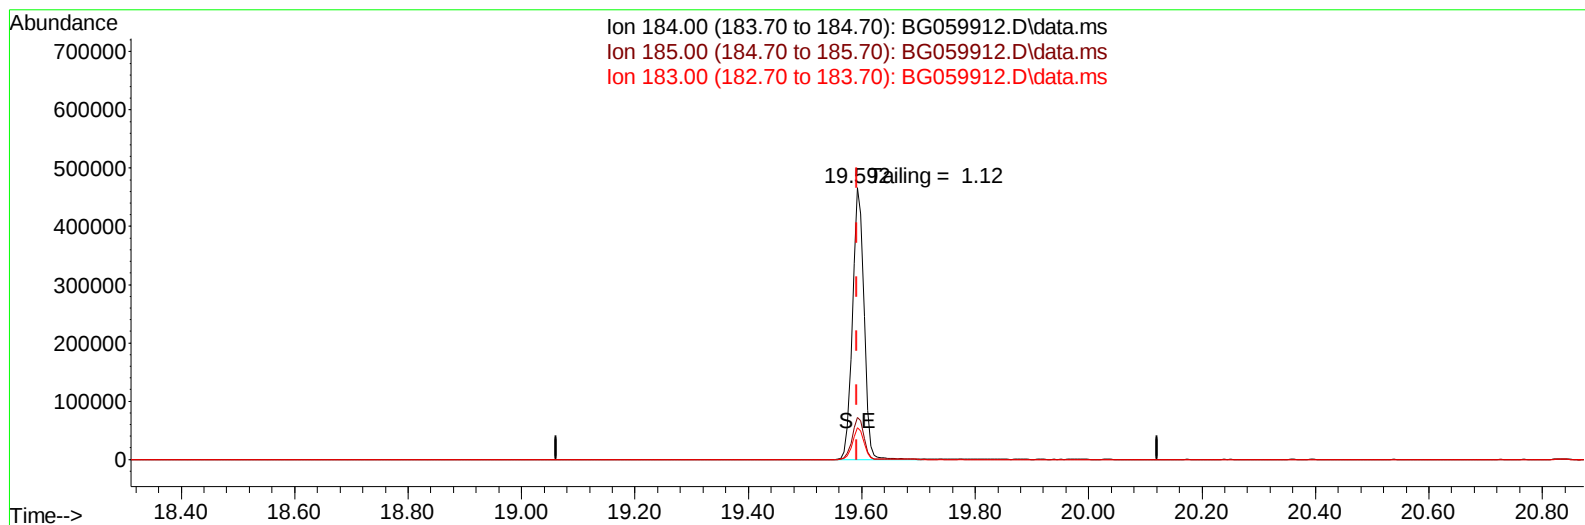

TIC: BG059912.D\data.ms

(77) Benzidine**19.592min (+ 0.001) 14932.09 ng****response 651012**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.51
183.00	11.20	11.64
0.00	0.00	0.00