
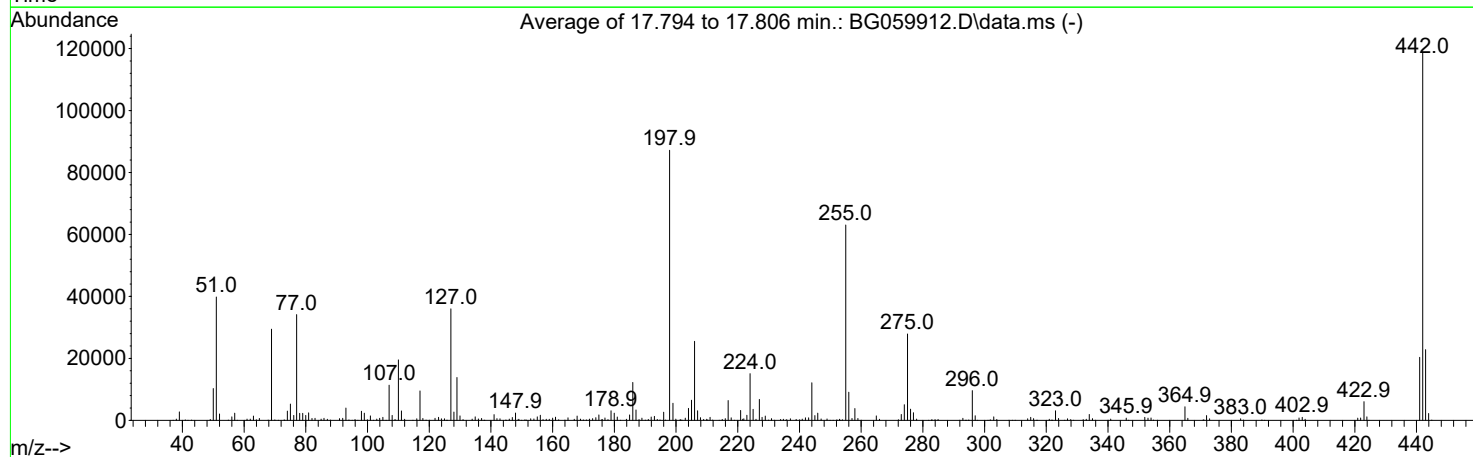


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113023\
 Data File : BG059912.D
 Acq On : 30 Nov 2023 16:23
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG113023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 01 03:37:46 2023

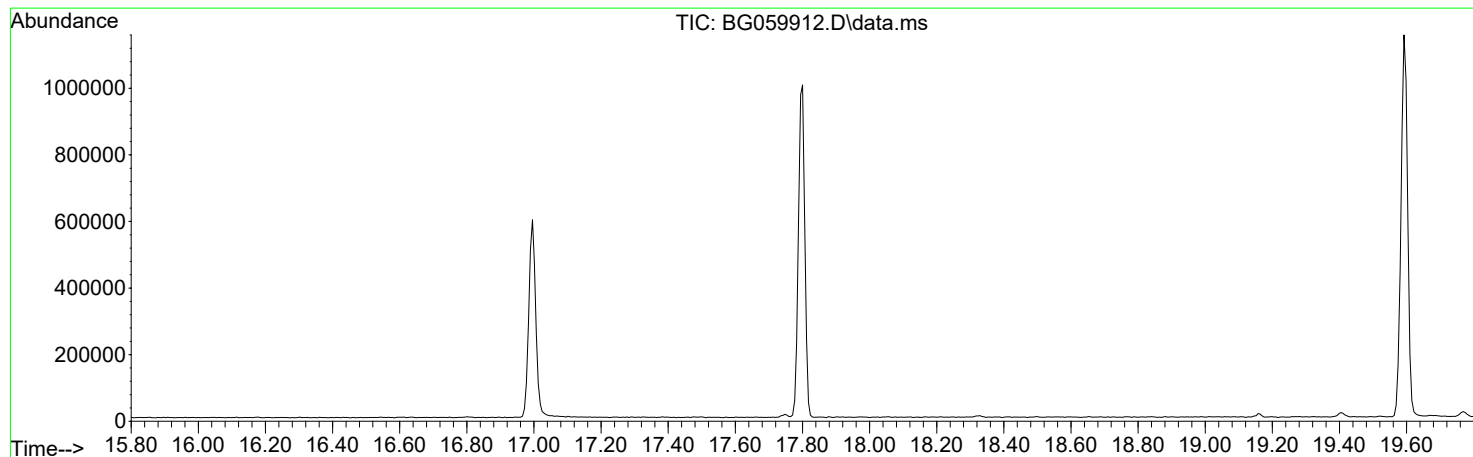




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	39797	PASS
68	69	0.00	2	0.4	129	PASS
69	198	0.00	100	33.8	29441	PASS
70	69	0.00	2	0.6	175	PASS
127	198	10	80	41.3	36016	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87195	PASS
199	198	5	9	6.3	5504	PASS
275	198	10	60	32.0	27901	PASS
365	198	1	100	5.0	4402	PASS
441	198	0.01	100	23.3	20357	PASS
442	442	50	100	100.0	118725	PASS
443	442	15	24	19.2	22837	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113023\
Data File : BG059912.D
Acq On : 30 Nov 2023 16:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 01 03:57:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG113023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 03:37:46 2023
Response via : Initial Calibration

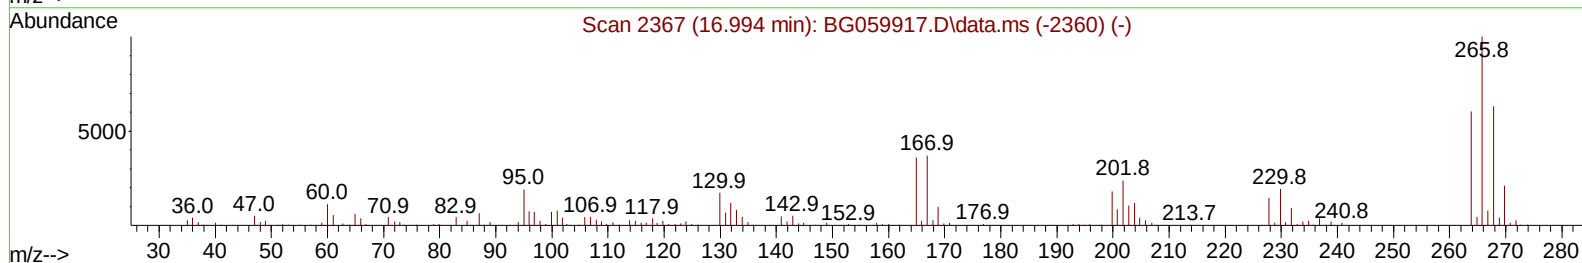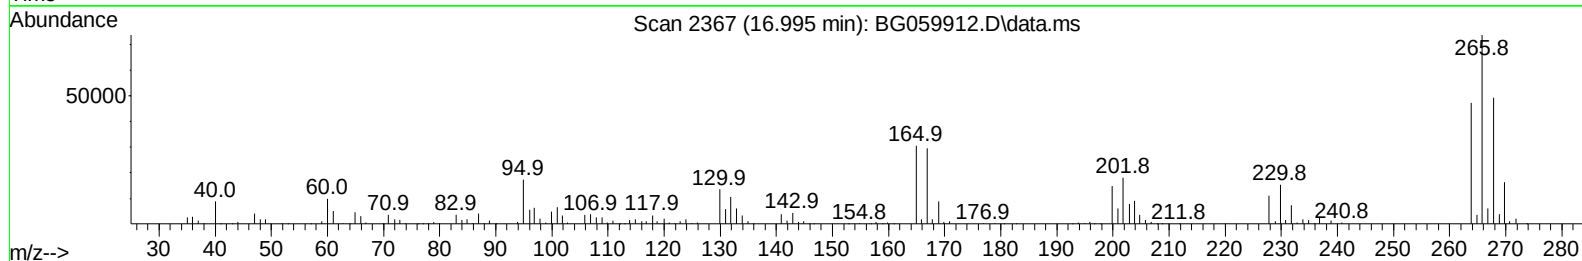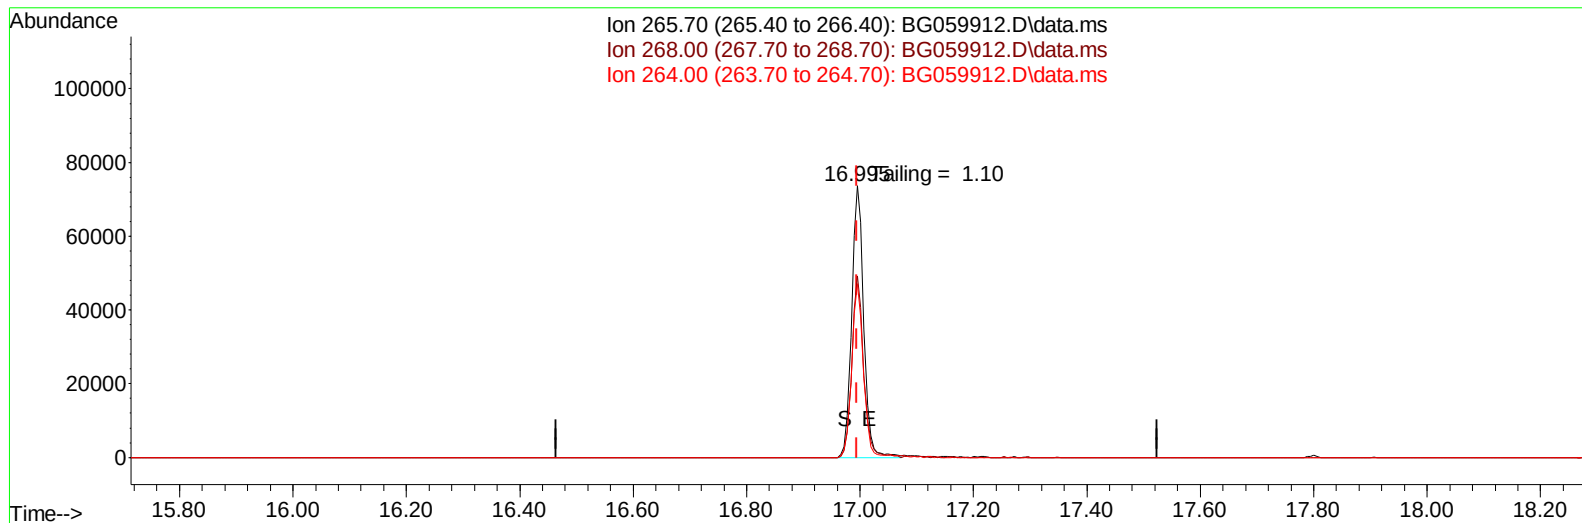

TIC: BG059912.D\data.ms

(70) Pentachlorophenol (C)

16.995min (+ 0.001) 120072.13 ng




response 109048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	66.74
264.00	60.30	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113023\
Data File : BG059912.D
Acq On : 30 Nov 2023 16:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 01 03:57:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG113023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 03:37:46 2023
Response via : Initial Calibration

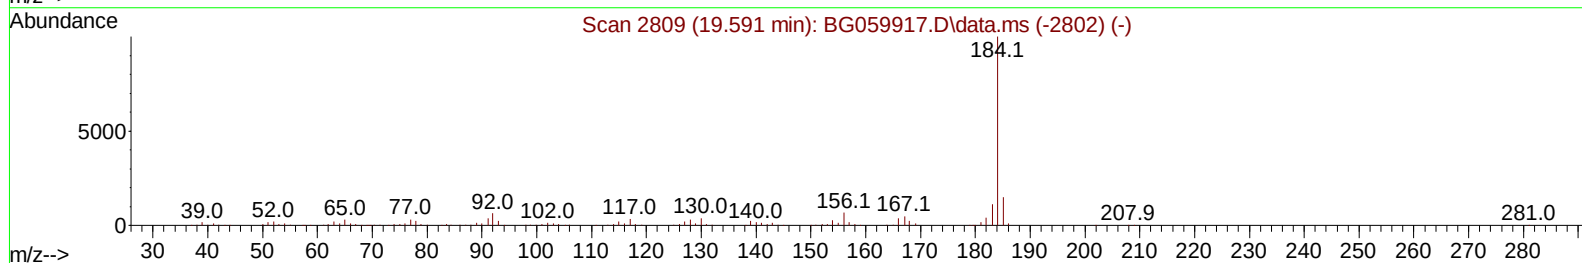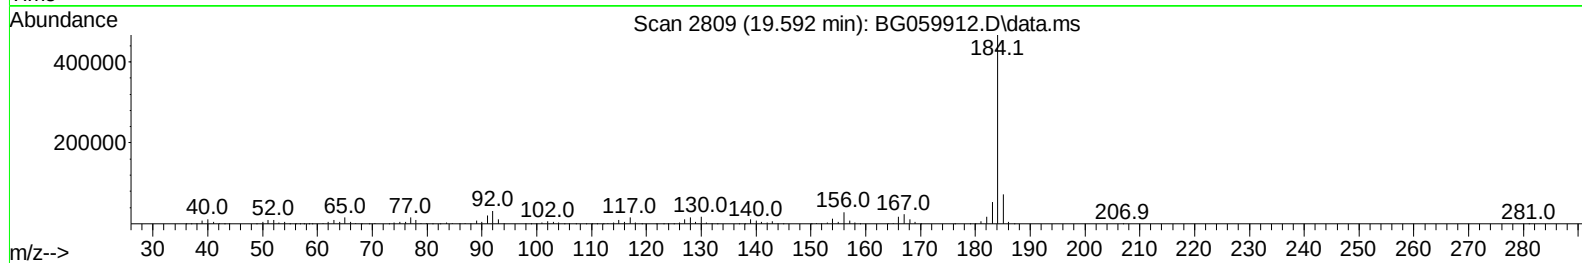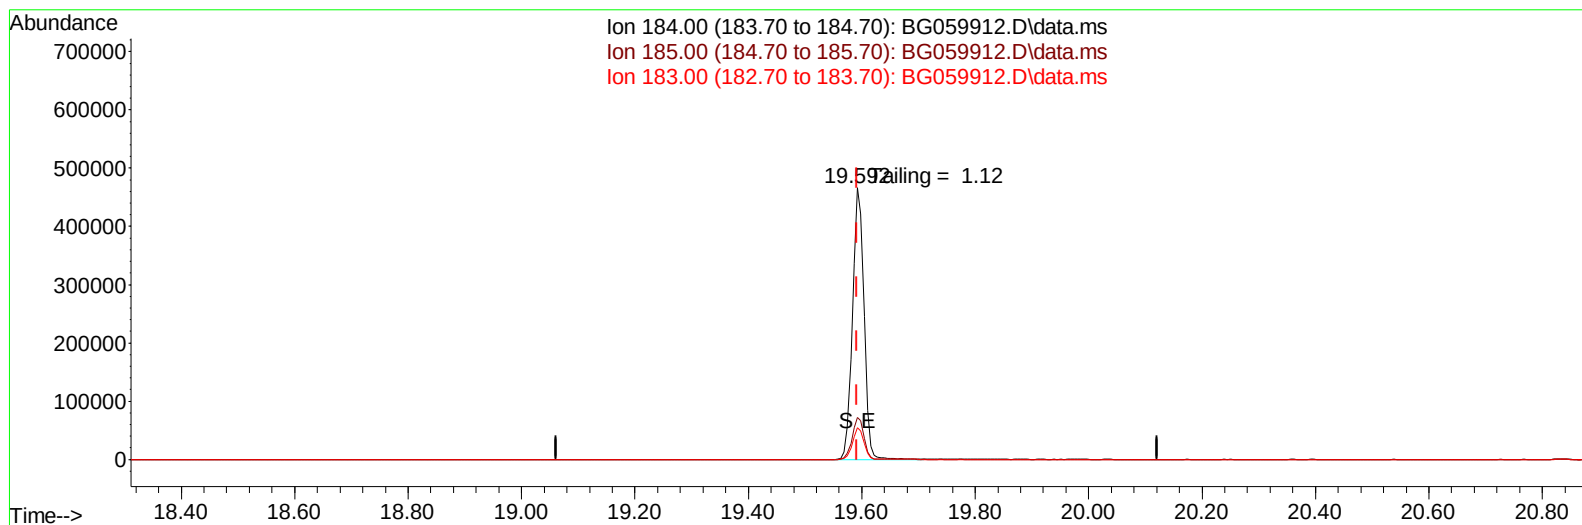

TIC: BG059912.D\data.ms

(77) Benzidine

19.592min (+ 0.001) 14932.09 ng

response 651012

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.51
183.00	11.20	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/30/2023	BNA_G	BG059912.D
Compound Name	Response	Retention Time
DDT	270863	20.832
DDD	10935	20.391
DDE	212	19.968
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11147	282010	3.95

Instrument :
BNA_G
ClientSampleId :
DFTPP